


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP111119\
 Data File : BP001018.D
 Acq On : 11 Nov 2019 15:56
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 06 17:07:13 2019

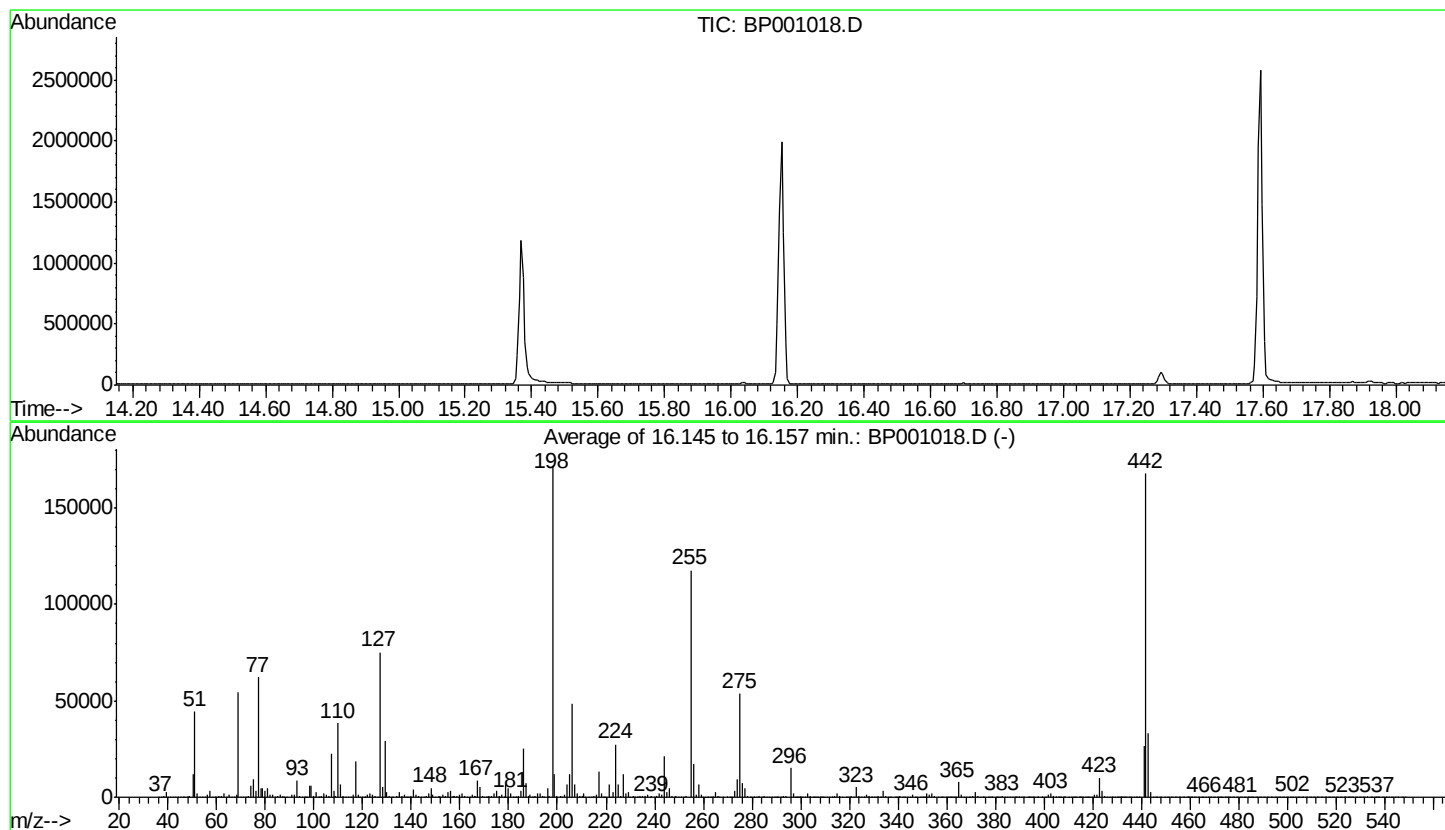

AutoFind: Scans 2390, 2391, 2392; Background Corrected with Scan 2382

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.8	44437	PASS
68	69	0.00	2	2.0	1089	PASS
69	198	0.00	100	31.7	54548	PASS
70	69	0.00	2	0.5	265	PASS
127	198	10	80	43.7	75154	PASS
197	198	0.00	2	0.3	525	PASS
198	198	100	100	100.0	172010	PASS
199	198	5	9	6.8	11749	PASS
275	198	10	60	31.1	53581	PASS
365	198	1	100	4.6	7869	PASS
441	198	0.01	100	15.5	26578	PASS
442	198	50	100	97.6	167824	PASS
443	442	15	24	19.7	33048	PASS