


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111125\
Data File : BP026089.D
Acq On : 11 Nov 2025 14:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 11 15:18:53 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 30 11:51:34 2025
Response via : Initial Calibration

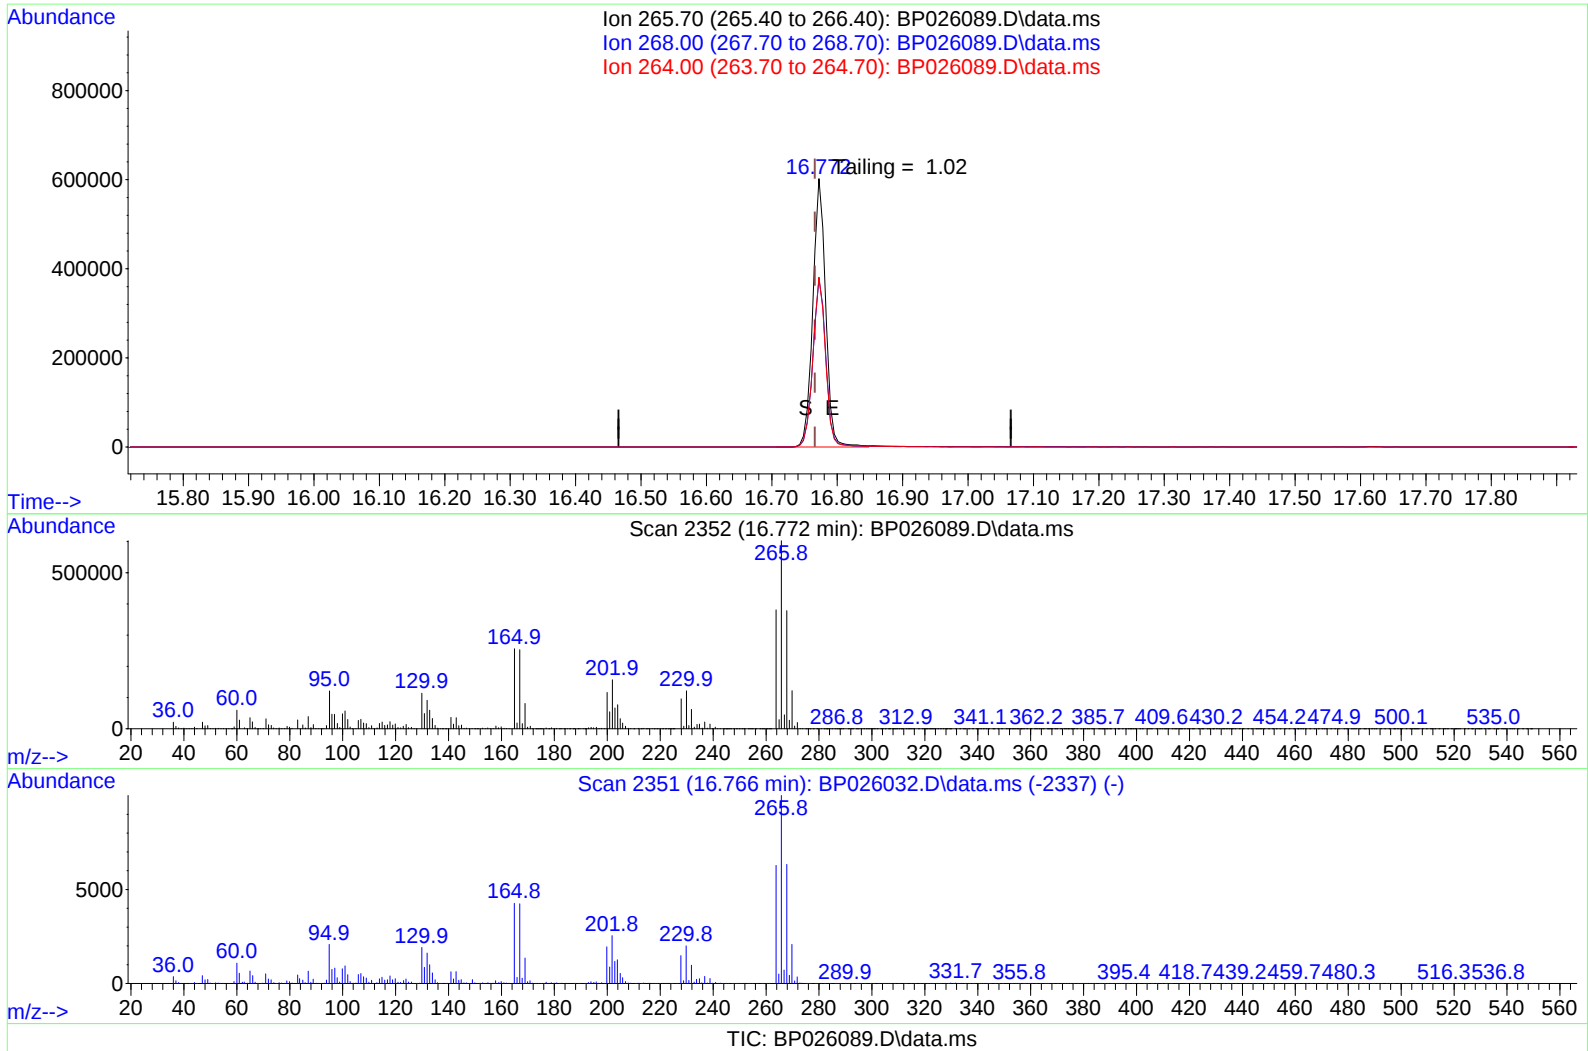

(70) Pentachlorophenol (C)




16.772min (+ 0.006) 1462042.63 ng

response 823223

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	62.80
264.00	62.80	63.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111125\
Data File : BP026089.D
Acq On : 11 Nov 2025 14:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 11 15:18:53 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 30 11:51:34 2025
Response via : Initial Calibration

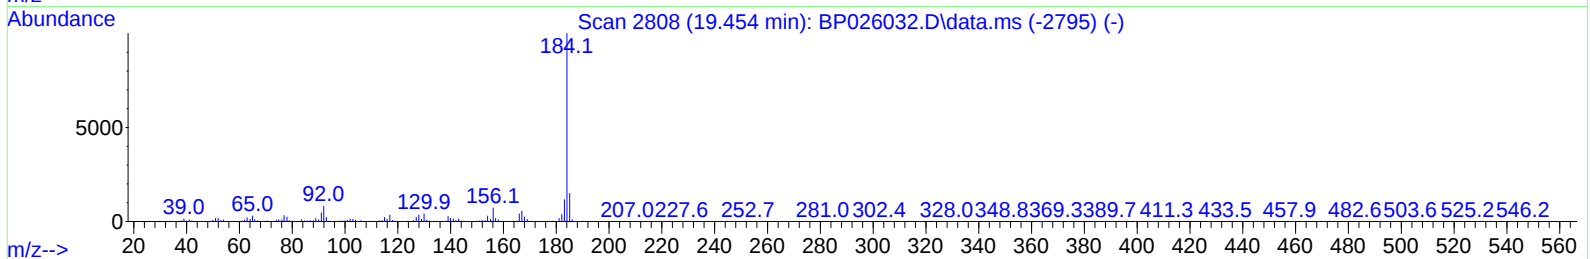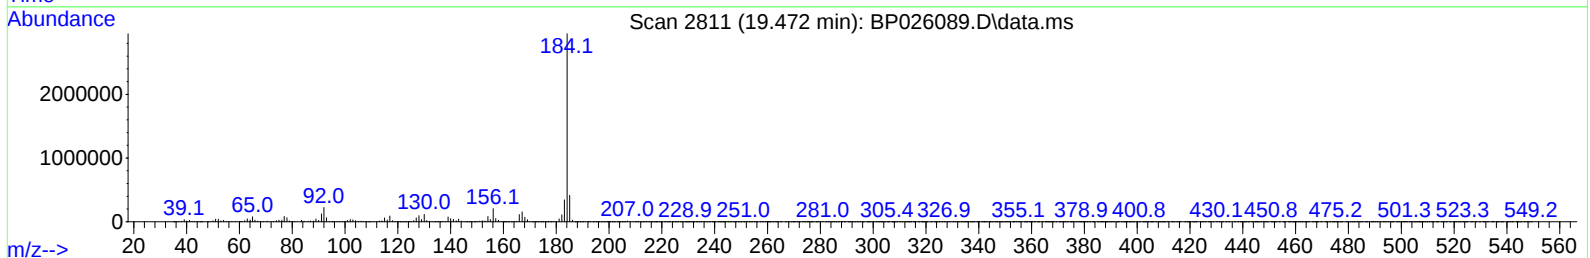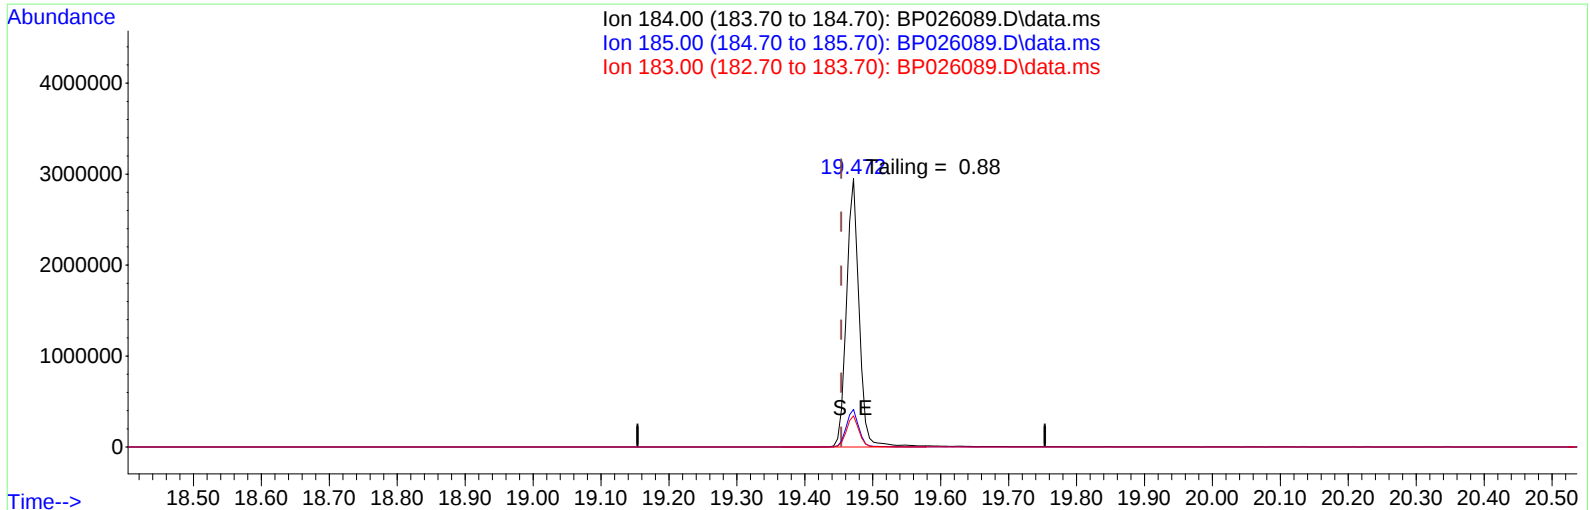

TIC: BP026089.D\data.ms

(77) Benzidine**19.472min (+ 0.018) 657528.85 ng****response 3788584**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.00
183.00	11.50	11.65
0.00	0.00	0.00