

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111125\
 Data File : BP026091.D
 Acq On : 11 Nov 2025 15:25
 Operator : RC/JU
 Sample : PB170478BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB170478BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP026091.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.290	394	400	411	rBV	5267639	7723861	36.26%	9.035%
2	6.849	657	665	677	rBV	4847966	7688332	36.09%	8.994%
3	7.672	797	805	815	rBV	1042999	1676164	7.87%	1.961%
4	8.813	991	999	1018	rBV	2967217	4912776	23.06%	5.747%
5	10.449	1268	1277	1291	rBV	1288147	2303110	10.81%	2.694%
6	12.931	1691	1699	1714	rBV	8311404	11823647	55.50%	13.831%
7	14.325	1928	1936	1943	rBV	2400649	3144849	14.76%	3.679%
8	15.837	2185	2193	2213	rBV	6760308	9976193	46.83%	11.670%
9	17.131	2404	2413	2425	rBV2	2457002	4245535	19.93%	4.966%
10	19.878	2874	2880	2885	rBV	17641367	21303574	100.00%	24.920%
11	21.583	3164	3170	3184	rBV	3579773	5186173	24.34%	6.067%
12	24.924	3729	3738	3750	rVB	2128527	5503313	25.83%	6.438%




Sum of corrected areas: 85487527

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111125\
Data File : BP026091.D
Acq On : 11 Nov 2025 15:25
Operator : RC/JU
Sample : PB170478BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB170478BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

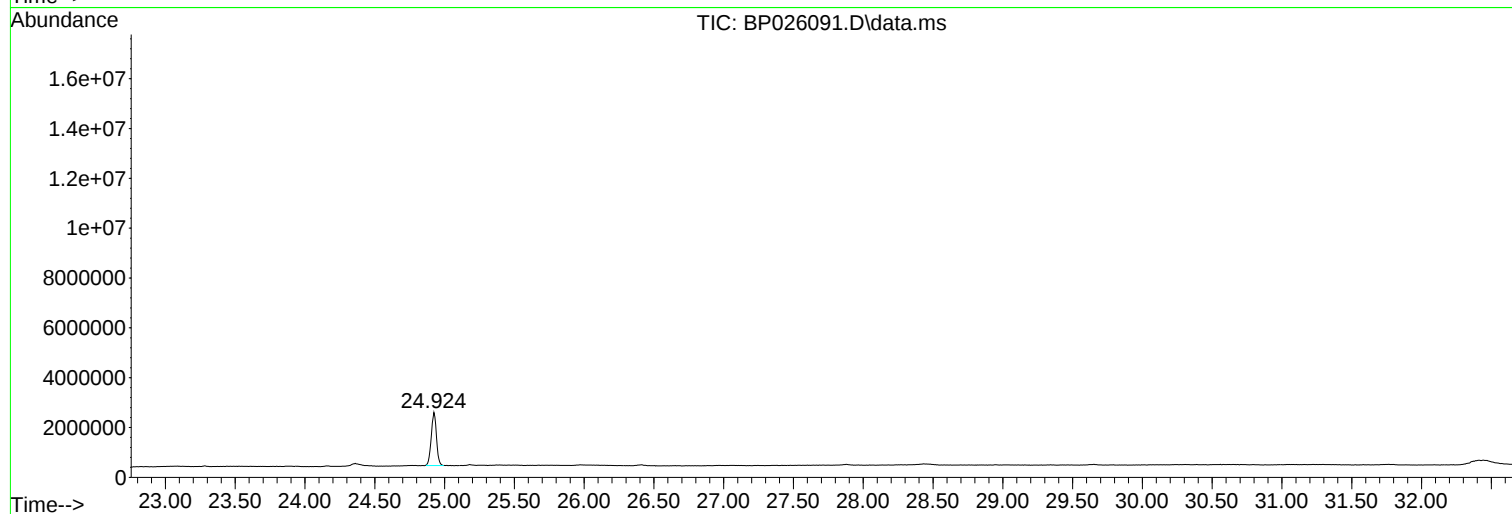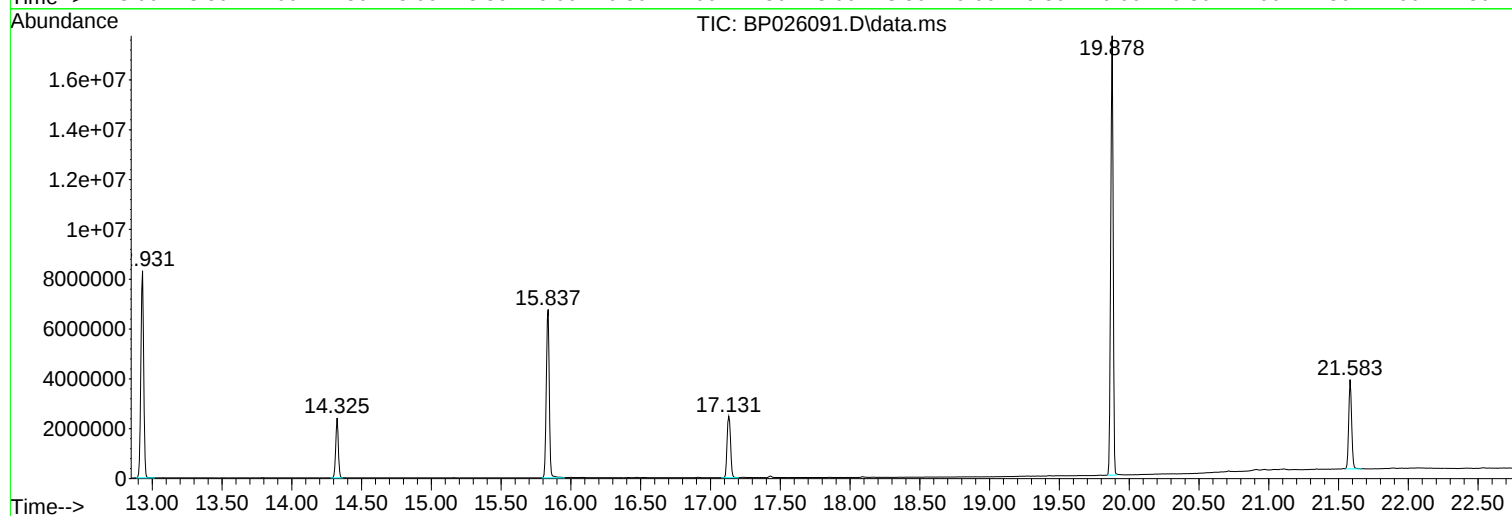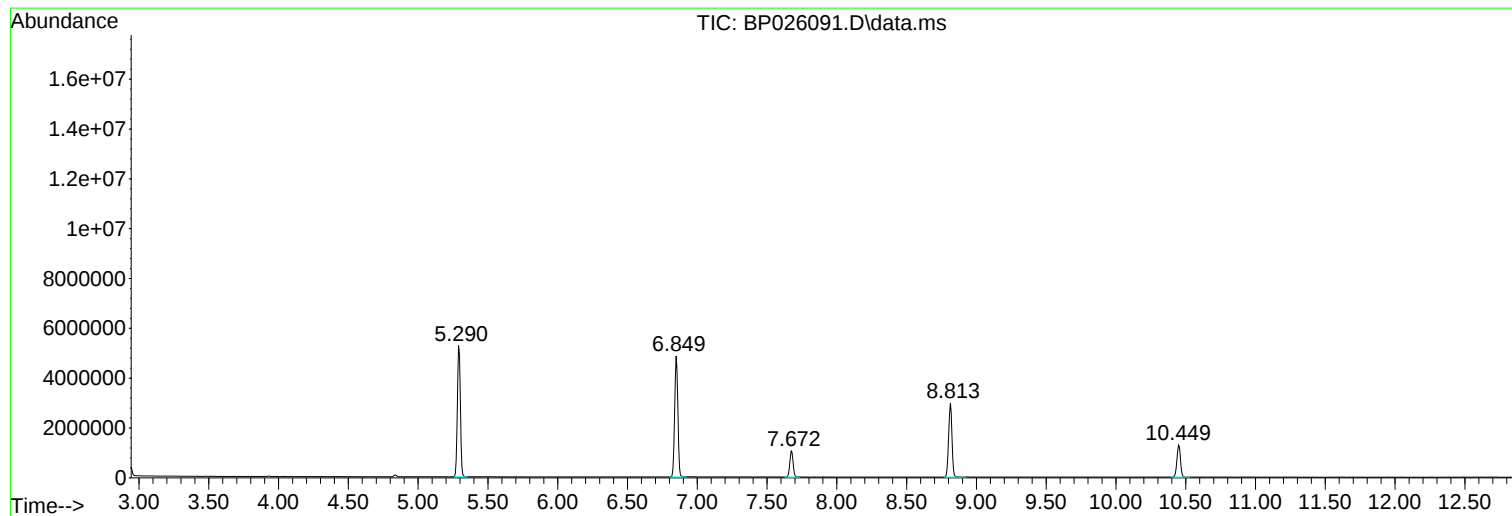

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111125\
Data File : BP026091.D
Acq On : 11 Nov 2025 15:25
Operator : RC/JU
Sample : PB170478BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB170478BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111125\
Data File : BP026091.D
Acq On : 11 Nov 2025 15:25
Operator : RC/JU
Sample : PB170478BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB170478BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------