

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111220\
 Data File : BP003941.D
 Acq On : 12 Nov 2020 16:33
 Operator : CG/JU
 Sample : L4719-07
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 TP-3-D

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP003941.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.928	3	7	18	rVB	1179851	1278026	25.95%	3.938%
2	3.087	28	34	44	rBV	109306	216691	4.40%	0.668%
3	3.175	44	49	62	rVB	355861	420849	8.54%	1.297%
4	5.805	488	496	510	rBV	2055047	3021758	61.35%	9.312%
5	7.452	768	776	789	rBV	1942680	3088694	62.71%	9.518%
6	7.852	838	844	852	rVB	48121	75026	1.52%	0.231%
7	8.281	909	917	925	rBV	567086	895294	18.18%	2.759%
8	9.446	1106	1115	1122	rBV	1189593	2008560	40.78%	6.190%
9	11.110	1389	1398	1405	rBV	684776	1149473	23.34%	3.542%
10	13.528	1801	1809	1820	rBV	2552680	3857710	78.32%	11.888%
11	14.328	1939	1945	1956	rBV	363656	549285	11.15%	1.693%
12	14.628	1990	1996	2001	rBV	95264	161321	3.28%	0.497%
13	14.687	2001	2006	2020	rVB2	33836	92806	1.88%	0.286%
14	14.904	2037	2043	2052	rBV	922435	1340494	27.21%	4.131%
15	16.387	2286	2295	2311	rBV	1807929	2713467	55.09%	8.362%
16	17.639	2501	2508	2512	rBV	1053337	1526105	30.98%	4.703%
17	17.675	2512	2514	2518	rVB	50882	67401	1.37%	0.208%
18	17.769	2525	2530	2534	rVB	71963	100797	2.05%	0.311%
19	18.481	2647	2651	2656	rBV2	37506	66515	1.35%	0.205%
20	18.533	2656	2660	2665	rVB2	42228	58388	1.19%	0.180%
21	18.604	2669	2672	2678	rVB	41057	54836	1.11%	0.169%
22	18.681	2678	2685	2688	rBV4	52136	116427	2.36%	0.359%
23	19.228	2774	2778	2783	rBV2	67370	94044	1.91%	0.290%
24	19.357	2796	2800	2805	rBV3	43633	70335	1.43%	0.217%
25	19.610	2839	2843	2848	rBV	101054	131179	2.66%	0.404%
26	19.963	2898	2903	2910	rVB	166261	246533	5.01%	0.760%
27	20.133	2927	2932	2938	rBV	4253035	4925626	100.00%	15.179%
28	20.727	3030	3033	3036	rBV	45801	58791	1.19%	0.181%
29	20.998	3076	3079	3084	rBV	100431	127930	2.60%	0.394%
30	21.322	3130	3134	3143	rVB2	445201	563803	11.45%	1.737%
31	21.669	3187	3193	3198	rBV	1299281	1817211	36.89%	5.600%
32	24.151	3609	3615	3623	rBV2	793587	1555143	31.57%	4.792%




Sum of corrected areas: 32450518

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111220\
Data File : BP003941.D
Acq On : 12 Nov 2020 16:33
Operator : CG/JU
Sample : L4719-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TP-3-D

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

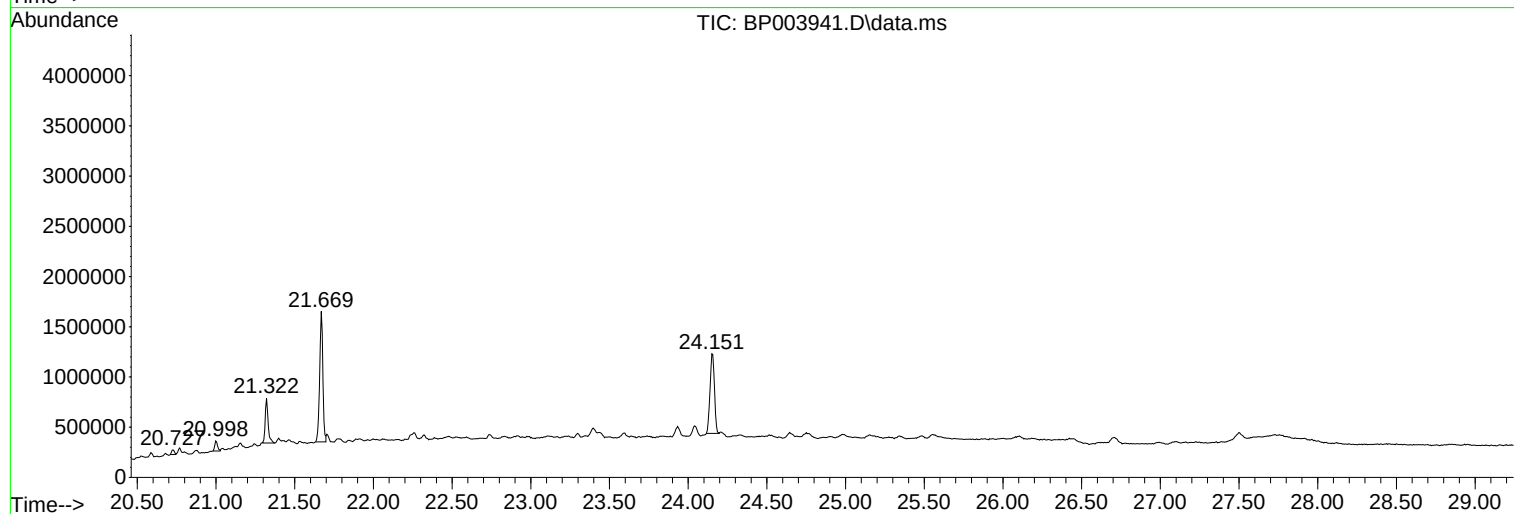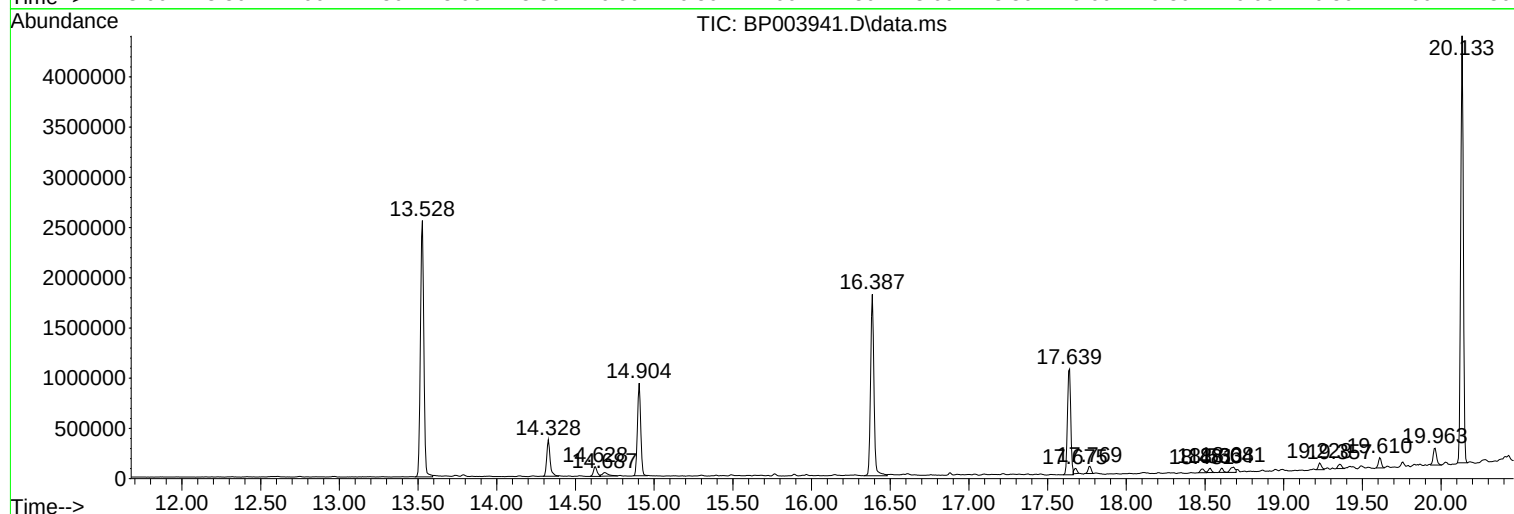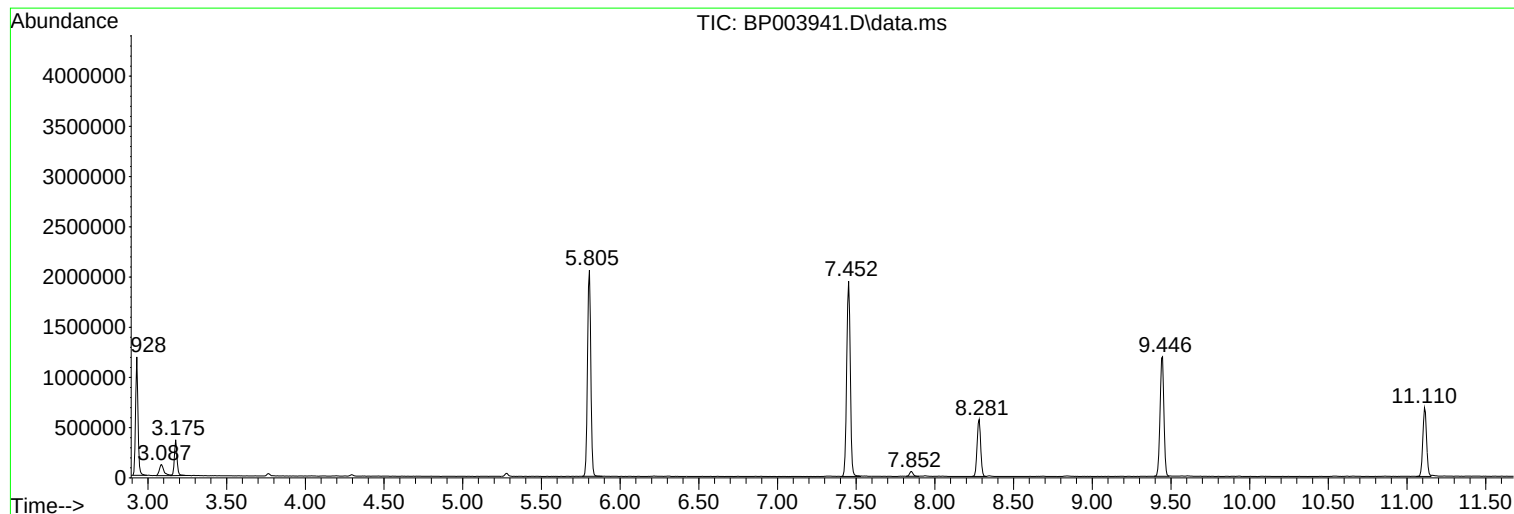

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111220\
Data File : BP003941.D
Acq On : 12 Nov 2020 16:33
Operator : CG/JU
Sample : L4719-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TP-3-D

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111220\
Data File : BP003941.D
Acq On : 12 Nov 2020 16:33
Operator : CG/JU
Sample : L4719-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TP-3-D

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
