

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111220\
 Data File : BP003942.D
 Acq On : 12 Nov 2020 17:07
 Operator : CG/JU
 Sample : L4714-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EROC-SP-2

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP003942.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.928	3	7	25	rVB	5714664	6689537	100.00%	18.453%
2	3.081	27	33	44	rVV	120296	223498	3.34%	0.617%
3	3.175	44	49	60	rVB	411485	491998	7.35%	1.357%
4	5.805	488	496	507	rBV	2070357	3062649	45.78%	8.448%
5	7.452	767	776	788	rBV	1914872	3034407	45.36%	8.370%
6	7.852	839	844	851	rVB	48614	76484	1.14%	0.211%
7	8.281	909	917	924	rBV	522942	837525	12.52%	2.310%
8	9.446	1106	1115	1124	rBV	1214597	2052855	30.69%	5.663%
9	11.110	1389	1398	1405	rBV	636513	1090893	16.31%	3.009%
10	13.528	1801	1809	1830	rBV	2262820	3390660	50.69%	9.353%
11	14.328	1939	1945	1957	rBV	311142	441949	6.61%	1.219%
12	14.904	2036	2043	2052	rBV	883589	1292447	19.32%	3.565%
13	16.387	2286	2295	2314	rBV	1985383	2940580	43.96%	8.112%
14	17.639	2501	2508	2513	rBV	1122613	1668137	24.94%	4.602%
15	19.228	2774	2778	2783	rBV	59724	70945	1.06%	0.196%
16	19.610	2840	2843	2848	rVB	68629	81477	1.22%	0.225%
17	19.963	2899	2903	2908	rVB	82844	110698	1.65%	0.305%
18	20.133	2927	2932	2938	rBV	3621787	4312095	64.46%	11.895%
19	21.322	3130	3134	3143	rBV	486533	599220	8.96%	1.653%
20	21.669	3188	3193	3198	rBV	1317230	1736594	25.96%	4.790%
21	22.739	3371	3375	3383	rVB	144291	213122	3.19%	0.588%
22	22.892	3398	3401	3406	rVB	110445	151798	2.27%	0.419%
23	24.151	3609	3615	3624	rVB2	824323	1682405	25.15%	4.641%




Sum of corrected areas: 36251973

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111220\
Data File : BP003942.D
Acq On : 12 Nov 2020 17:07
Operator : CG/JU
Sample : L4714-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EROC-SP-2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

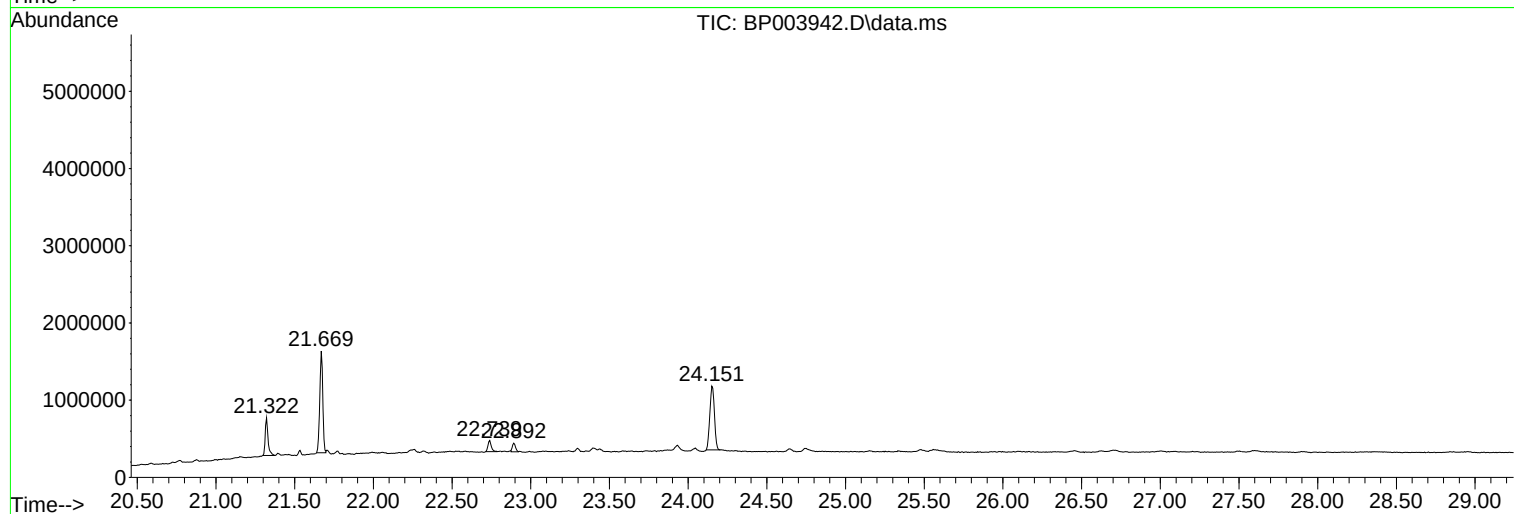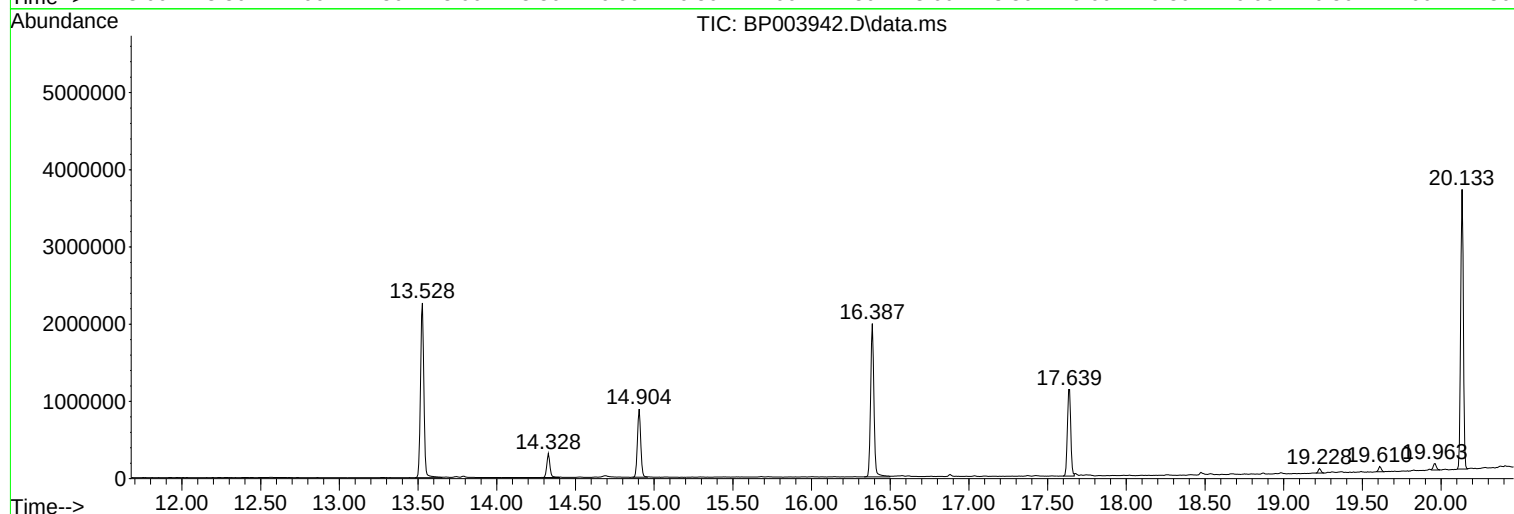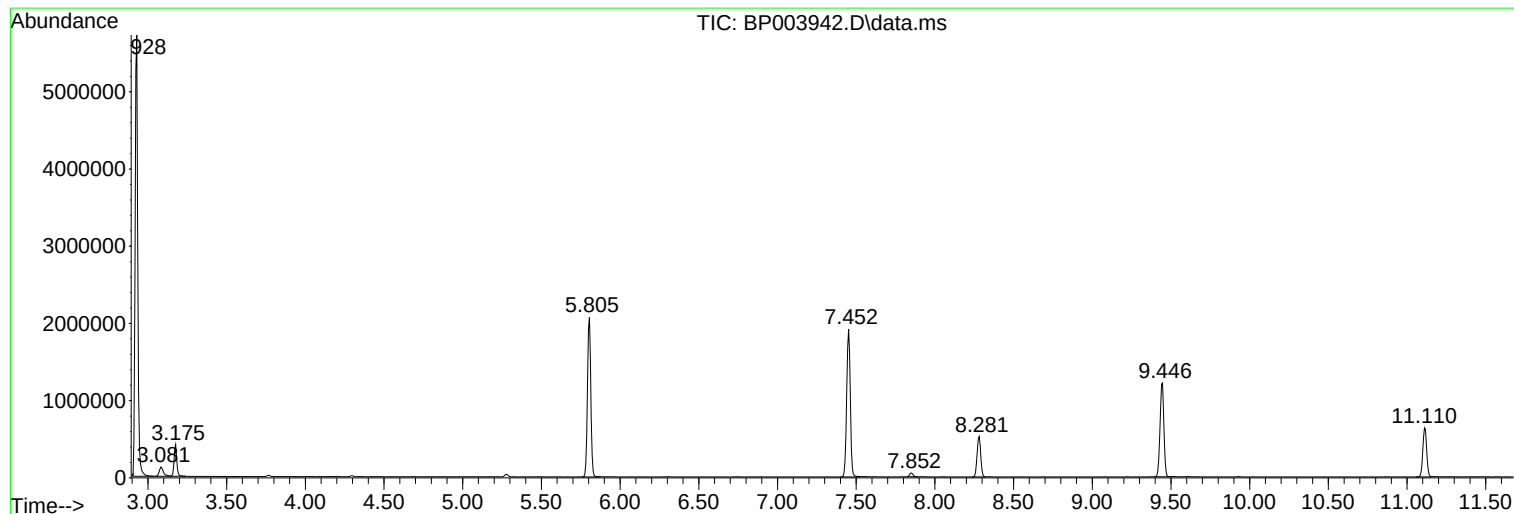

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111220\
Data File : BP003942.D
Acq On : 12 Nov 2020 17:07
Operator : CG/JU
Sample : L4714-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EROC-SP-2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111220\
Data File : BP003942.D
Acq On : 12 Nov 2020 17:07
Operator : CG/JU
Sample : L4714-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EROC-SP-2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
