

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111220\
 Data File : BP003943.D
 Acq On : 12 Nov 2020 17:41
 Operator : CG/JU
 Sample : L4685-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 72-11978

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP003943.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.928	3	7	20	rVB	5219026	5730587	100.00%	14.901%
2	3.081	27	33	37	rBV	121503	213180	3.72%	0.554%
3	3.122	37	40	45	rVV	133276	165882	2.89%	0.431%
4	3.175	45	49	57	rVB	372447	428298	7.47%	1.114%
5	5.804	489	496	510	rVB	2034685	3011507	52.55%	7.831%
6	5.951	515	521	534	rBV	88735	149555	2.61%	0.389%
7	7.457	768	777	789	rBV	1848675	3081140	53.77%	8.012%
8	7.851	838	844	851	rBV	74323	111862	1.95%	0.291%
9	8.281	909	917	924	rBV	553827	869860	15.18%	2.262%
10	9.445	1104	1115	1126	rBV	1185217	1996730	34.84%	5.192%
11	10.963	1366	1373	1378	rBV	161507	233171	4.07%	0.606%
12	11.110	1390	1398	1414	rBV	651926	1148067	20.03%	2.985%
13	13.527	1801	1809	1825	rBV	2445722	3756086	65.54%	9.767%
14	14.327	1939	1945	1952	rBV	438059	621666	10.85%	1.617%
15	14.904	2036	2043	2051	rBV	915515	1353866	23.63%	3.521%
16	16.386	2288	2295	2311	rBV	1829306	2760043	48.16%	7.177%
17	17.639	2502	2508	2512	rBV	1041770	1543196	26.93%	4.013%
18	17.674	2512	2514	2522	rVB	223037	292416	5.10%	0.760%
19	18.474	2646	2650	2656	rBV2	116088	194625	3.40%	0.506%
20	18.533	2657	2660	2665	rVB2	45687	67215	1.17%	0.175%
21	18.674	2680	2684	2688	rBV4	41587	65098	1.14%	0.169%
22	18.992	2734	2738	2747	rVB3	57837	90940	1.59%	0.236%
23	19.492	2819	2823	2827	rBV	104532	128888	2.25%	0.335%
24	19.609	2839	2843	2848	rBV	525877	678778	11.84%	1.765%
25	19.657	2848	2851	2854	rVV2	59290	65096	1.14%	0.169%
26	19.927	2894	2897	2899	rBV2	69289	95392	1.66%	0.248%
27	19.962	2899	2903	2910	rVB	435061	588666	10.27%	1.531%
28	20.133	2927	2932	2938	rBV	3851979	4545424	79.32%	11.820%
29	21.321	3130	3134	3143	rVB3	487656	634005	11.06%	1.649%
30	21.533	3167	3170	3176	rVB	162088	182492	3.18%	0.475%
31	21.668	3187	3193	3197	rBV2	1231739	1902829	33.20%	4.948%
32	21.709	3197	3200	3205	rVB	206212	263291	4.59%	0.685%
33	24.156	3610	3616	3622	rVB2	744074	1486770	25.94%	3.866%




Sum of corrected areas: 38456621

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111220\
Data File : BP003943.D
Acq On : 12 Nov 2020 17:41
Operator : CG/JU
Sample : L4685-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
72-11978

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

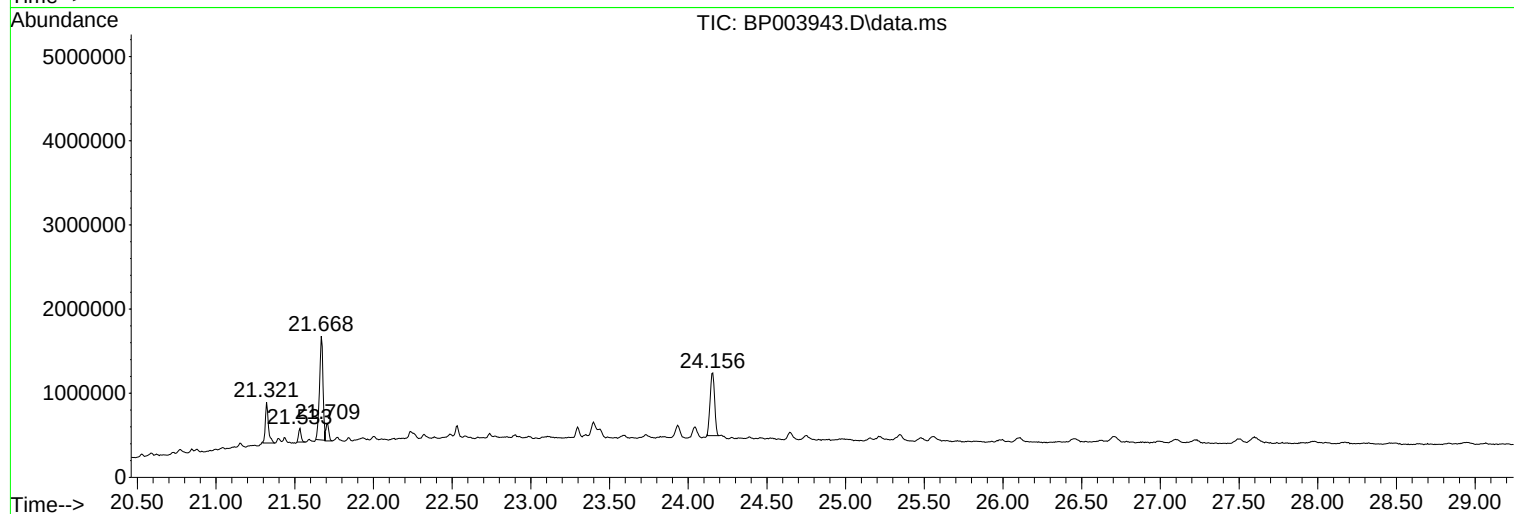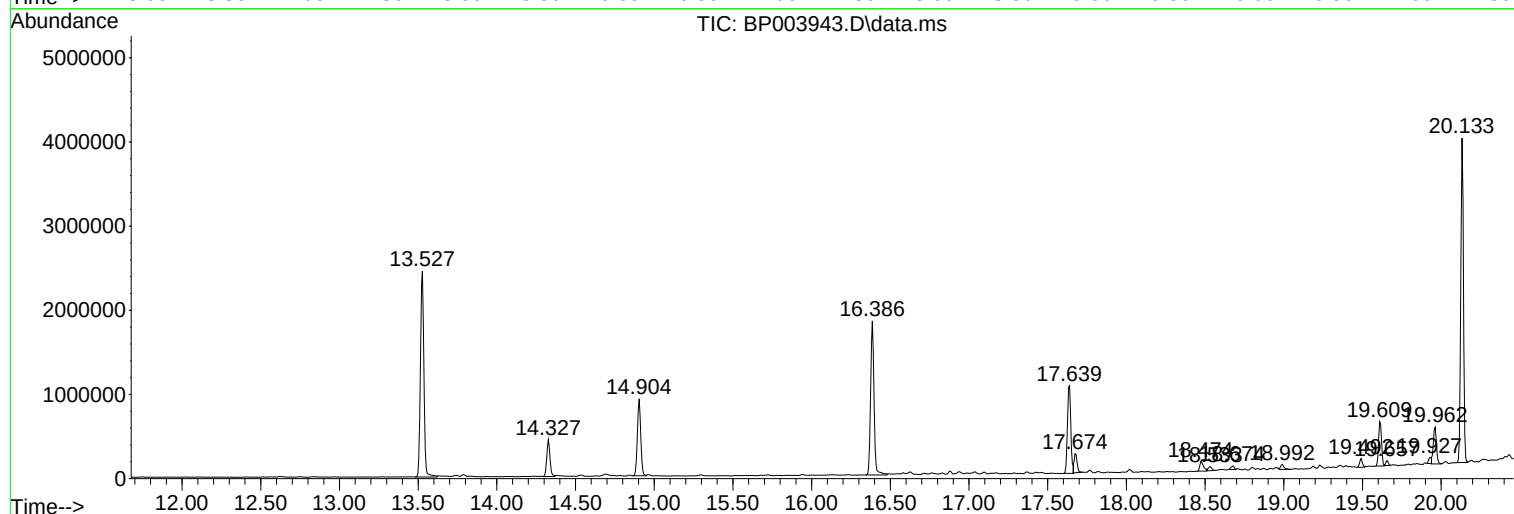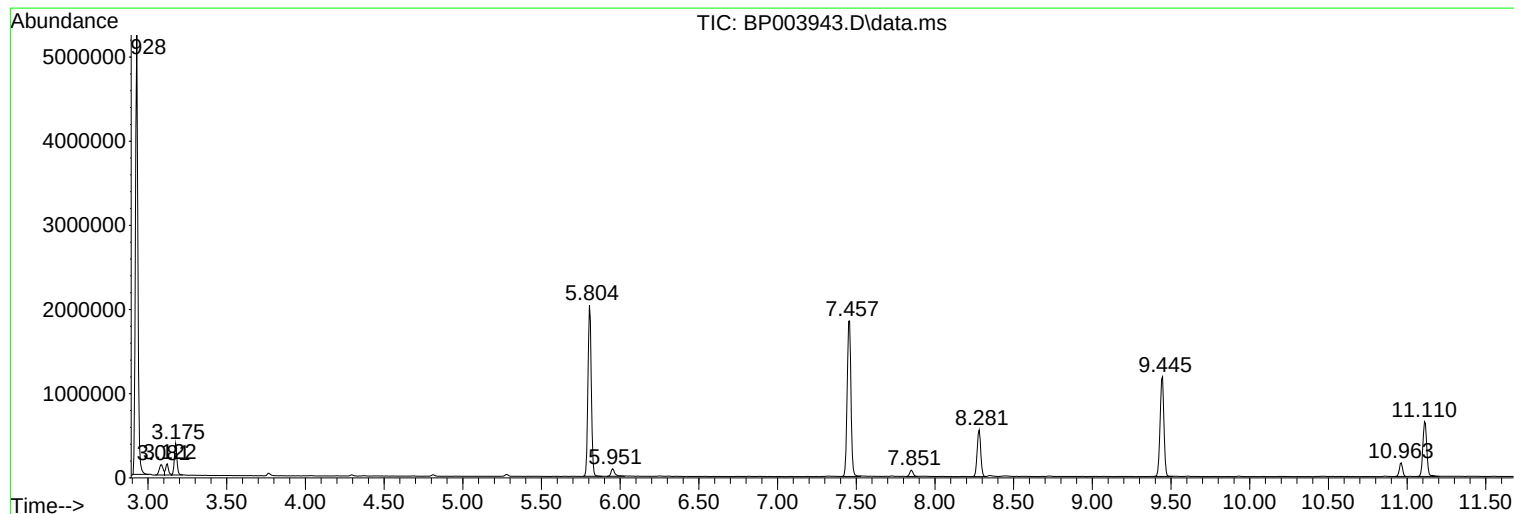

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111220\
Data File : BP003943.D
Acq On : 12 Nov 2020 17:41
Operator : CG/JU
Sample : L4685-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
72-11978

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111220\
Data File : BP003943.D
Acq On : 12 Nov 2020 17:41
Operator : CG/JU
Sample : L4685-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
72-11978

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------