


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111220\
 Data File : BP003937.D
 Acq On : 12 Nov 2020 13:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 12 15:22:47 2020

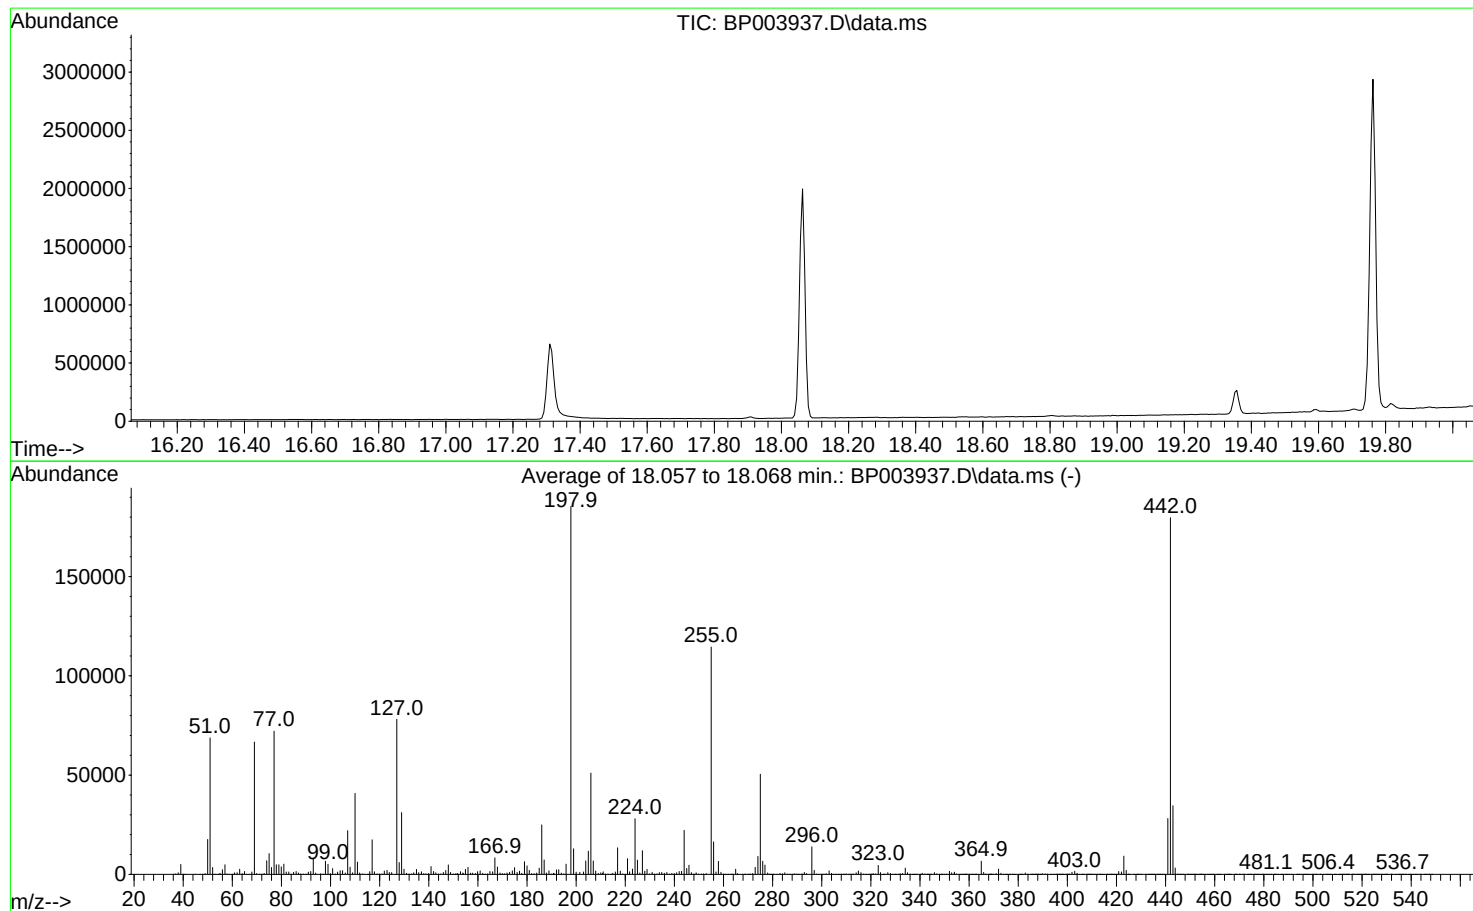

AutoFind: Scans 2579, 2580, 2581; Background Corrected with Scan 2570

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.1	68746	PASS
68	69	0.00	2	1.9	1235	PASS
69	198	0.00	100	36.0	66665	PASS
70	69	0.00	2	0.6	382	PASS
127	198	10	80	42.1	78077	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	185312	PASS
199	198	5	9	7.0	12926	PASS
275	198	10	60	27.2	50432	PASS
365	198	1	100	3.6	6602	PASS
441	198	0.01	100	15.2	28146	PASS
442	198	50	100	96.9	179642	PASS
443	442	15	24	19.2	34547	PASS