
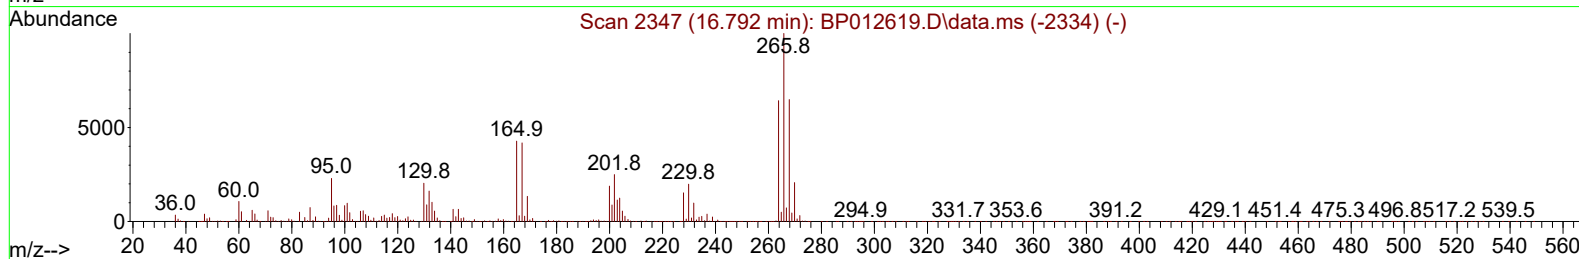
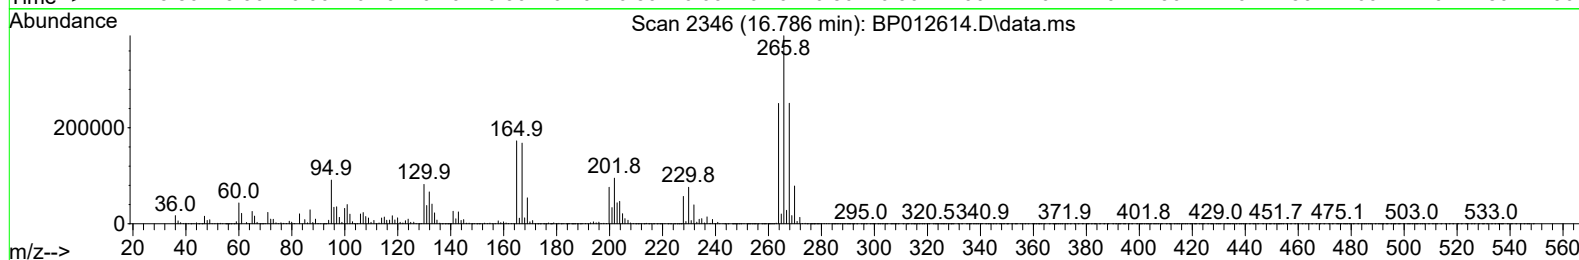


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111222\
 Data File : BP012614.D
 Acq On : 12 Nov 2022 09:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 14 07:57:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 14 04:00:17 2022
 Response via : Initial Calibration

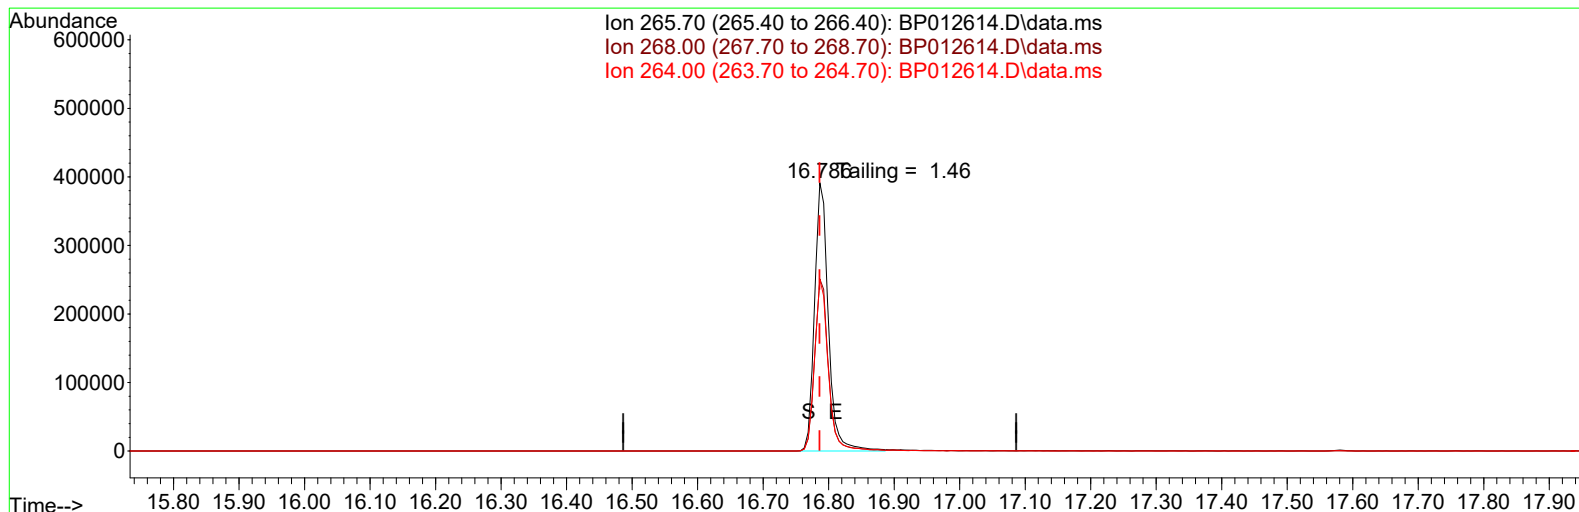

TIC: BP012614.D\data.ms

(70) Pentachlorophenol (C)




16.786min (0.000) 2255058.54 ng

response 578620

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.80	64.08
264.00	64.30	64.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111222\
 Data File : BP012614.D
 Acq On : 12 Nov 2022 09:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 14 07:57:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 14 04:00:17 2022
 Response via : Initial Calibration

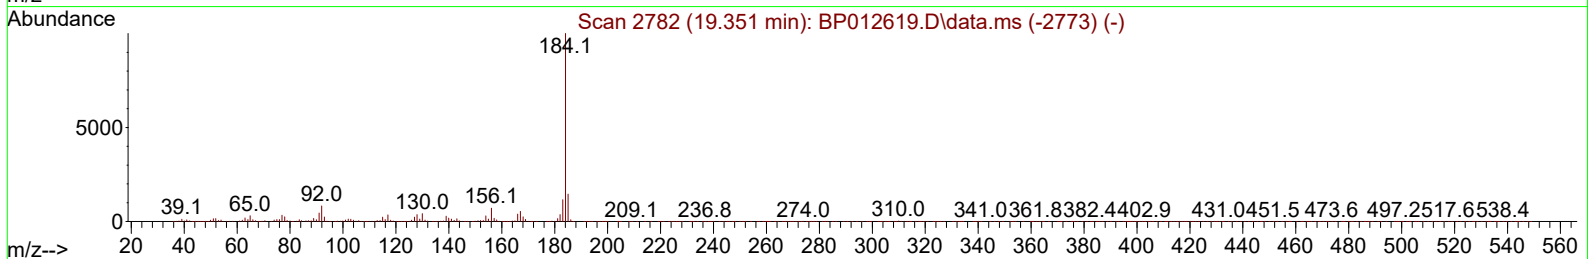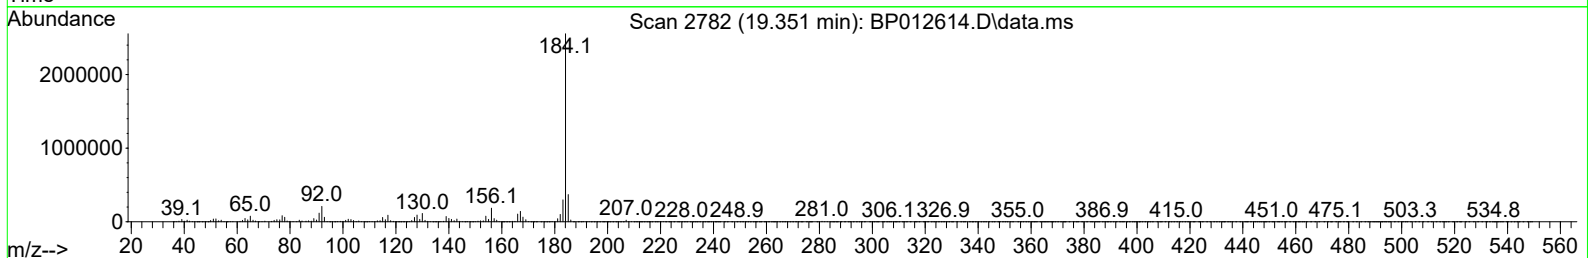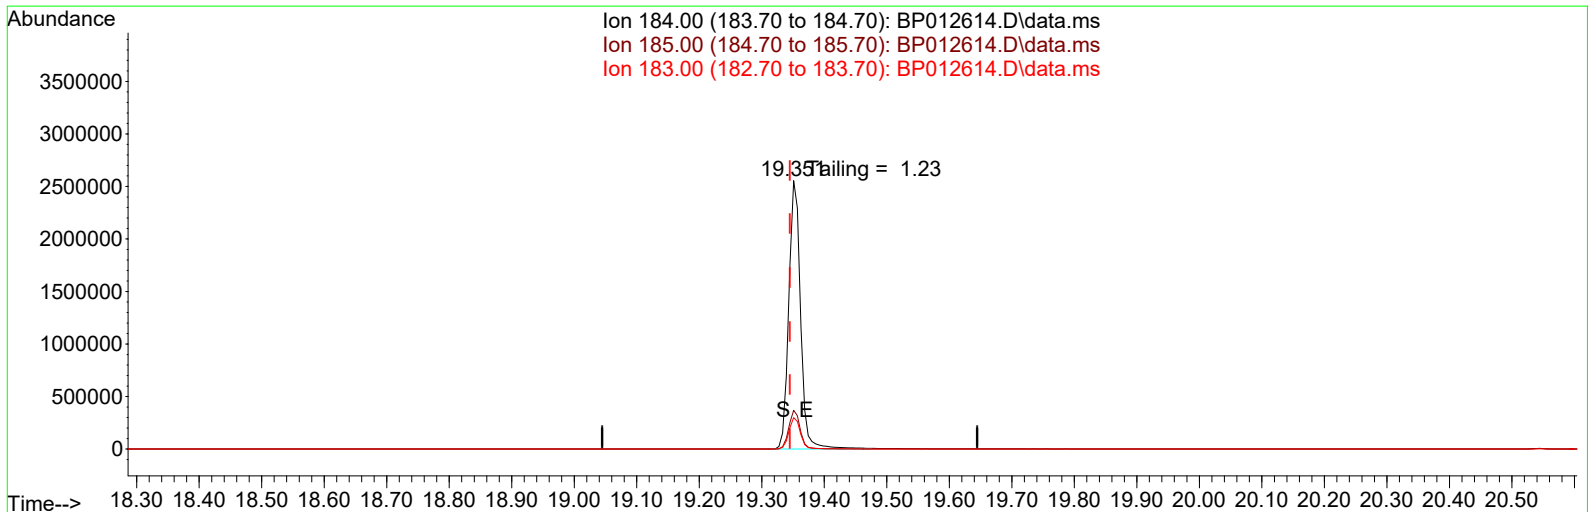

TIC: BP012614.D\data.ms

(77) Benzidine

19.351min (+ 0.006) 814357.46 ng

response 3377700

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.44
183.00	11.60	11.70
0.00	0.00	0.00