
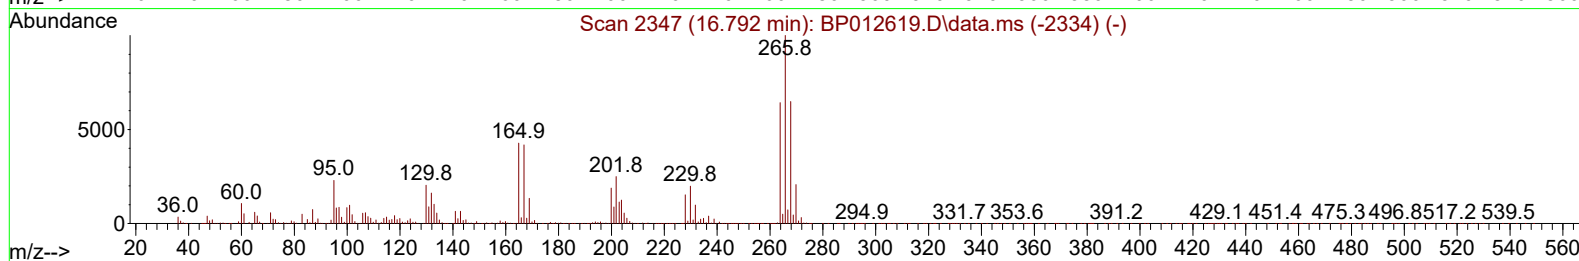
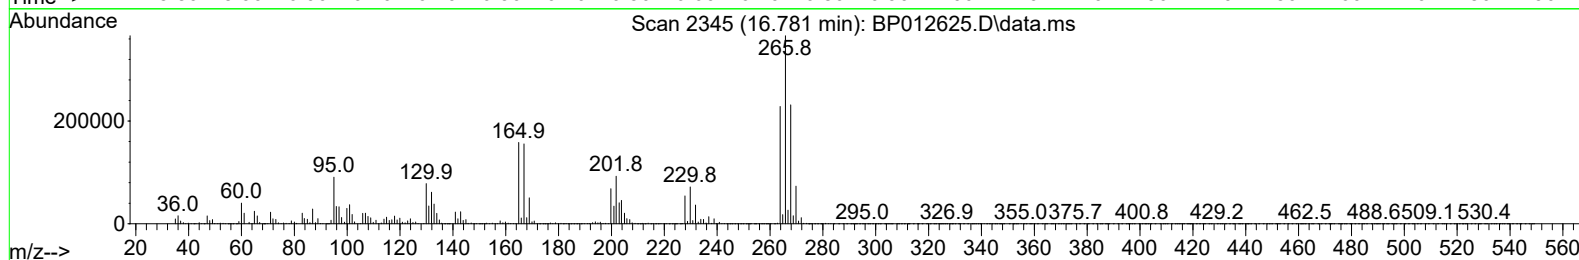


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111222\
 Data File : BP012625.D
 Acq On : 12 Nov 2022 18:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 14 08:01:10 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 14 04:00:17 2022
 Response via : Initial Calibration

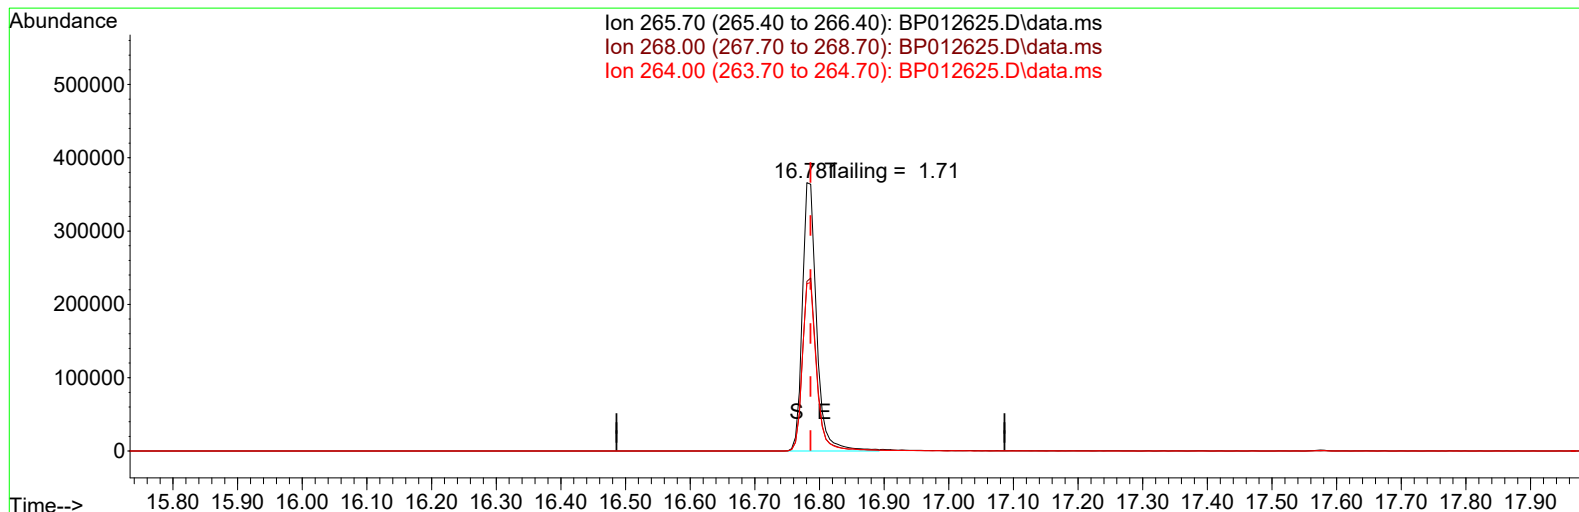

TIC: BP012625.D\data.ms

(70) Pentachlorophenol (C)




16.781min (-0.006) 254201.87 ng

response 563881

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.80	63.22
264.00	64.30	62.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111222\
Data File : BP012625.D
Acq On : 12 Nov 2022 18:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 14 08:01:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 14 04:00:17 2022
Response via : Initial Calibration

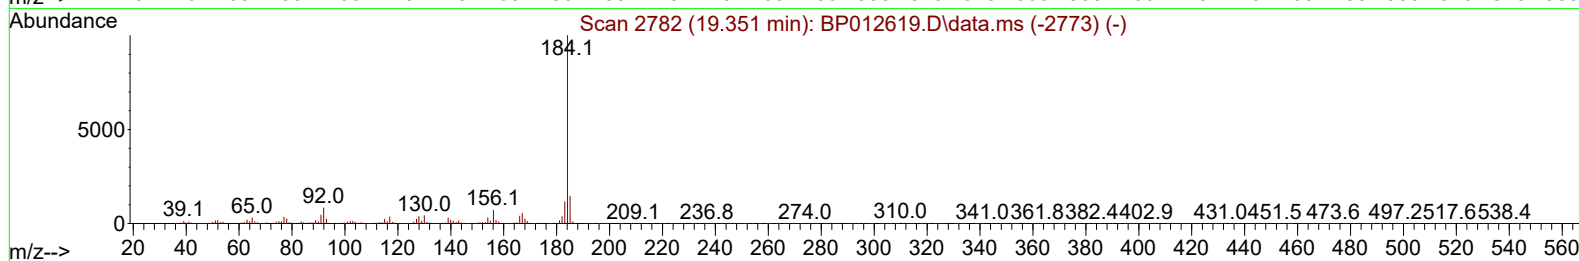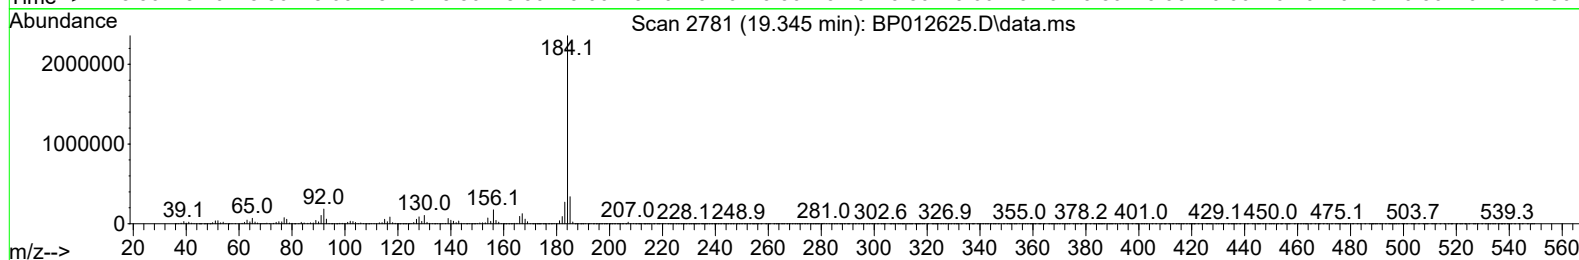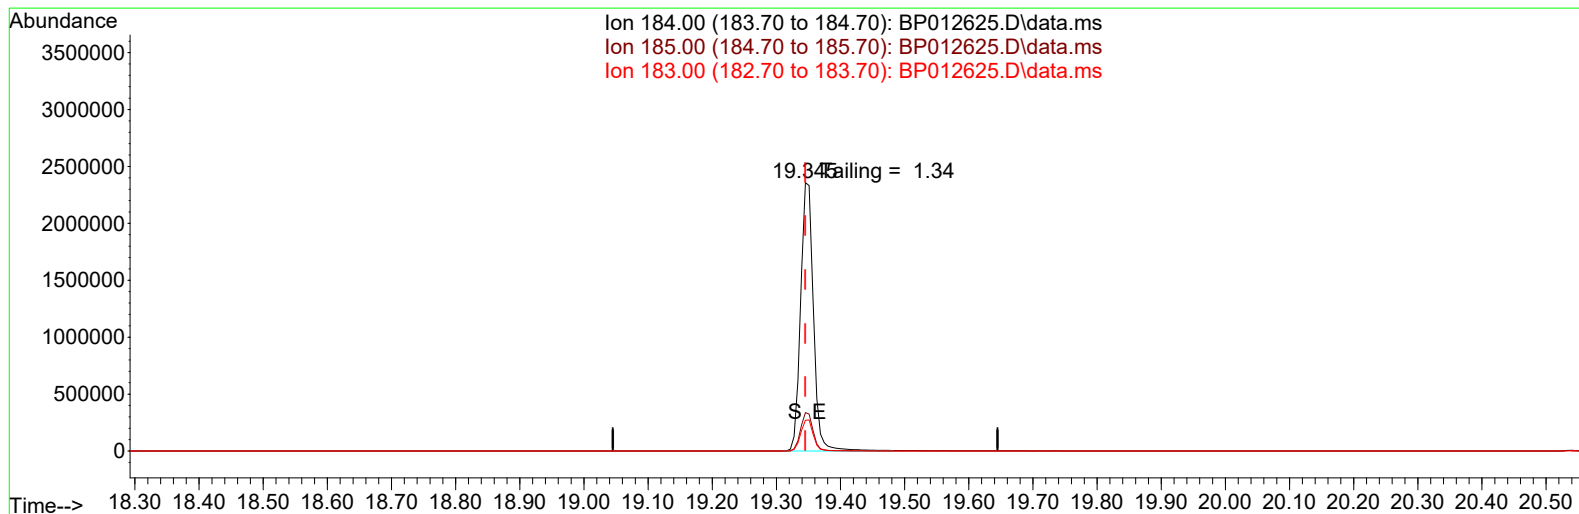

TIC: BP012625.D\data.ms

(77) Benzidine**19.345min (+ 0.000) 199533.99 ng****response 3301614**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.35
183.00	11.60	11.47
0.00	0.00	0.00