
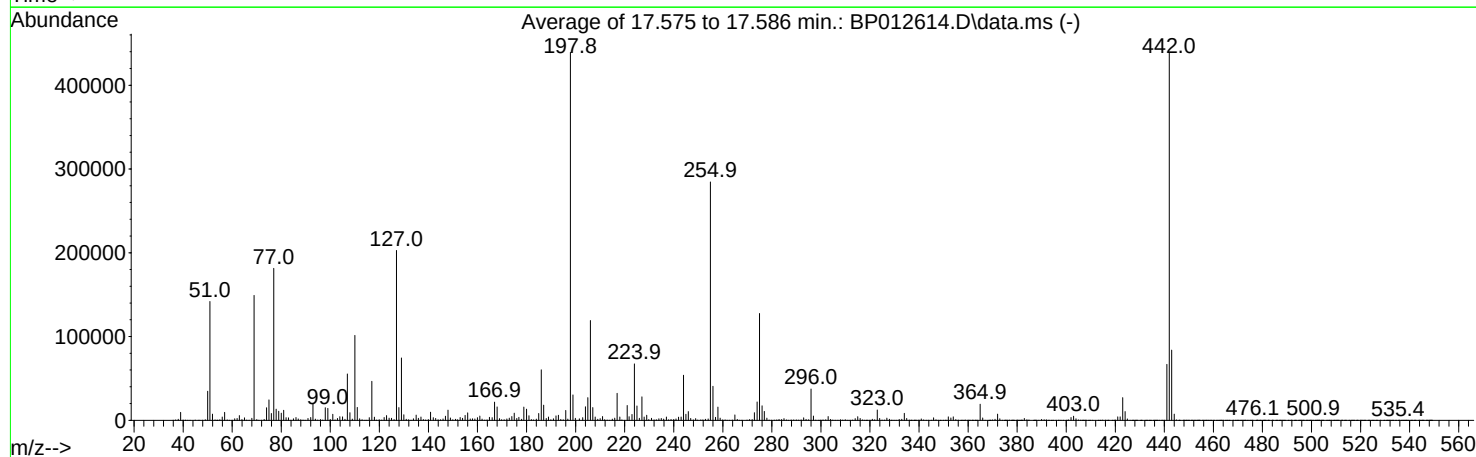


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111222\
 Data File : BP012614.D
 Acq On : 12 Nov 2022 09:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 14 04:00:17 2022

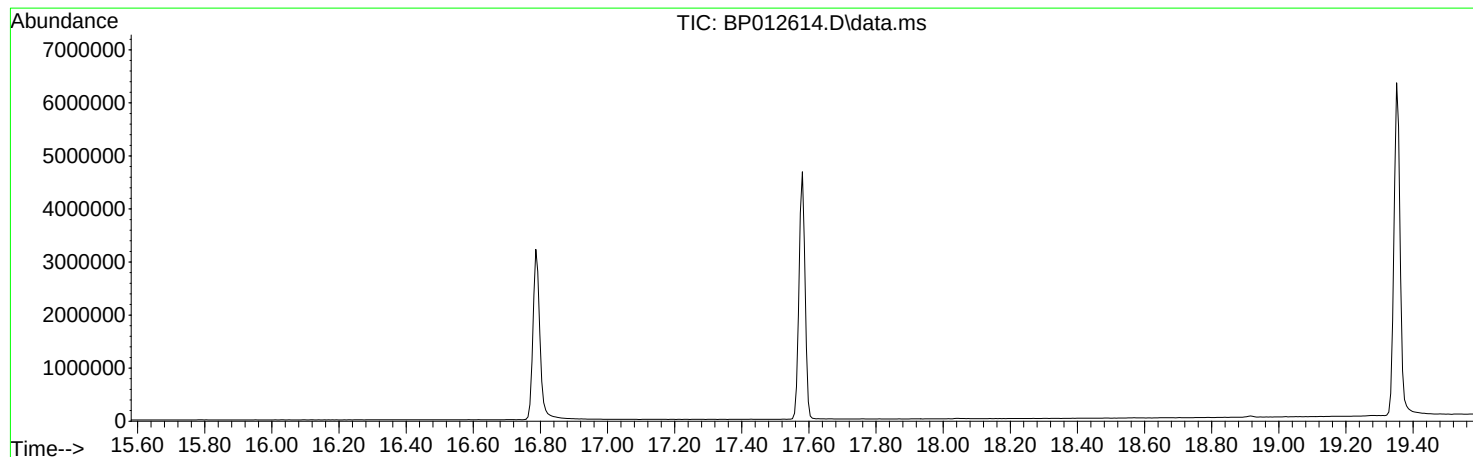




AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.3	141763	PASS
68	69	0.00	2	1.6	2370	PASS
69	198	0.00	100	33.9	149025	PASS
70	69	0.00	2	0.6	936	PASS
127	198	10	80	46.2	202795	PASS
197	198	0.00	2	0.3	1431	PASS
198	198	100	100	100.0	439184	PASS
199	198	5	9	6.9	30202	PASS
275	198	10	60	29.0	127485	PASS
365	198	1	100	4.4	19269	PASS
441	198	0.01	100	15.2	66867	PASS
442	442	100	100	100.0	438545	PASS
443	442	15	24	19.1	83744	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111222\
 Data File : BP012614.D
 Acq On : 12 Nov 2022 09:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Nov 14 07:57:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 14 04:00:17 2022
 Response via : Initial Calibration

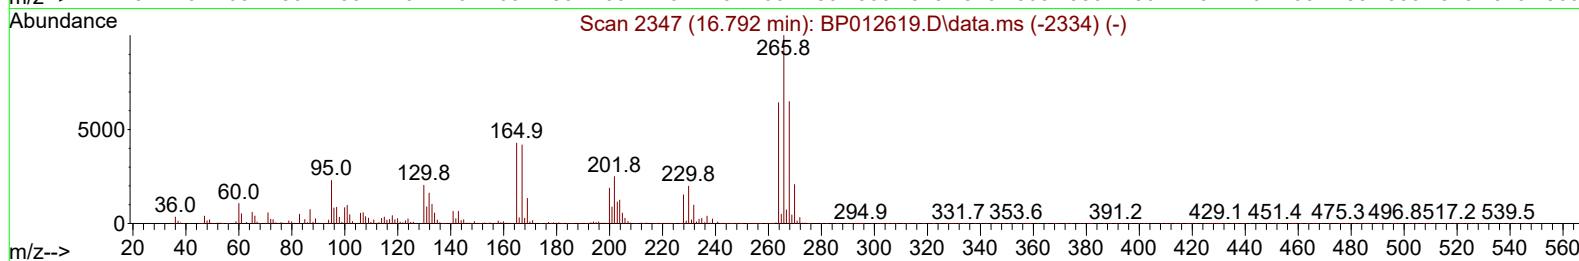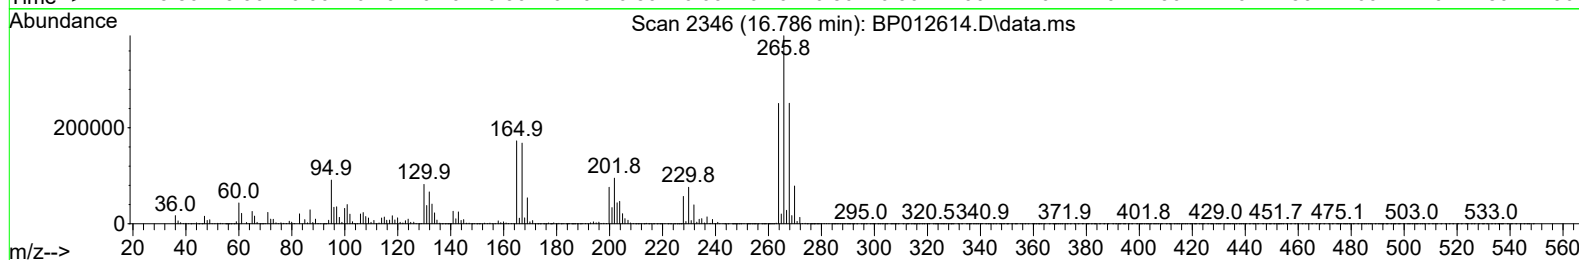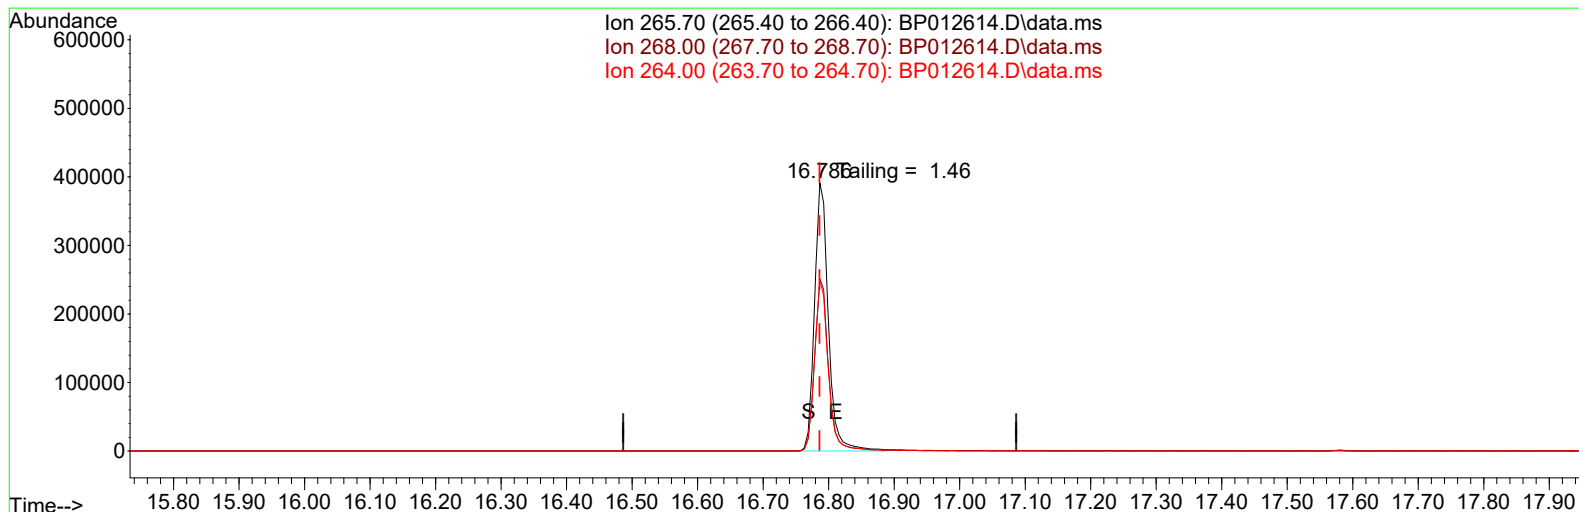

TIC: BP012614.D\data.ms

(70) Pentachlorophenol (C)

16.786min (0.000) 2255058.54 ng




response 578620

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.80	64.08
264.00	64.30	64.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111222\
 Data File : BP012614.D
 Acq On : 12 Nov 2022 09:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Nov 14 07:57:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 14 04:00:17 2022
 Response via : Initial Calibration

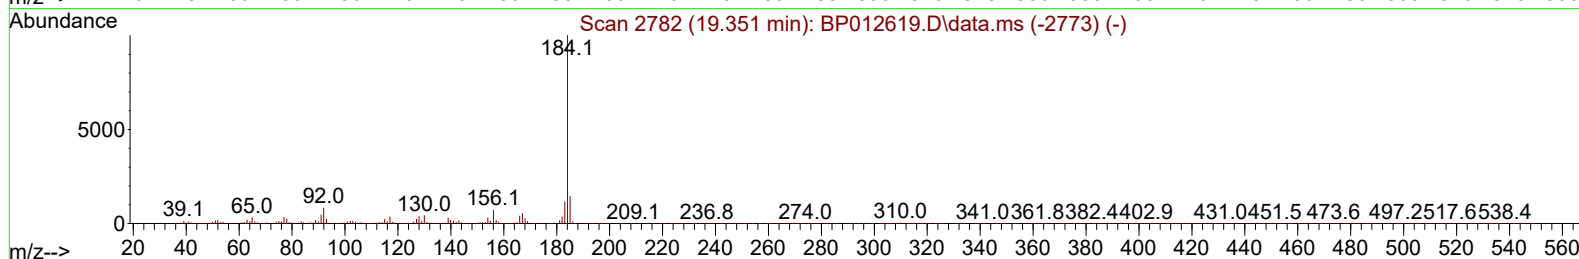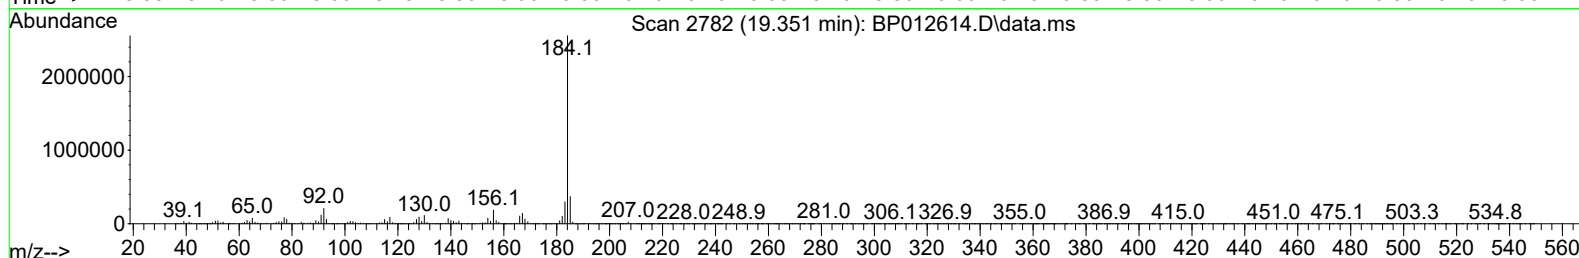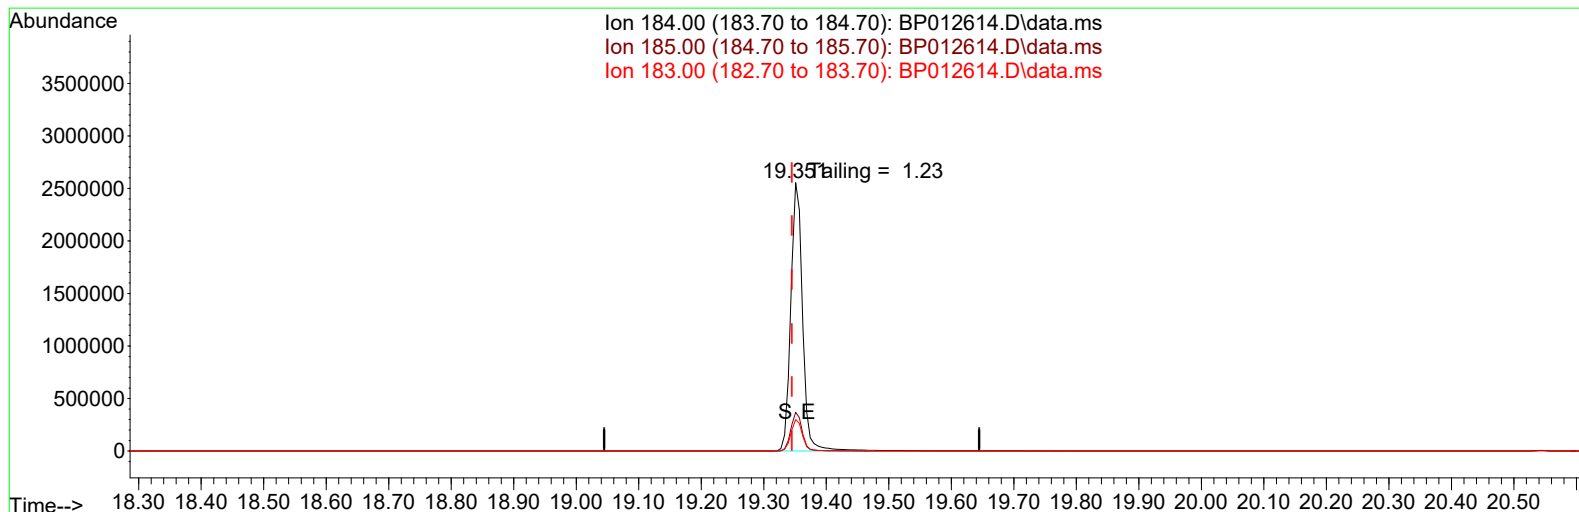

TIC: BP012614.D\data.ms

(77) Benzidine

19.351min (+ 0.006) 814357.46 ng

response 3377700

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.44
183.00	11.60	11.70
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/12/2022	BNA_P	<u>BP012614.D</u>
Compound Name	Response	Retention Time
DDT	1635057	20.545
DDD	17987	20.163
DDE	699	19.616
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18686	1653743	1.13

Instrument :
BNA_P
ClientSampleId :
DFTPP