


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111222\
 Data File : BP012625.D
 Acq On : 12 Nov 2022 18:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 14 04:00:17 2022

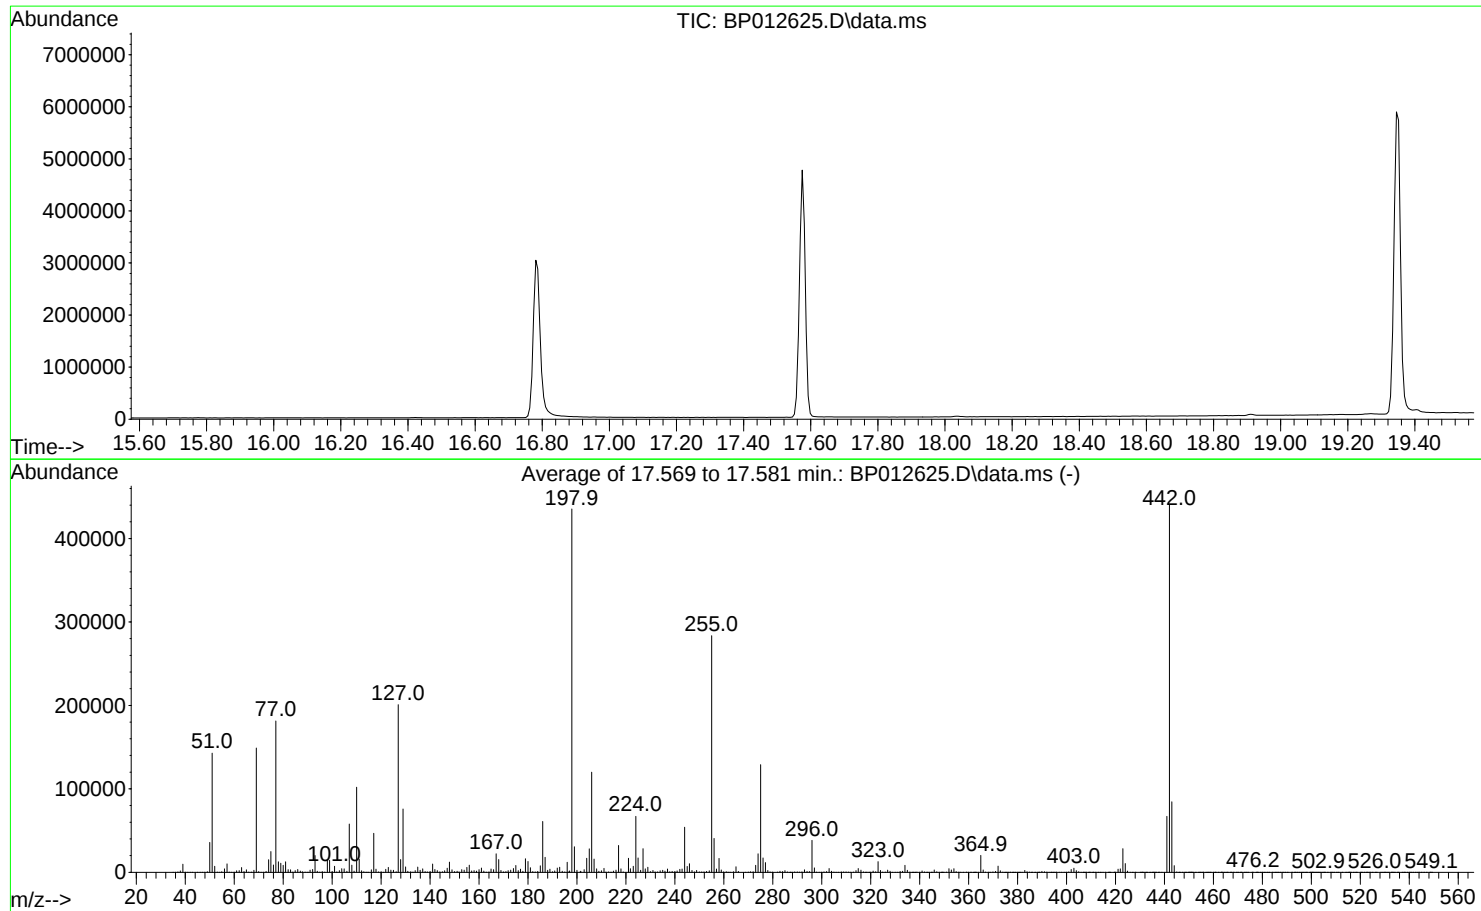


AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.8	142779	PASS
68	69	0.00	2	1.6	2420	PASS
69	198	0.00	100	34.2	148816	PASS
70	69	0.00	2	0.6	821	PASS
127	198	10	80	46.1	200832	PASS
197	198	0.00	2	0.4	1626	PASS
198	198	100	100	100.0	435456	PASS
199	198	5	9	7.0	30584	PASS
275	198	10	60	29.6	129003	PASS
365	198	1	100	4.6	20193	PASS
441	198	0.01	100	15.4	67014	PASS
442	442	100	100	100.0	440869	PASS
443	442	15	24	19.2	84533	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111222\
 Data File : BP012625.D
 Acq On : 12 Nov 2022 18:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Nov 14 08:01:10 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 14 04:00:17 2022
 Response via : Initial Calibration

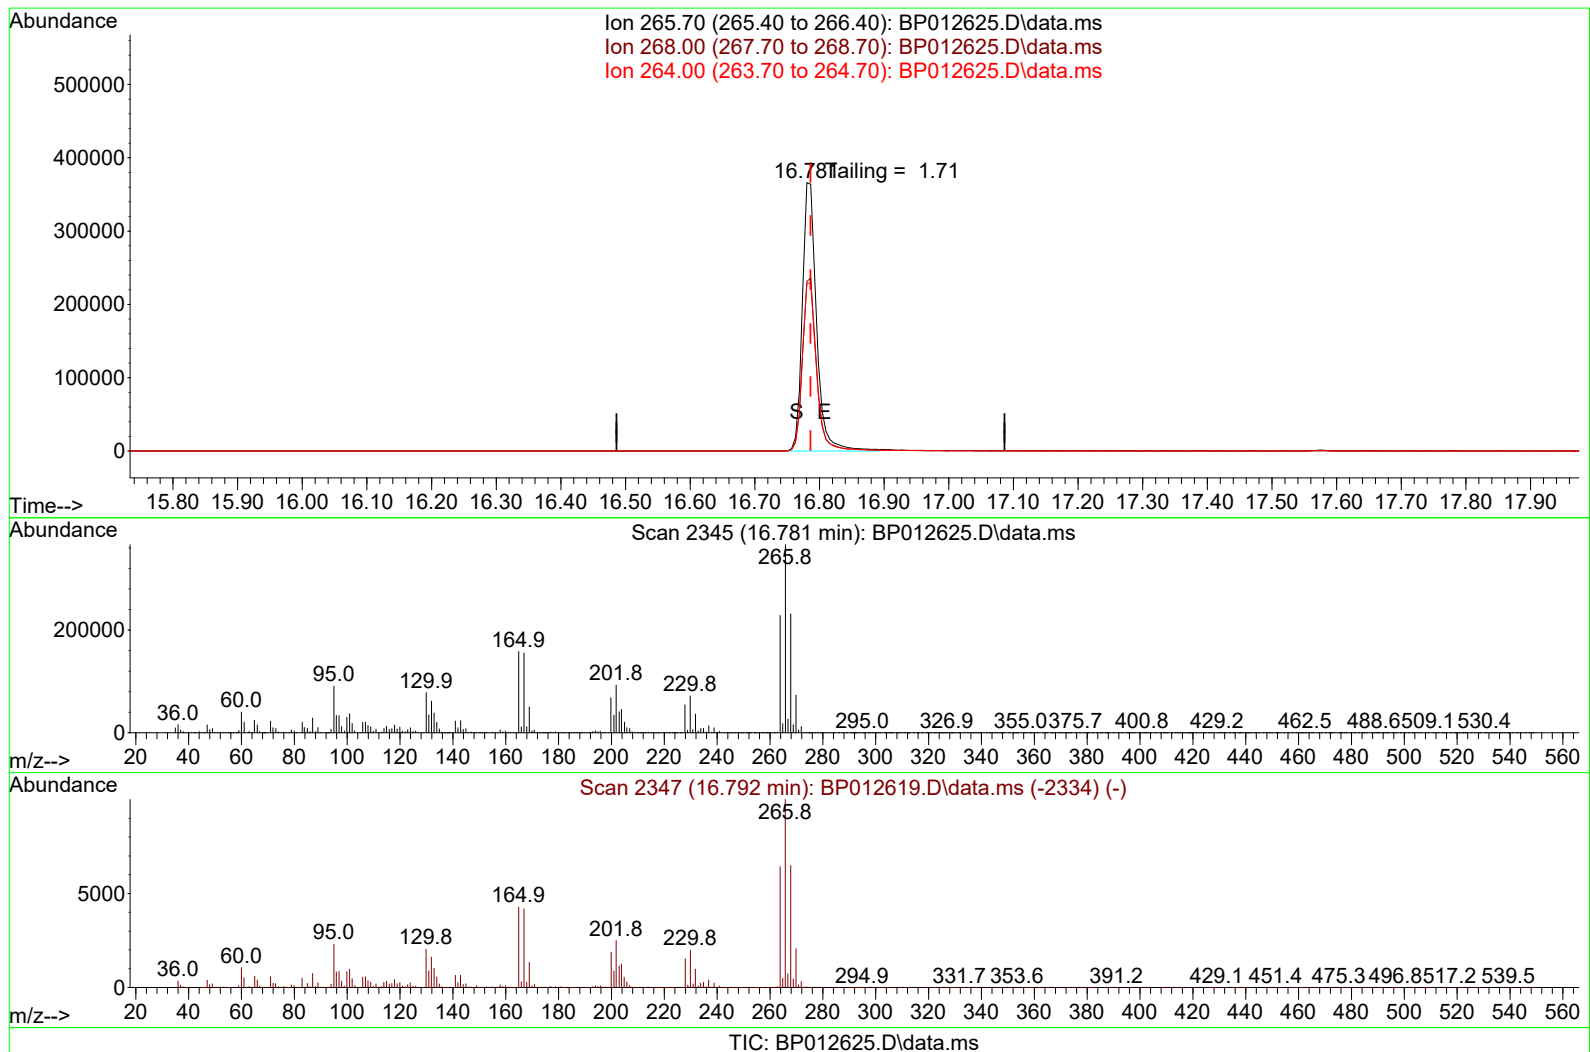

TIC: BP012625.D\data.ms

(70) Pentachlorophenol (C)

16.781min (-0.006) 254201.87 ng




response 563881

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.80	63.22
264.00	64.30	62.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111222\
 Data File : BP012625.D
 Acq On : 12 Nov 2022 18:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Nov 14 08:01:10 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 14 04:00:17 2022
 Response via : Initial Calibration

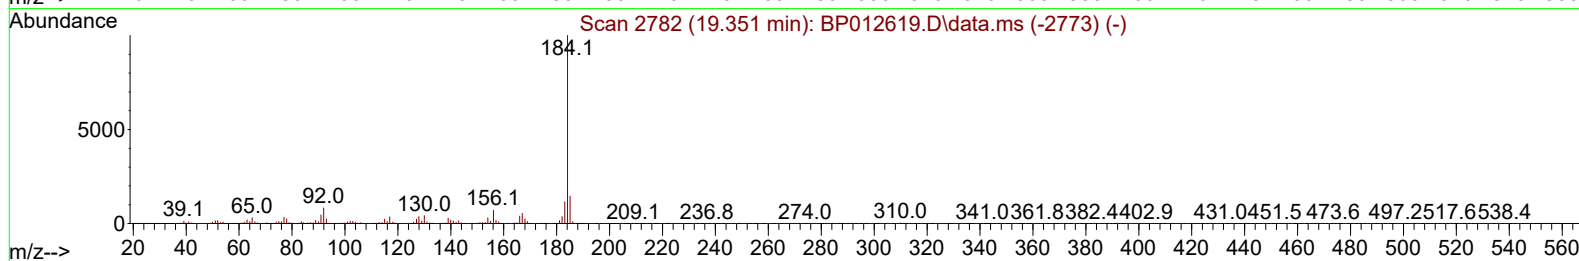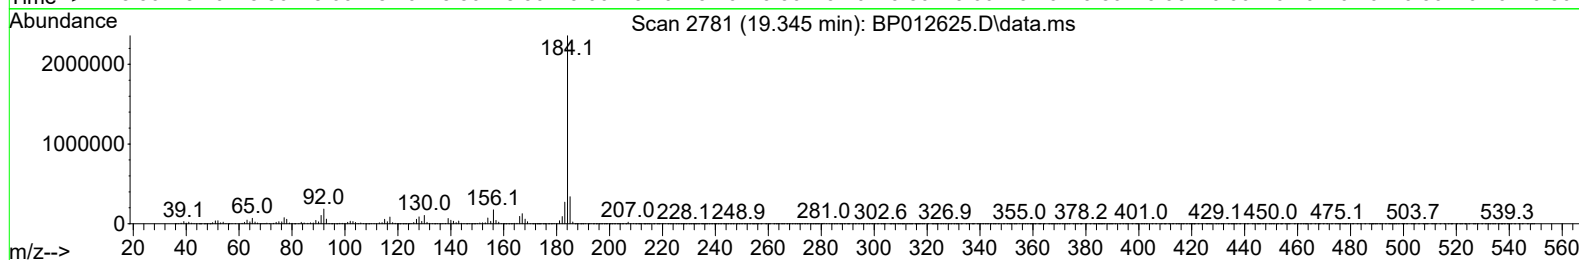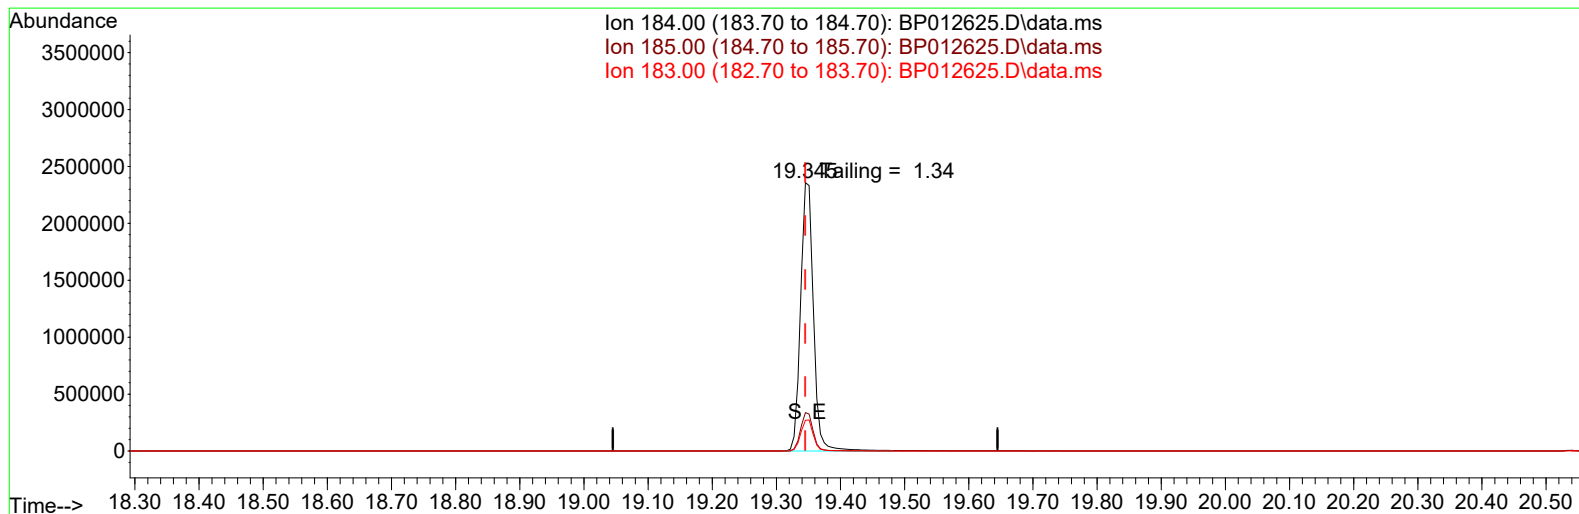

TIC: BP012625.D\data.ms

(77) Benzidine

19.345min (+ 0.000) 199533.99 ng

response 3301614

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.35
183.00	11.60	11.47
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/12/2022	BNA_P	<u>BP012625.D</u>
Compound Name	Response	Retention Time
DDT	1568187	20.539
DDD	43863	20.11
DDE	1261	19.61
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
45124	1613311	2.80

Instrument :
BNA_P
ClientSampleId :
DFTPP