

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111320\
 Data File : BP003955.D
 Acq On : 13 Nov 2020 15:21
 Operator : CG/JU
 Sample : PB132993BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB132993BL

Quant Time: Nov 13 16:23:05 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 12 15:22:47 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.281	152	133777	20.00	ng	0.00
21) Naphthalene-d8	11.110	136	507629	20.00	ng	# 0.00
39) Acenaphthene-d10	14.904	164	313253	20.00	ng	0.00
64) Phenanthrene-d10	17.639	188	660187	20.00	ng	# 0.00
76) Chrysene-d12	21.669	240	602595	20.00	ng	0.00
86) Perylene-d12	24.157	264	601150	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.805	112	1190078	148.47	ng	0.00
7) Phenol-d6	7.452	99	1514954	131.66	ng	0.00
23) Nitrobenzene-d5	9.446	82	982809	94.82	ng	0.00
42) 2,4,6-Tribromophenol	16.392	330	552732	141.07	ng	0.00
45) 2-Fluorobiphenyl	13.528	172	2104926	93.94	ng	0.00
79) Terphenyl-d14	20.139	244	2914471	93.44	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111320\
Data File : BP003955.D
Acq On : 13 Nov 2020 15:21
Operator : CG/JU
Sample : PB132993BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB132993BL

Quant Time: Nov 13 16:23:05 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 12 15:22:47 2020
Response via : Initial Calibration



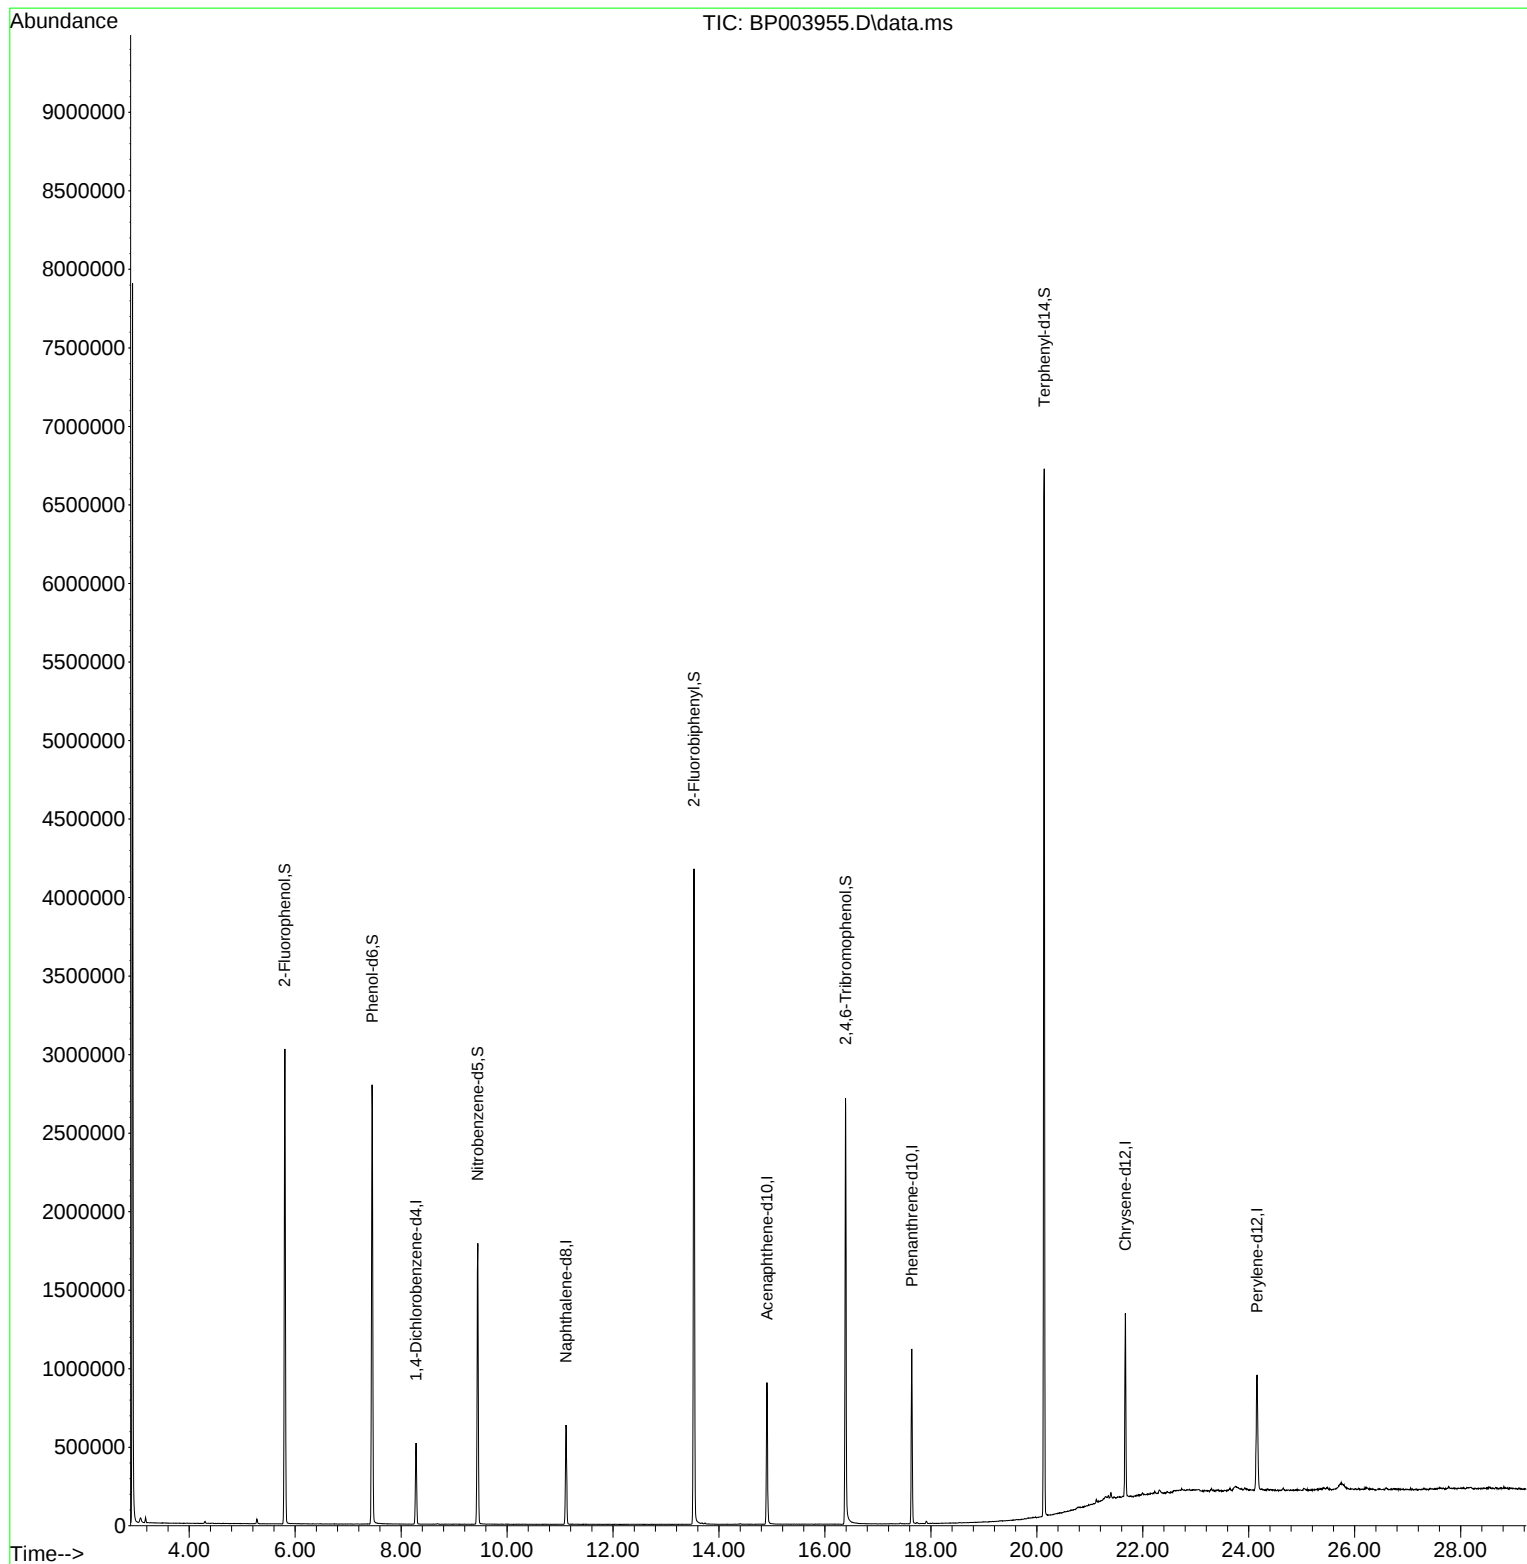


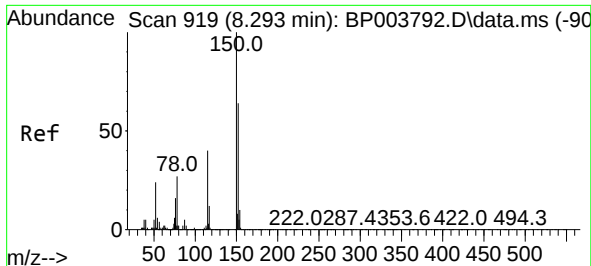

#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.281 min Scan# 917
Delta R.T. 0.000 min
Lab File: BP003955.D
Acq: 13 Nov 2020 15:21




Instrument :
BNA_P
ClientSampleId :
PB132993BL

Tgt Ion:152 Resp: 133777
Ion Ratio Lower Upper
152 100
150 152.0 123.8 185.6
115 59.1 43.8 65.6

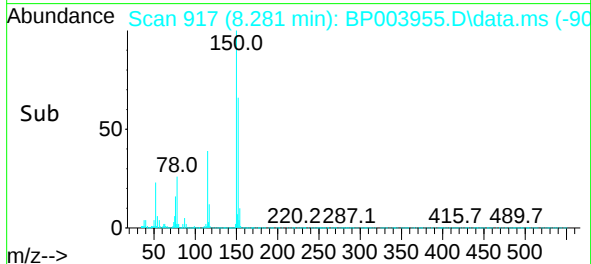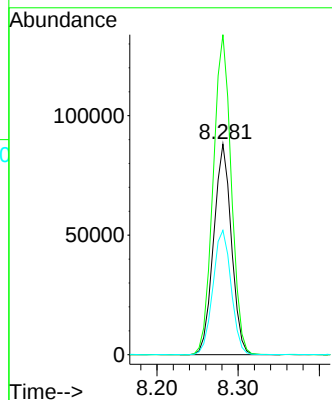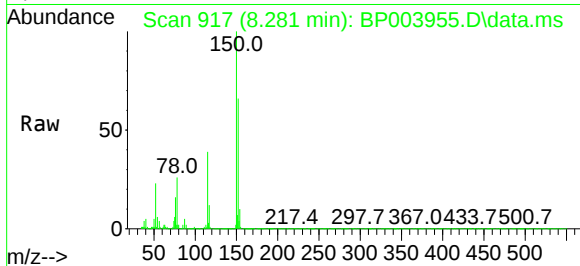

#5
2-Fluorophenol
Concen: 148.47 ng
RT: 5.805 min Scan# 496
Delta R.T. 0.000 min
Lab File: BP003955.D
Acq: 13 Nov 2020 15:21

Tgt Ion:112 Resp: 1190078
Ion Ratio Lower Upper
112 100
64 64.7 32.8 49.2#
63 33.8 17.0 25.4#


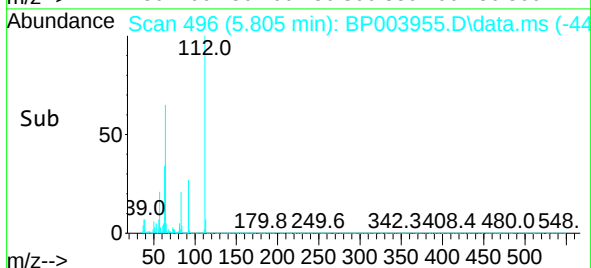
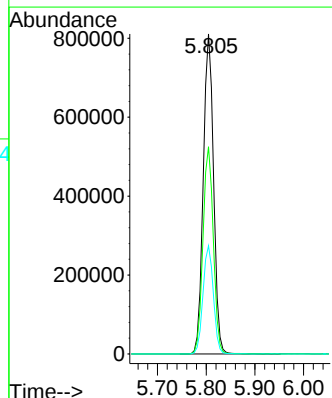
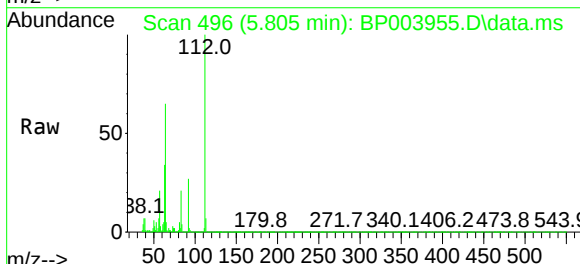




#7
Phenol-d6
Concen: 131.66 ng
RT: 7.452 min Scan# 776
Delta R.T. 0.000 min
Lab File: BP003955.D
Acq: 13 Nov 2020 15:21




Instrument :
BNA_P
ClientSampleId :
PB132993BL

Tgt Ion: 99 Resp: 1514954
Ion Ratio Lower Upper
99 100
42 20.4 8.6 13.0#
71 36.6 23.4 35.2#

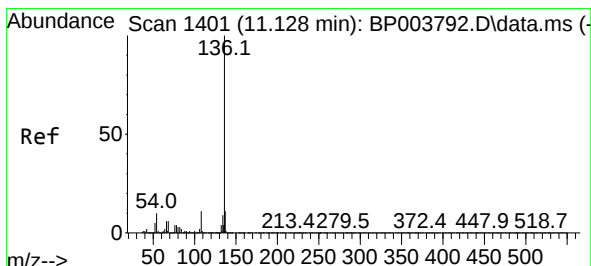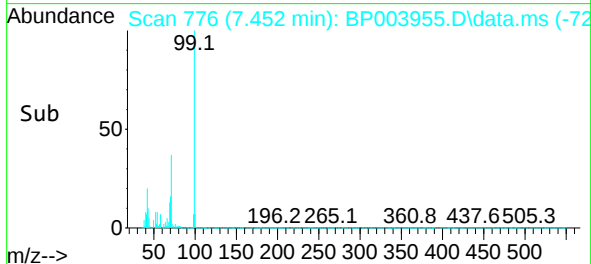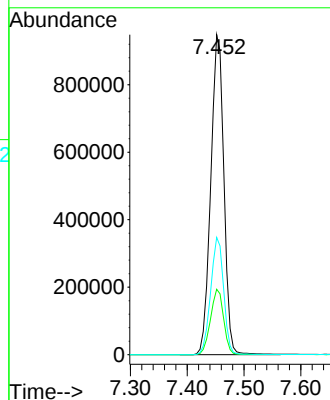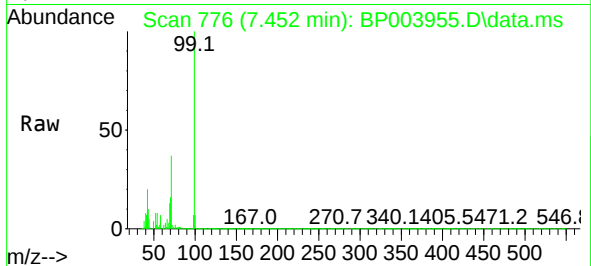

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 11.110 min Scan# 1398
Delta R.T. -0.006 min
Lab File: BP003955.D
Acq: 13 Nov 2020 15:21

Tgt Ion: 136 Resp: 507629
Ion Ratio Lower Upper
136 100
137 10.8 8.6 13.0
54 9.7 3.6 5.4#
68 6.1 3.3 4.9#


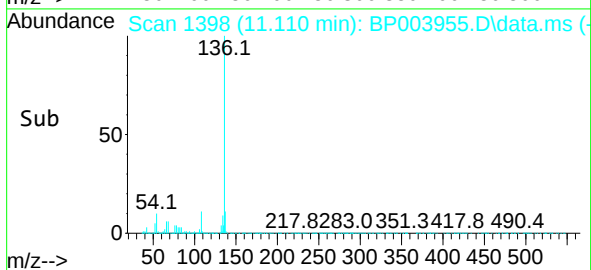
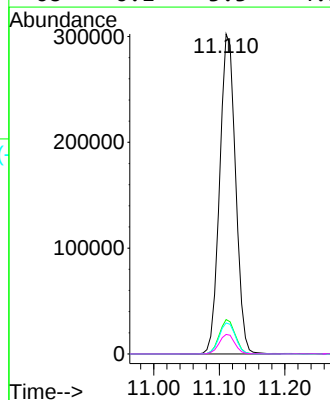
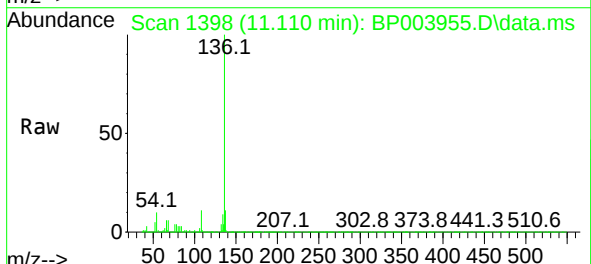




#23
Nitrobenzene-d5
Concen: 94.82 ng
RT: 9.446 min Scan# 1115
Delta R.T. 0.000 min
Lab File: BP003955.D
Acq: 13 Nov 2020 15:21




Instrument :
BNA_P
ClientSampleId :
PB132993BL


Tgt Ion: 82 Resp: 982809
Ion Ratio Lower Upper
82 100
128 41.4 45.6 68.4#
54 55.6 30.1 45.1#

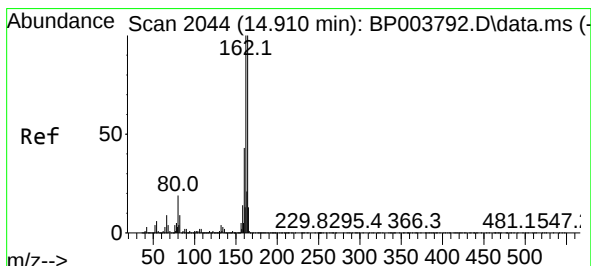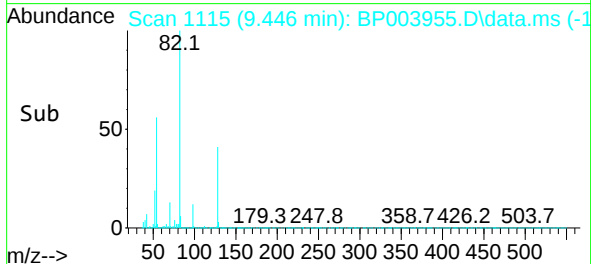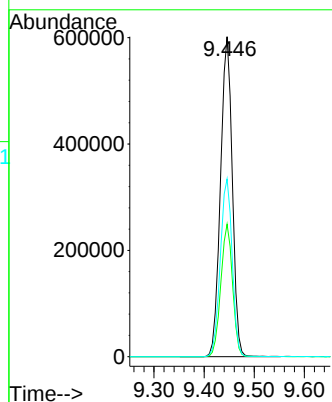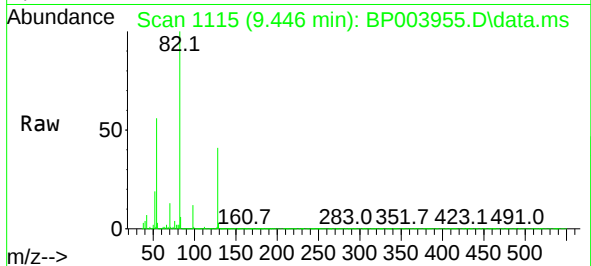

#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.904 min Scan# 2043
Delta R.T. -0.006 min
Lab File: BP003955.D
Acq: 13 Nov 2020 15:21

Tgt Ion: 164 Resp: 313253
Ion Ratio Lower Upper
164 100
162 102.2 79.4 119.2
160 43.8 36.1 54.1


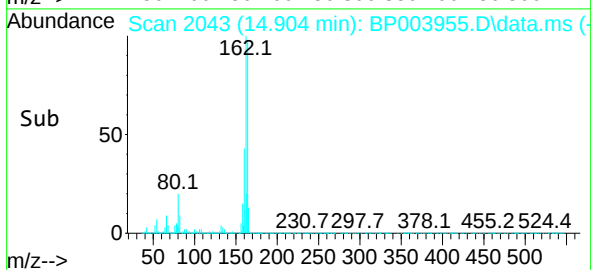
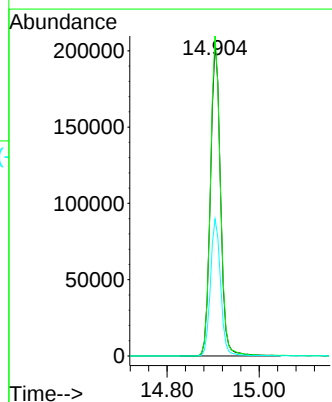
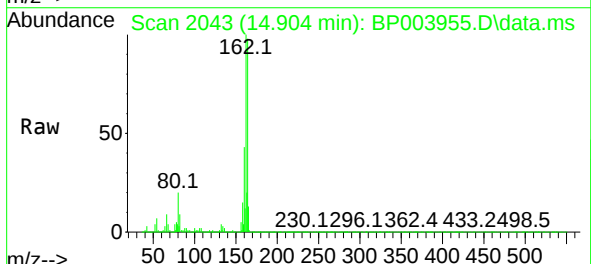


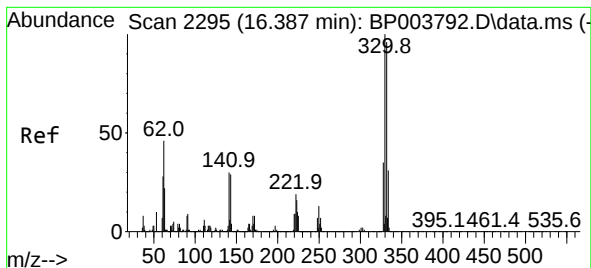

#42
2,4,6-Tribromophenol
Concen: 141.07 ng
RT: 16.392 min Scan# 2296
Delta R.T. 0.000 min
Lab File: BP003955.D
Acq: 13 Nov 2020 15:21




Instrument :
BNA_P
ClientSampleId :
PB132993BL


Tgt Ion:330 Resp: 552732
Ion Ratio Lower Upper
330 100
332 96.8 77.1 115.7
141 31.9 23.4 35.2

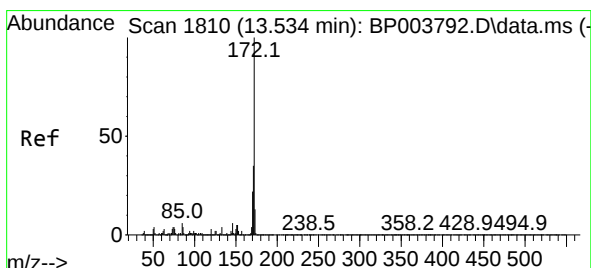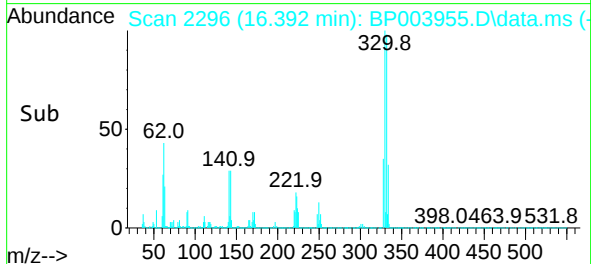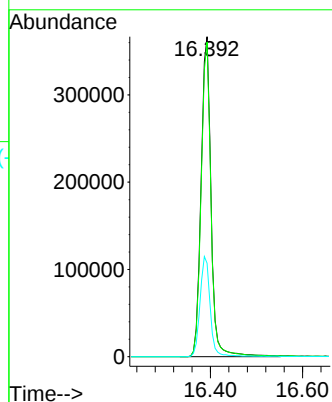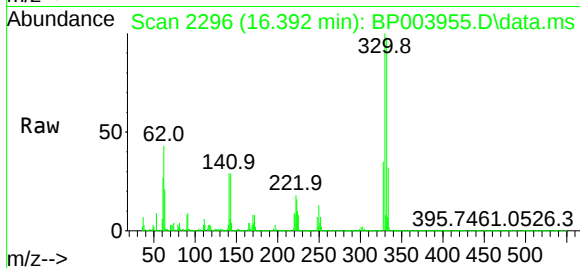

#45
2-Fluorobiphenyl
Concen: 93.94 ng
RT: 13.528 min Scan# 1809
Delta R.T. 0.000 min
Lab File: BP003955.D
Acq: 13 Nov 2020 15:21

Tgt Ion:172 Resp: 2104926
Ion Ratio Lower Upper
172 100
171 35.1 28.5 42.7
170 22.8 19.2 28.8


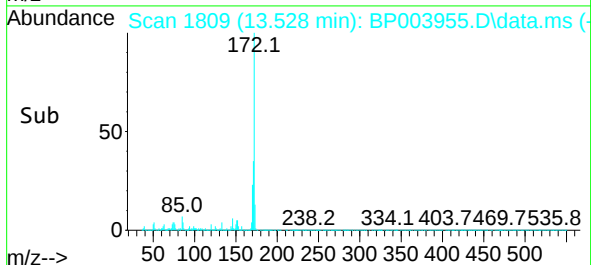
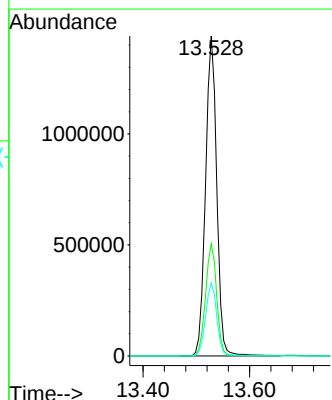
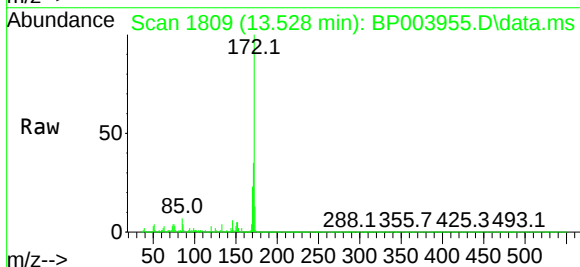


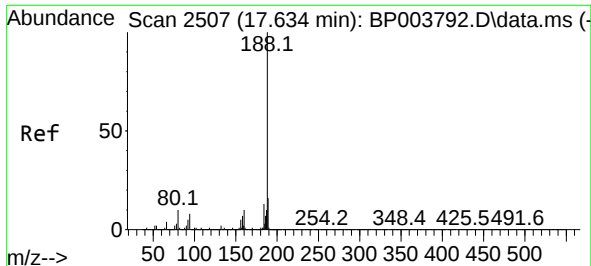

#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.639 min Scan# 2508
Delta R.T. 0.000 min
Lab File: BP003955.D
Acq: 13 Nov 2020 15:21




Instrument :
BNA_P
ClientSampleId :
PB132993BL


Tgt Ion:188 Resp: 660187
Ion Ratio Lower Upper
188 100
94 8.2 6.2 9.2
80 9.6 6.2 9.2#

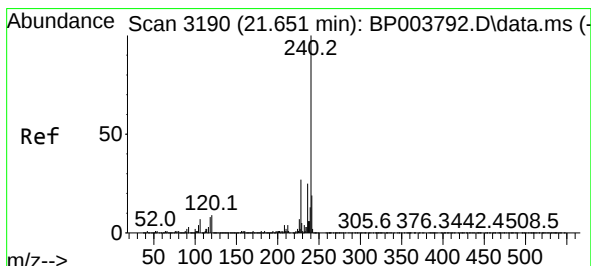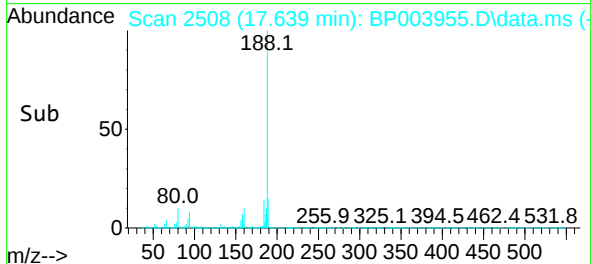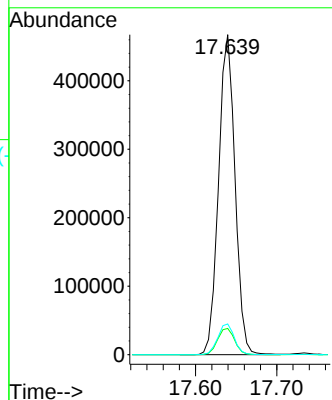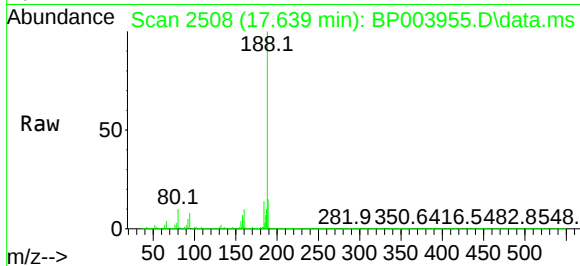

#76
Chrysene-d12
Concen: 20.00 ng
RT: 21.669 min Scan# 3193
Delta R.T. -0.006 min
Lab File: BP003955.D
Acq: 13 Nov 2020 15:21

Tgt Ion:240 Resp: 602595
Ion Ratio Lower Upper
240 100
120 9.1 7.8 11.6
236 25.0 20.8 31.2


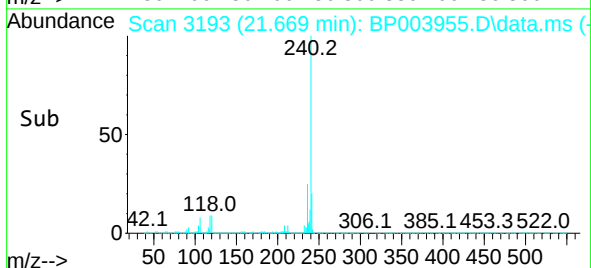
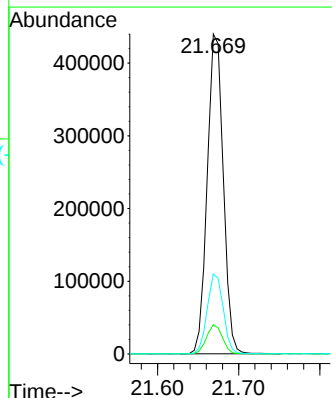
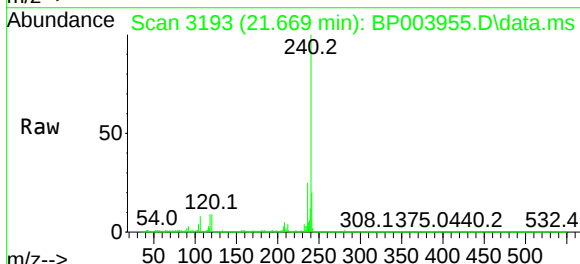


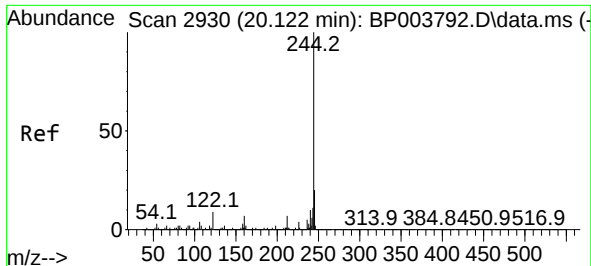

#79
Terphenyl-d14
Concen: 93.44 ng
RT: 20.139 min Scan# 2933
Delta R.T. 0.006 min
Lab File: BP003955.D
Acq: 13 Nov 2020 15:21

Instrument :
BNA_P
ClientSampleId :
PB132993BL

Tgt Ion:244 Resp: 2914471
Ion Ratio Lower Upper
244 100
212 7.2 5.8 8.6
122 8.8 7.8 11.8

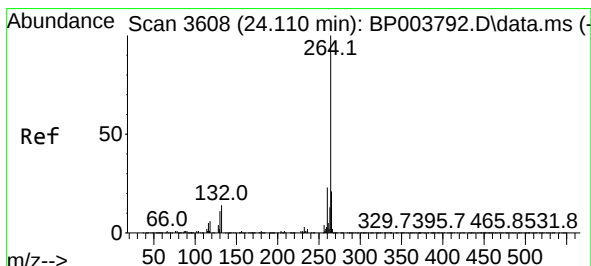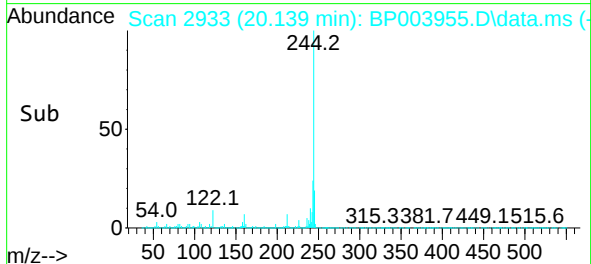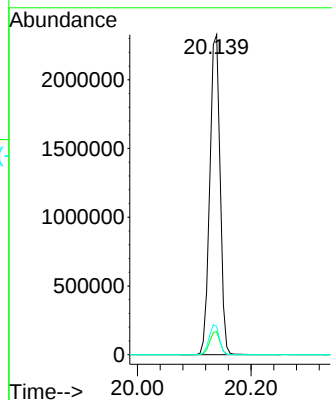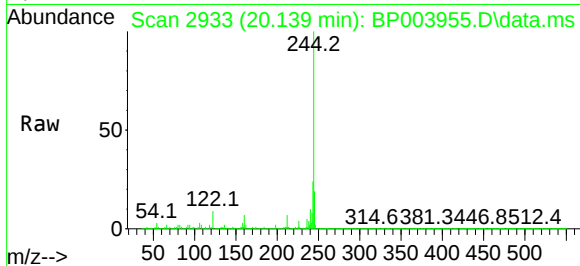

#86
Perylene-d12
Concen: 20.00 ng
RT: 24.157 min Scan# 3616
Delta R.T. 0.000 min
Lab File: BP003955.D
Acq: 13 Nov 2020 15:21

Tgt Ion:264 Resp: 601150
Ion Ratio Lower Upper
264 100
260 21.9 18.8 28.2
265 21.2 17.4 26.2

