

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111320\
 Data File : BP003962.D
 Acq On : 13 Nov 2020 19:32
 Operator : CG/JU
 Sample : L4719-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 TP-3-D

Quant Time: Nov 16 08:20:33 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 12 15:22:47 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.281	152	127376	20.00	ng	0.00
21) Naphthalene-d8	11.110	136	487351	20.00	ng	# 0.00
39) Acenaphthene-d10	14.904	164	288033	20.00	ng	0.00
64) Phenanthrene-d10	17.639	188	597340	20.00	ng	# 0.00
76) Chrysene-d12	21.668	240	537998	20.00	ng	0.00
86) Perylene-d12	24.157	264	544072	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.805	112	813617	106.61	ng	0.00
7) Phenol-d6	7.452	99	932179	85.09	ng	0.00
23) Nitrobenzene-d5	9.440	82	773562	77.74	ng	0.00
42) 2,4,6-Tribromophenol	16.386	330	429754	119.29	ng	0.00
45) 2-Fluorobiphenyl	13.528	172	1602504	77.78	ng	0.00
79) Terphenyl-d14	20.133	244	2157668	77.48	ng	0.00
Target Compounds						
32) Benzoic acid	10.416	122	18031	11.60	ng	# 71
50) Dimethylphthalate	14.328	163	191949	8.53	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111320\
Data File : BP003962.D
Acq On : 13 Nov 2020 19:32
Operator : CG/JU
Sample : L4719-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TP-3-D

Quant Time: Nov 16 08:20:33 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 12 15:22:47 2020
Response via : Initial Calibration




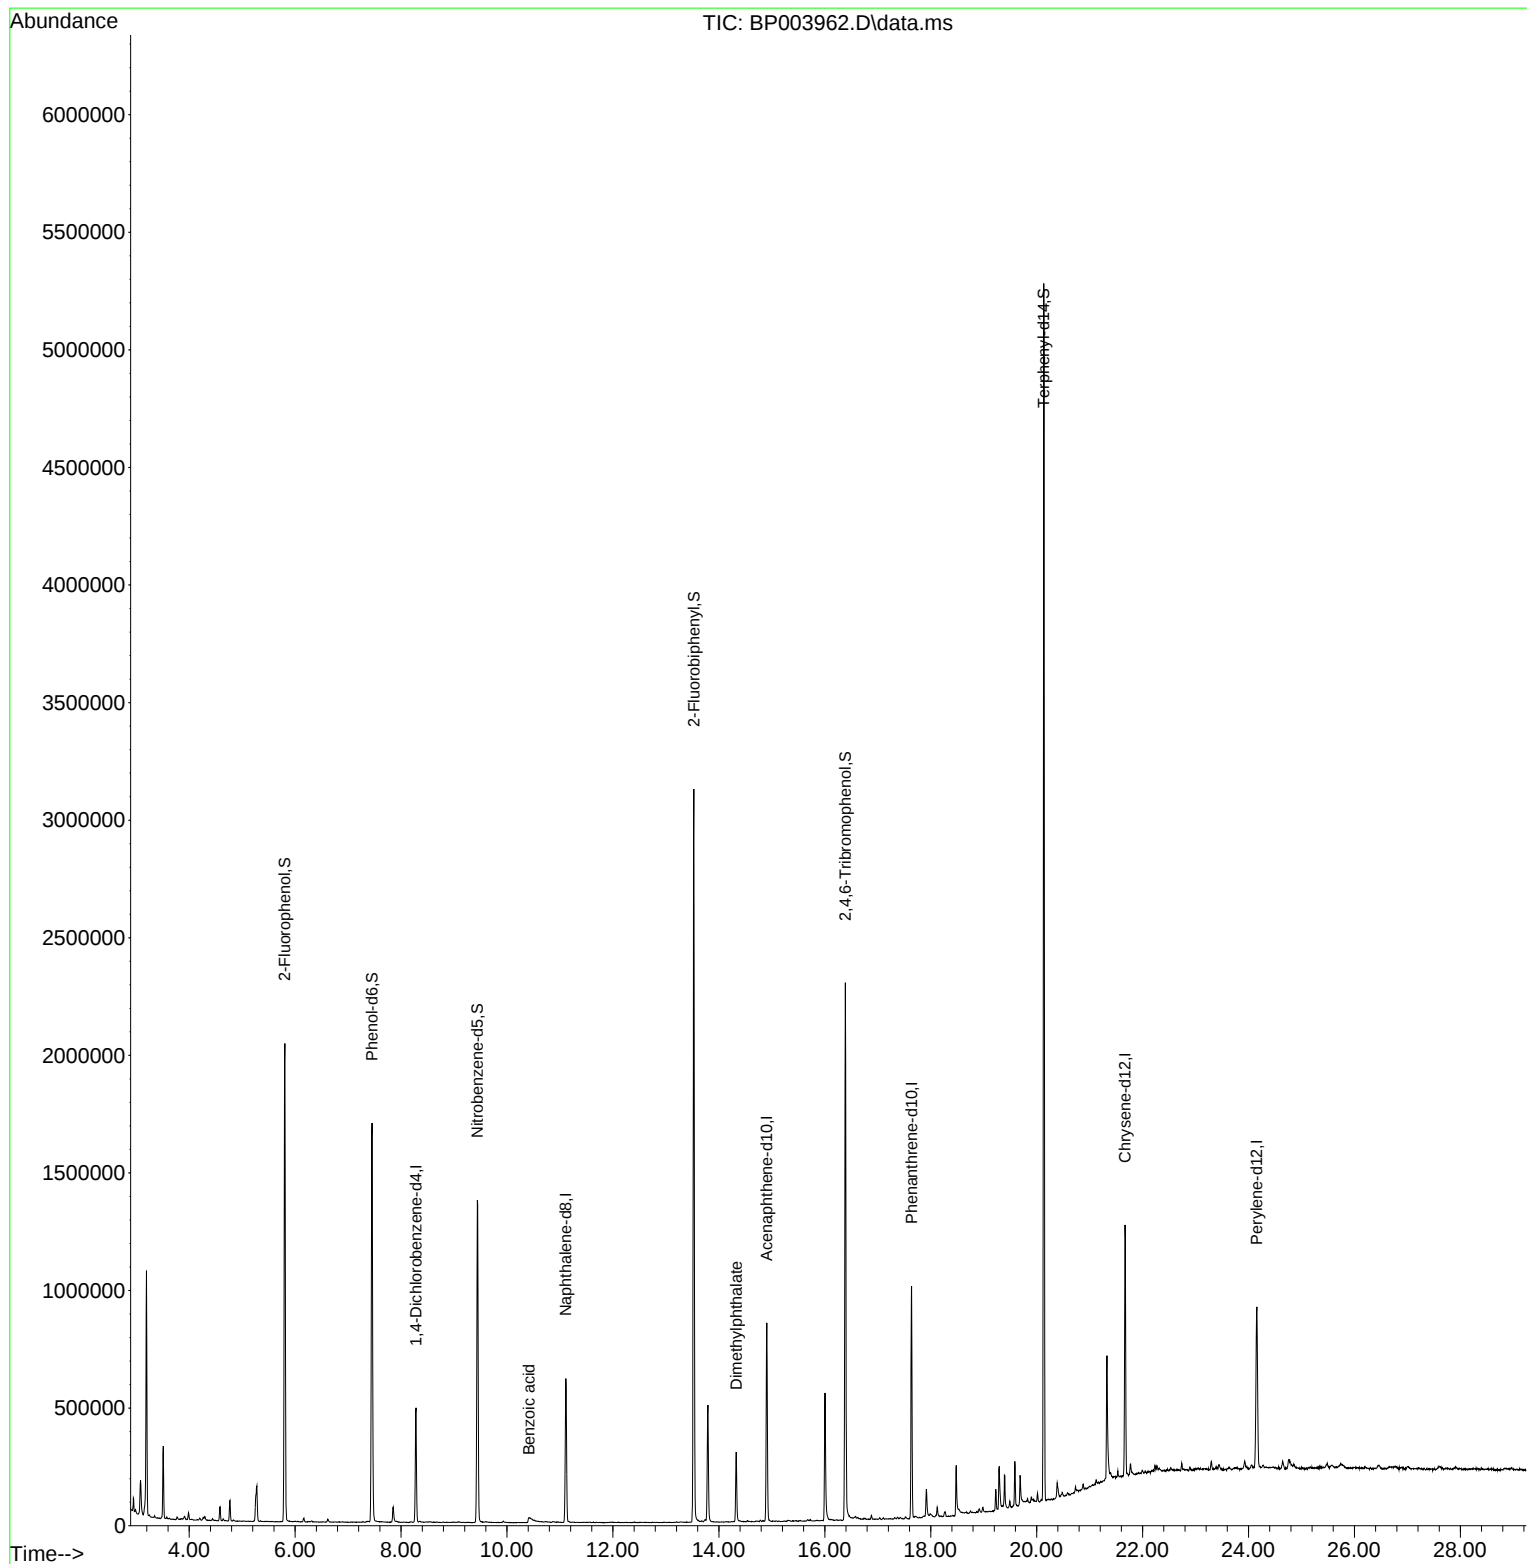




#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.281 min Scan# 917
Delta R.T. -0.000 min
Lab File: BP003962.D
Acq: 13 Nov 2020 19:32




Instrument :
BNA_P
ClientSampleId :
TP-3-D

Tgt Ion:152 Resp: 127376
Ion Ratio Lower Upper
152 100
150 152.3 123.8 185.6
115 59.9 43.8 65.6

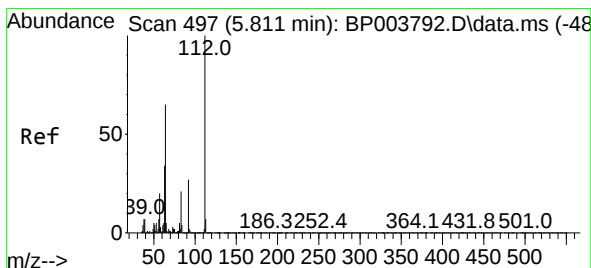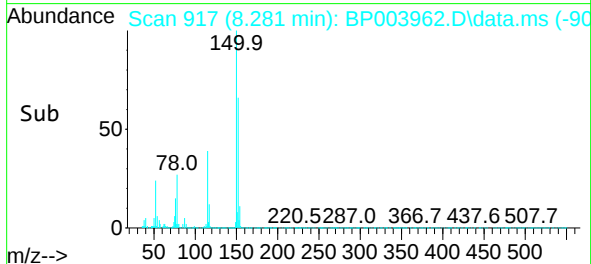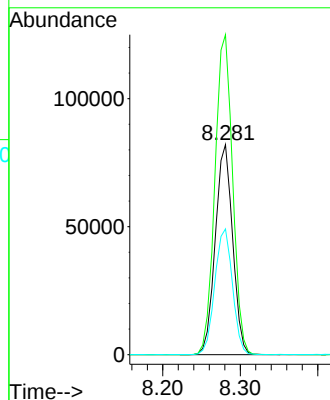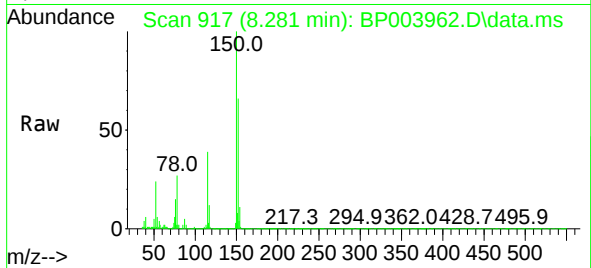

#5
2-Fluorophenol
Concen: 106.61 ng
RT: 5.805 min Scan# 496
Delta R.T. -0.000 min
Lab File: BP003962.D
Acq: 13 Nov 2020 19:32

Tgt Ion:112 Resp: 813617
Ion Ratio Lower Upper
112 100
64 64.0 32.8 49.2#
63 33.9 17.0 25.4#


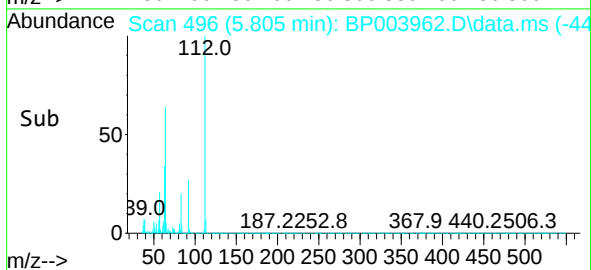
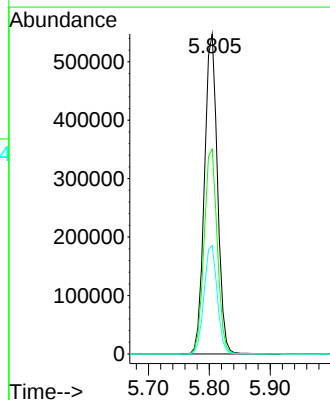
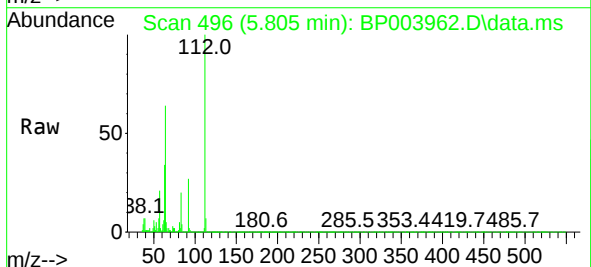




#7
Phenol-d6
Concen: 85.09 ng
RT: 7.452 min Scan# 776
Delta R.T. -0.000 min
Lab File: BP003962.D
Acq: 13 Nov 2020 19:32




Instrument :
BNA_P
ClientSampleId :
TP-3-D


Tgt Ion: 99 Resp: 932179
Ion Ratio Lower Upper
99 100
42 19.9 8.6 13.0#
71 36.8 23.4 35.2#

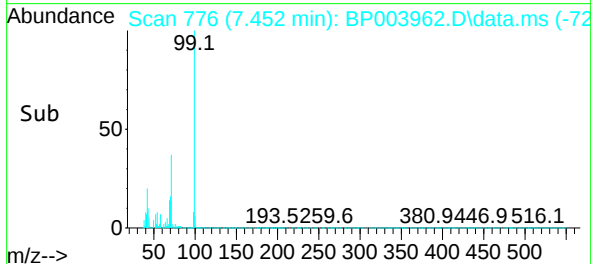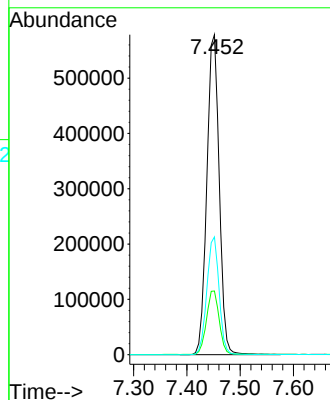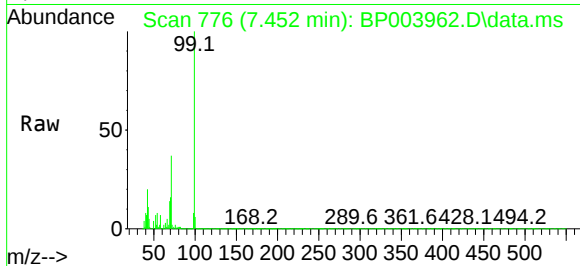

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 11.110 min Scan# 1398
Delta R.T. -0.006 min
Lab File: BP003962.D
Acq: 13 Nov 2020 19:32

Tgt Ion: 136 Resp: 487351
Ion Ratio Lower Upper
136 100
137 10.7 8.6 13.0
54 9.7 3.6 5.4#
68 6.2 3.3 4.9#


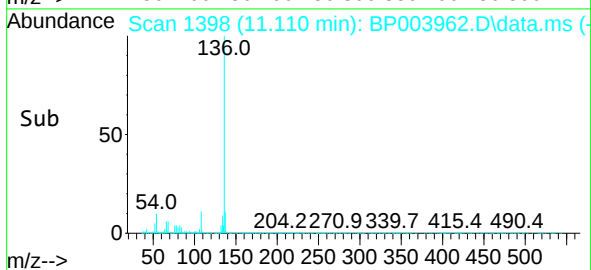
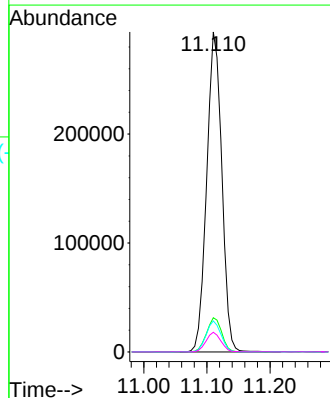
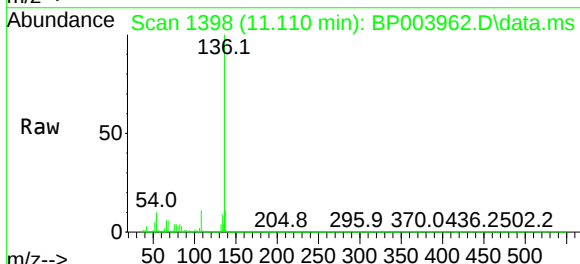


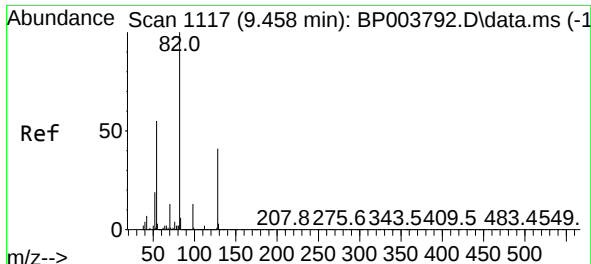

#23
Nitrobenzene-d5
Concen: 77.74 ng
RT: 9.440 min Scan# 1114
Delta R.T. -0.006 min
Lab File: BP003962.D
Acq: 13 Nov 2020 19:32




Instrument :
BNA_P
ClientSampleId :
TP-3-D


Tgt Ion: 82 Resp: 773562
Ion Ratio Lower Upper
82 100
128 40.2 45.6 68.4#
54 55.2 30.1 45.1#

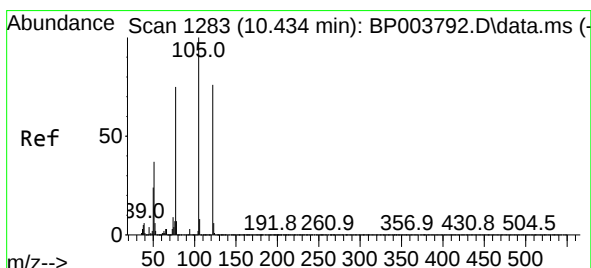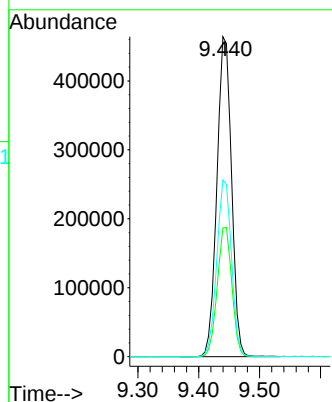

#32
Benzoic acid
Concen: 11.60 ng
RT: 10.416 min Scan# 1280
Delta R.T. -0.024 min
Lab File: BP003962.D
Acq: 13 Nov 2020 19:32

Tgt Ion: 122 Resp: 18031
Ion Ratio Lower Upper
122 100
105 134.5 94.1 134.1#
77 106.7 50.1 90.1#


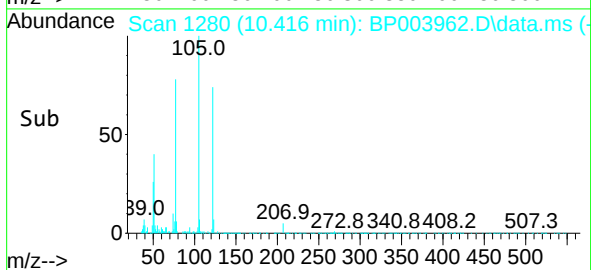
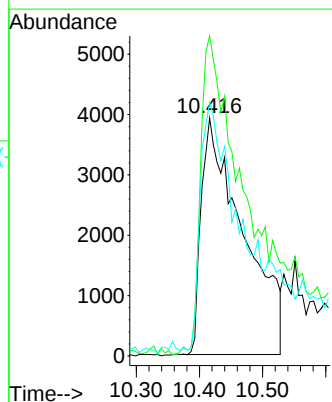
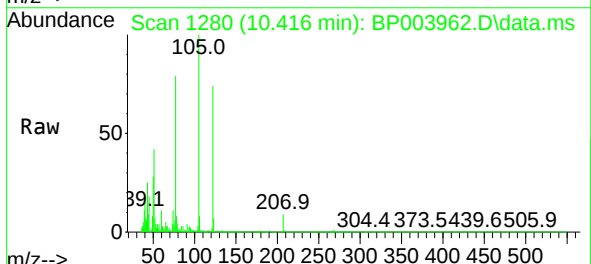




#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.904 min Scan# 2043
Delta R.T. -0.006 min
Lab File: BP003962.D
Acq: 13 Nov 2020 19:32




Instrument :
BNA_P
ClientSampled :
TP-3-D


Tgt Ion:164 Resp: 288033
Ion Ratio Lower Upper
164 100
162 101.8 79.4 119.2
160 44.8 36.1 54.1

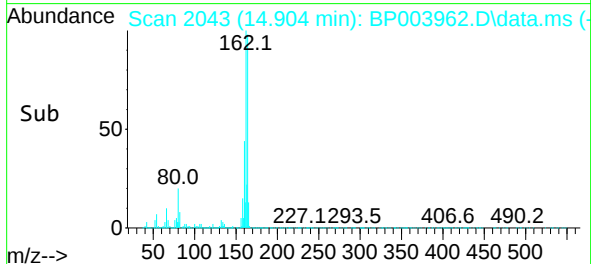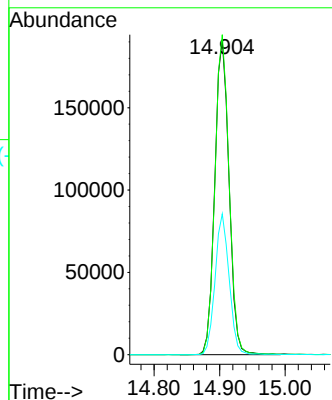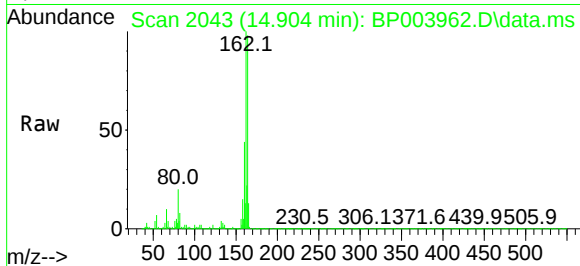

#42
2,4,6-Tribromophenol
Concen: 119.29 ng
RT: 16.386 min Scan# 2295
Delta R.T. -0.006 min
Lab File: BP003962.D
Acq: 13 Nov 2020 19:32

Tgt Ion:330 Resp: 429754
Ion Ratio Lower Upper
330 100
332 97.0 77.1 115.7
141 33.4 23.4 35.2


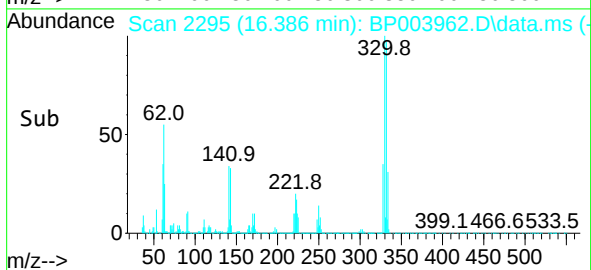
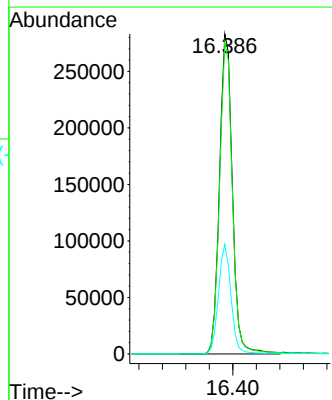
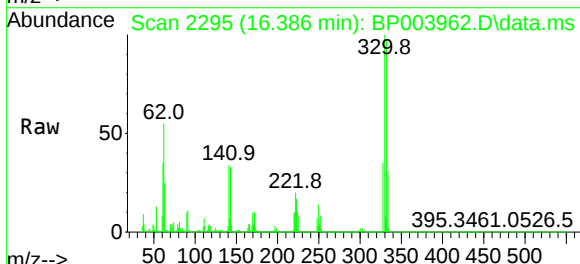




#45
2-Fluorobiphenyl
Concen: 77.78 ng
RT: 13.528 min Scan# 1809
Delta R.T. -0.000 min
Lab File: BP003962.D
Acq: 13 Nov 2020 19:32




Instrument :
BNA_P
ClientSampleId :
TP-3-D


Tgt Ion:172 Resp: 1602504
Ion Ratio Lower Upper
172 100
171 34.9 28.5 42.7
170 22.6 19.2 28.8

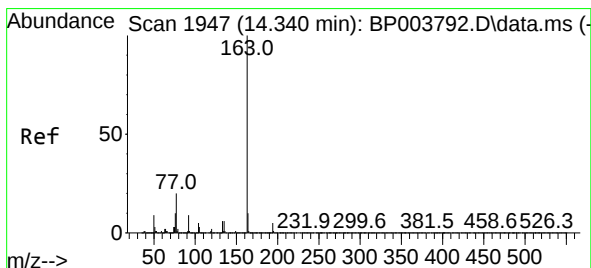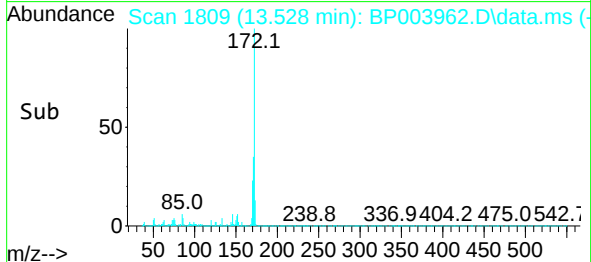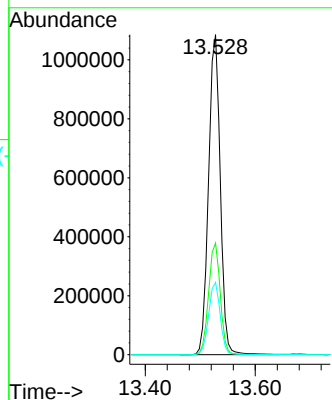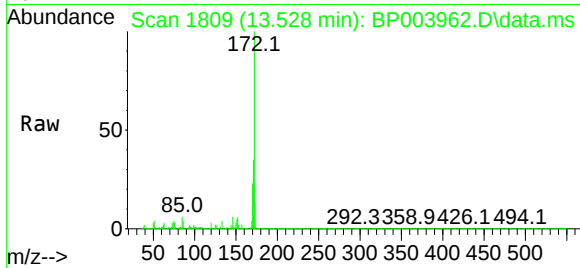

#50
Dimethylphthalate
Concen: 8.53 ng
RT: 14.328 min Scan# 1945
Delta R.T. -0.006 min
Lab File: BP003962.D
Acq: 13 Nov 2020 19:32

Tgt Ion:163 Resp: 191949
Ion Ratio Lower Upper
163 100
194 4.3 3.3 4.9
164 10.7 8.2 12.2


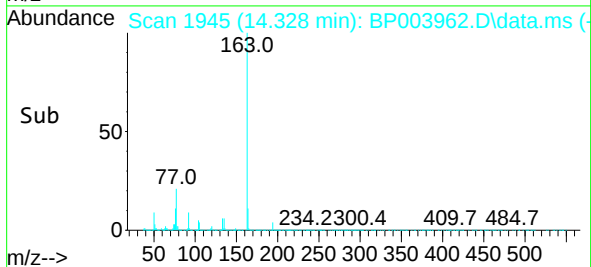
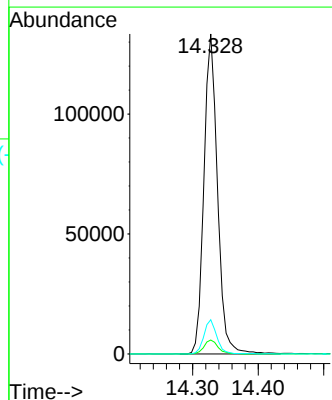
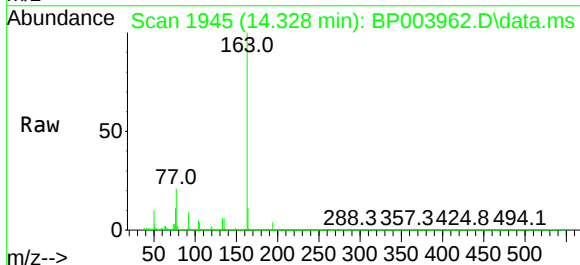




#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.639 min Scan# 2508
Delta R.T. -0.000 min
Lab File: BP003962.D
Acq: 13 Nov 2020 19:32




Instrument :
BNA_P
ClientSampleId :
TP-3-D


Tgt Ion:188 Resp: 597340
Ion Ratio Lower Upper
188 100
94 7.9 6.2 9.2
80 9.6 6.2 9.2#

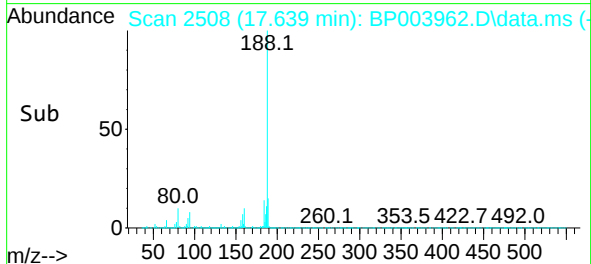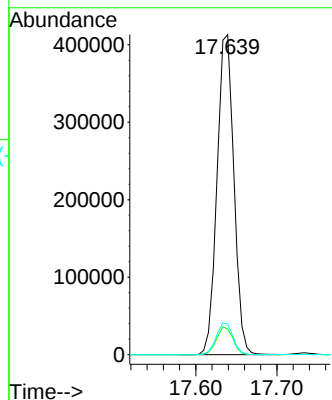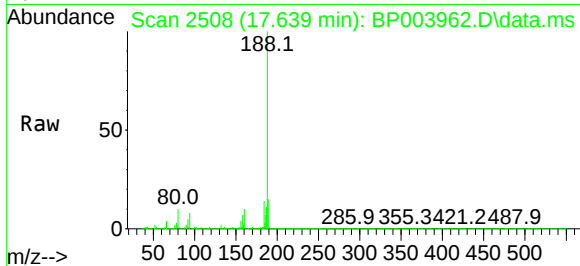

#76
Chrysene-d12
Concen: 20.00 ng
RT: 21.668 min Scan# 3193
Delta R.T. -0.006 min
Lab File: BP003962.D
Acq: 13 Nov 2020 19:32

Tgt Ion:240 Resp: 537998
Ion Ratio Lower Upper
240 100
120 9.2 7.8 11.6
236 25.4 20.8 31.2


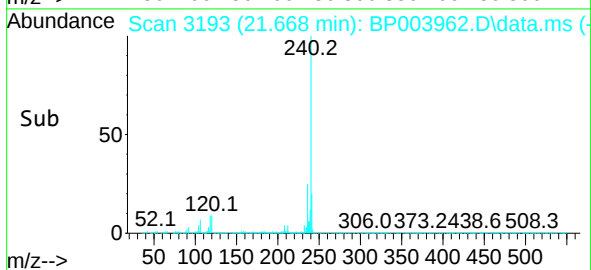
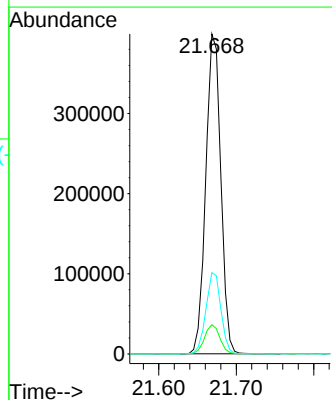
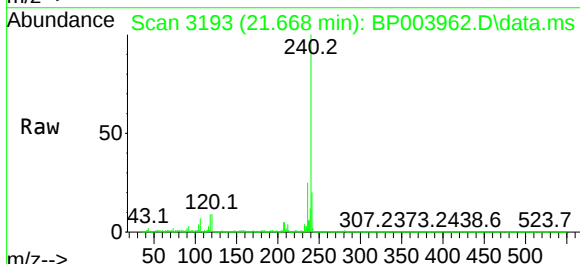




#79
 Terphenyl-d14
 Concen: 77.48 ng
 RT: 20.133 min Scan# 2932
 Delta R.T. -0.000 min
 Lab File: BP003962.D
 Acq: 13 Nov 2020 19:32

Instrument :
 BNA_P
 ClientSampled :
 TP-3-D

Tgt Ion:244 Resp: 2157668
 Ion Ratio Lower Upper
 244 100
 212 7.5 5.8 8.6
 122 9.8 7.8 11.8

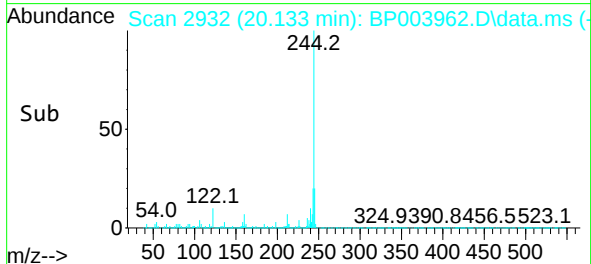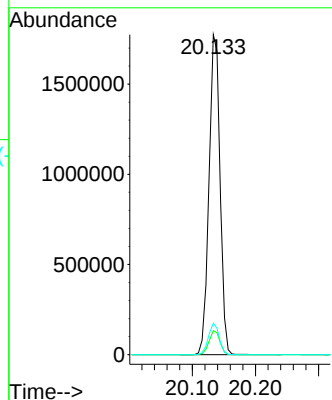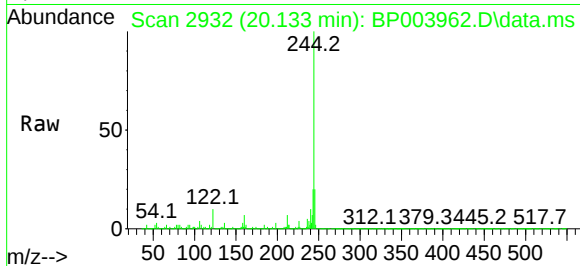

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 24.157 min Scan# 3616
 Delta R.T. -0.000 min
 Lab File: BP003962.D
 Acq: 13 Nov 2020 19:32

Tgt Ion:264 Resp: 544072
 Ion Ratio Lower Upper
 264 100
 260 22.8 18.8 28.2
 265 22.3 17.4 26.2

