

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP111320\  
 Data File : BP003952.D  
 Acq On : 13 Nov 2020 13:39  
 Operator : CG/JU  
 Sample : PB132989BL  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 PB132989BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\8270-BP110320.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP003952.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 3.081       | 27            | 33          | 44           | rVB3     | 47635          | 105494        | 1.00%           | 0.237%        |
| 2         | 4.293       | 234           | 239         | 247          | rBV      | 85968          | 123952        | 1.18%           | 0.279%        |
| 3         | 5.805       | 487           | 496         | 506          | rBV      | 2178435        | 3191387       | 30.36%          | 7.174%        |
| 4         | 7.452       | 768           | 776         | 791          | rBV      | 2011504        | 3219004       | 30.62%          | 7.236%        |
| 5         | 8.281       | 909           | 917         | 925          | rBV      | 550401         | 864247        | 8.22%           | 1.943%        |
| 6         | 8.622       | 966           | 975         | 983          | rBV      | 2755436        | 4501178       | 42.82%          | 10.118%       |
| 7         | 9.446       | 1106          | 1115        | 1124         | rBV      | 2215021        | 3642556       | 34.65%          | 8.188%        |
| 8         | 11.116      | 1390          | 1399        | 1408         | rBV      | 666369         | 1122025       | 10.67%          | 2.522%        |
| 9         | 13.528      | 1798          | 1809        | 1833         | rBV      | 5275174        | 7598308       | 72.28%          | 17.080%       |
| 10        | 14.904      | 2036          | 2043        | 2058         | rBV2     | 939850         | 1443000       | 13.73%          | 3.244%        |
| 11        | 16.387      | 2288          | 2295        | 2313         | rBV      | 2003847        | 3063637       | 29.14%          | 6.887%        |
| 12        | 17.639      | 2501          | 2508        | 2520         | rBV      | 1225390        | 1725815       | 16.42%          | 3.879%        |
| 13        | 20.139      | 2927          | 2933        | 2938         | rBV      | 8673794        | 10512431      | 100.00%         | 23.630%       |
| 14        | 21.675      | 3188          | 3194        | 3199         | rBV      | 1240471        | 1706332       | 16.23%          | 3.836%        |
| 15        | 24.157      | 3609          | 3616        | 3624         | rVB      | 812352         | 1667809       | 15.87%          | 3.749%        |




Sum of corrected areas: 44487175

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP111320\  
Data File : BP003952.D  
Acq On : 13 Nov 2020 13:39  
Operator : CG/JU  
Sample : PB132989BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
PB132989BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\8270-BP110320.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

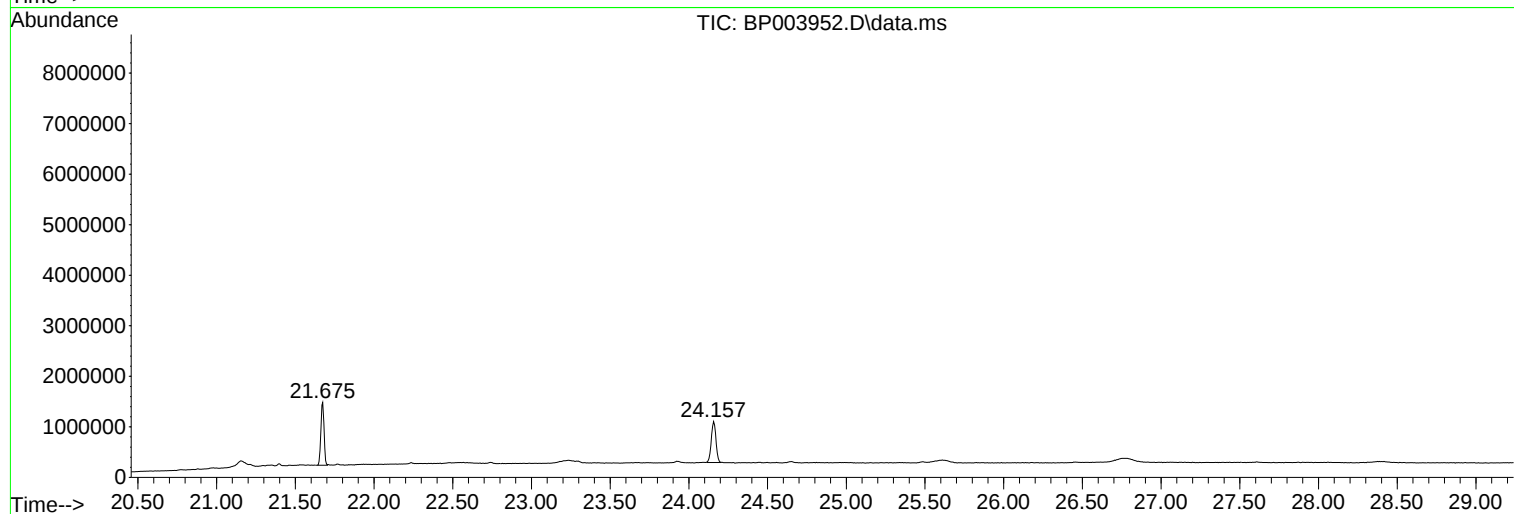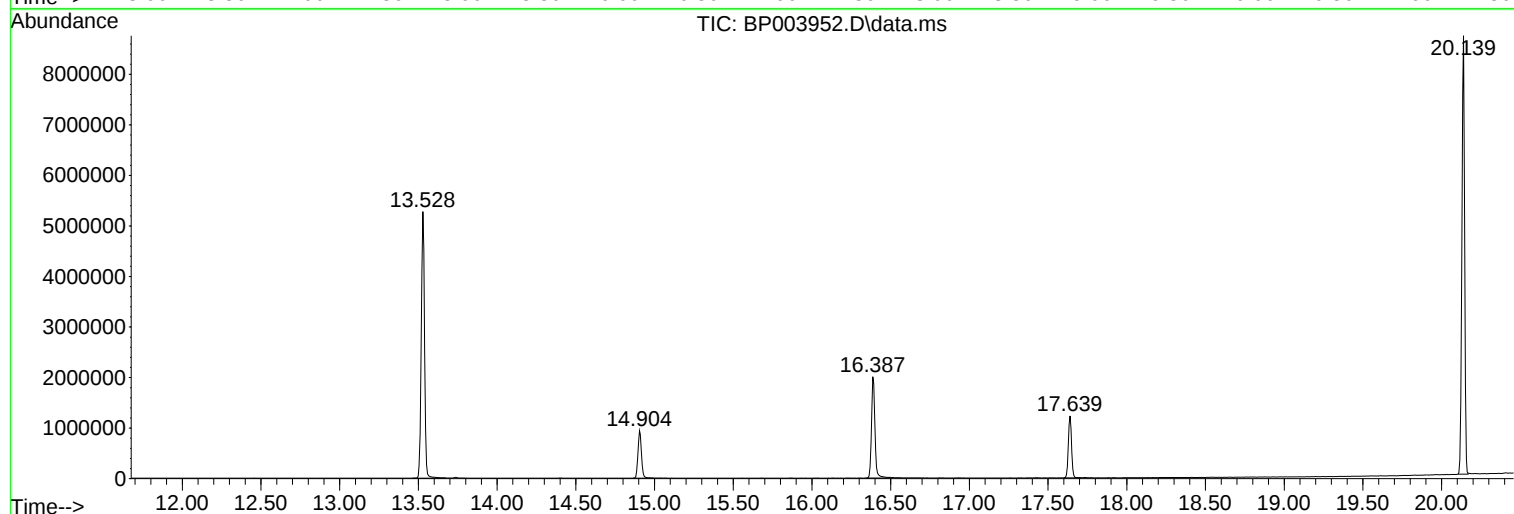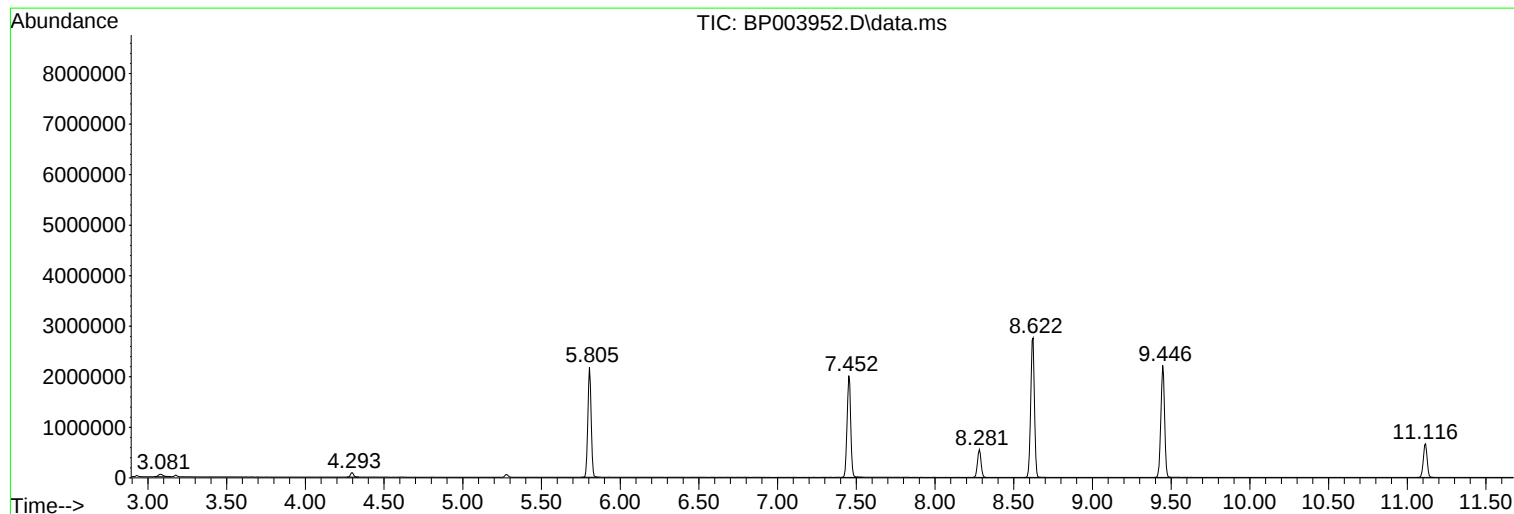

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP111320\  
Data File : BP003952.D  
Acq On : 13 Nov 2020 13:39  
Operator : CG/JU  
Sample : PB132989BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
PB132989BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\8270-BP110320.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP111320\  
Data File : BP003952.D  
Acq On : 13 Nov 2020 13:39  
Operator : CG/JU  
Sample : PB132989BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
PB132989BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\8270-BP110320.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|