
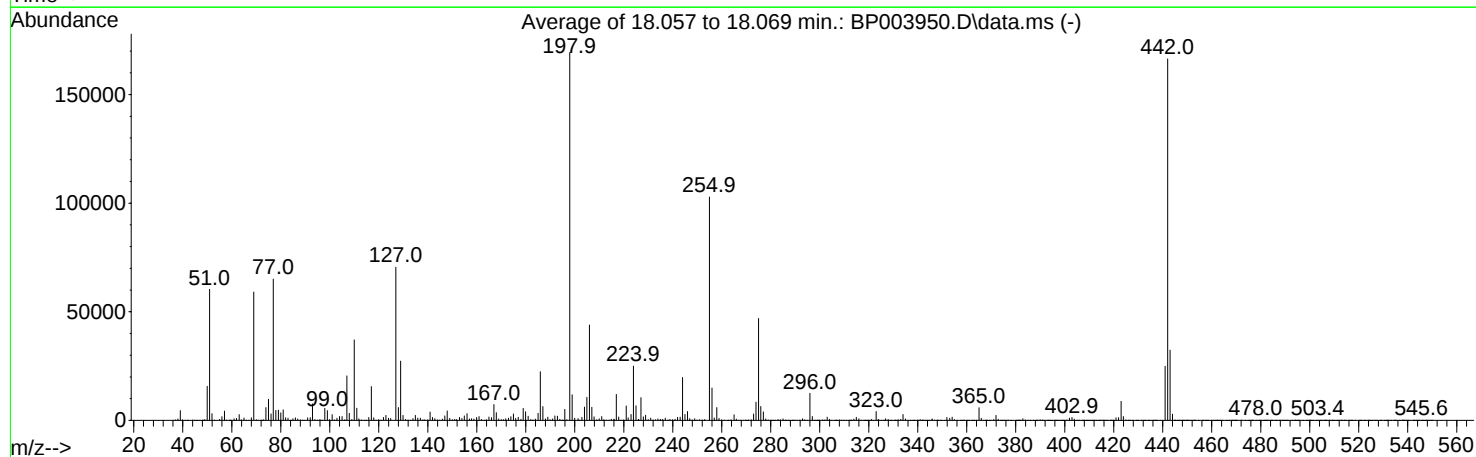


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111320\
 Data File : BP003950.D
 Acq On : 13 Nov 2020 12:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 12 15:22:47 2020

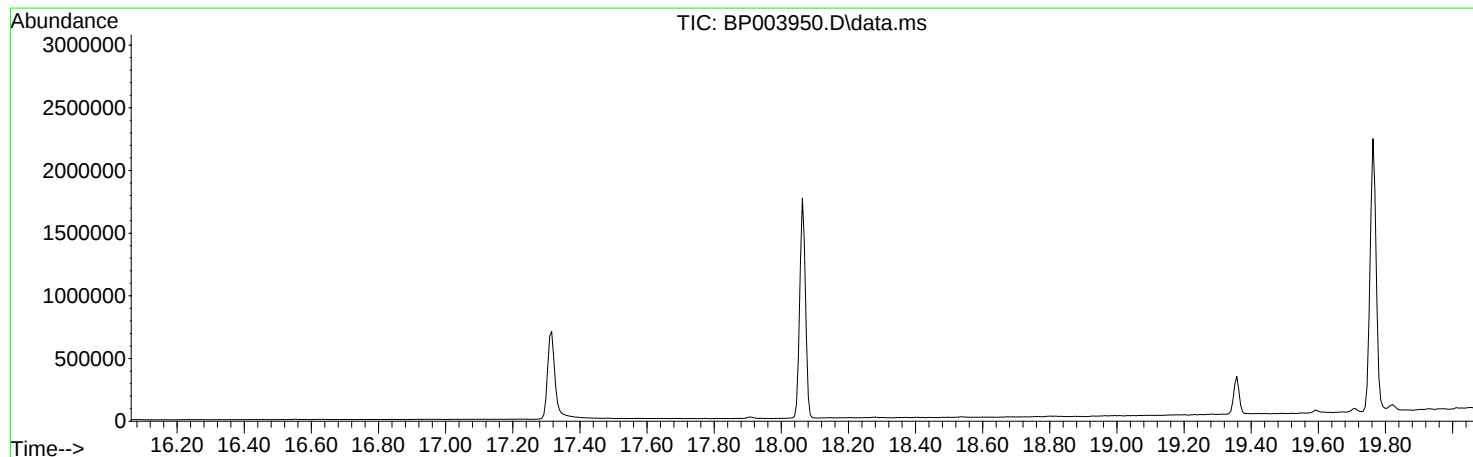

AutoFind: Scans 2579, 2580, 2581; Background Corrected with Scan 2566

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.6	60335	PASS
68	69	0.00	2	2.0	1156	PASS
69	198	0.00	100	34.9	59097	PASS
70	69	0.00	2	0.5	302	PASS
127	198	10	80	41.6	70525	PASS
197	198	0.00	2	0.2	282	PASS
198	198	100	100	100.0	169365	PASS
199	198	5	9	7.0	11831	PASS
275	198	10	60	27.7	46909	PASS
365	198	1	100	3.4	5799	PASS
441	198	0.01	100	14.7	24875	PASS
442	198	50	100	98.2	166395	PASS
443	442	15	24	19.5	32376	PASS