

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111323\
 Data File : BP018132.D
 Acq On : 13 Nov 2023 15:44
 Operator : MA/JU
 Sample : PB157055BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK055

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018132.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.164	10	13	22	rVB	22515	30347	1.54%	0.148%
2	3.605	84	88	110	rBV	124004	270241	13.69%	1.319%
3	3.899	136	138	143	rVB6	4570	4020	0.20%	0.020%
4	4.305	202	207	215	rBV	6205	11839	0.60%	0.058%
5	4.505	240	241	246	rVB5	2515	2385	0.12%	0.012%
6	4.652	263	266	269	rVB5	1734	2457	0.12%	0.012%
7	4.822	293	295	299	rBV5	1328	2012	0.10%	0.010%
8	5.022	326	329	331	rBV4	1578	2247	0.11%	0.011%
9	5.216	360	362	366	rVB5	2093	2371	0.12%	0.012%
10	6.258	537	539	543	rVB5	1915	2676	0.14%	0.013%
11	6.569	589	592	596	rBV6	1471	2580	0.13%	0.013%
12	6.752	618	623	628	rBV3	8663	14199	0.72%	0.069%
13	6.958	651	658	676	rBV	294148	533688	27.04%	2.605%
14	7.140	683	689	700	rBV	262451	406513	20.60%	1.984%
15	7.311	712	718	734	rBV	328304	554574	28.10%	2.707%
16	7.793	793	800	810	rBV	268460	455806	23.09%	2.225%
17	7.958	826	828	831	rBV4	1732	2278	0.12%	0.011%
18	8.516	917	923	941	rBV	355392	657770	33.33%	3.211%
19	8.999	999	1005	1024	rBV	312188	551873	27.96%	2.694%
20	9.175	1031	1035	1040	rVB4	3605	5384	0.27%	0.026%
21	9.340	1062	1063	1068	rVB5	1806	2165	0.11%	0.011%
22	9.710	1119	1126	1144	rBV	272881	504888	25.58%	2.465%
23	9.822	1144	1145	1151	rVB6	1622	2195	0.11%	0.011%
24	10.240	1208	1216	1236	rBV	301558	661851	33.53%	3.231%
25	10.610	1272	1279	1290	rVB	398549	644341	32.65%	3.145%
26	10.793	1304	1310	1329	rBV	226296	518927	26.29%	2.533%
27	11.028	1348	1350	1356	rVB7	1746	2244	0.11%	0.011%
28	11.599	1440	1447	1448	rBV7	2536	3802	0.19%	0.019%
29	12.228	1550	1554	1562	rBV10	3915	10001	0.51%	0.049%
30	12.440	1587	1590	1592	rBV4	1467	1992	0.10%	0.010%
31	12.469	1592	1595	1605	rVV	9819	20302	1.03%	0.099%
32	12.651	1621	1626	1633	rVB4	3876	6703	0.34%	0.033%
33	13.316	1734	1739	1746	rVB9	4878	10305	0.52%	0.050%
34	13.581	1778	1784	1788	rBV5	4010	6963	0.35%	0.034%
35	13.787	1813	1819	1822	rBV8	1119	2015	0.10%	0.010%
36	13.898	1830	1838	1850	rBV	816500	1164546	59.00%	5.685%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111323\
 Data File : BP018132.D
 Acq On : 13 Nov 2023 15:44
 Operator : MA/JU
 Sample : PB157055BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK055

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

37	14.087	1863	1870	1875	rVB10	2953	5850	0.30%	0.029%
38	14.175	1877	1885	1897	rBV	802480	1198688	60.73%	5.851%
39	14.316	1903	1909	1914	rVB7	5466	9517	0.48%	0.046%
40	14.475	1928	1936	1947	rBV	598500	878219	44.50%	4.287%
41	14.745	1976	1982	1997	rBV	104513	322338	16.33%	1.574%
42	15.104	2040	2043	2047	rVB6	3813	4788	0.24%	0.023%
43	15.216	2059	2062	2067	rBV4	5382	7608	0.39%	0.037%
44	15.257	2067	2069	2073	rVB5	1951	2315	0.12%	0.011%
45	15.475	2098	2106	2116	rBV	1067791	1534927	77.77%	7.493%
46	15.645	2129	2135	2145	rBV	106489	237867	12.05%	1.161%
47	15.875	2172	2174	2181	rVB8	2999	4068	0.21%	0.020%
48	16.187	2221	2227	2229	rBV6	1835	2915	0.15%	0.014%
49	16.269	2239	2241	2245	rVB5	1556	2279	0.12%	0.011%
50	16.369	2254	2258	2260	rVB4	2003	2285	0.12%	0.011%
51	16.504	2276	2281	2283	rBV6	2082	3150	0.16%	0.015%
52	16.622	2300	2301	2306	rBV5	1828	2177	0.11%	0.011%
53	16.769	2323	2326	2328	rVB4	1617	1999	0.10%	0.010%
54	16.922	2349	2352	2357	rVB7	2865	3896	0.20%	0.019%
55	17.122	2384	2386	2388	rBV3	2792	2682	0.14%	0.013%
56	17.257	2403	2409	2419	rBV	810230	1097904	55.63%	5.360%
57	17.357	2420	2426	2443	rVV2	1183723	1712354	86.76%	8.359%
58	17.833	2503	2507	2509	rBV5	2405	2962	0.15%	0.014%
59	17.886	2514	2516	2518	rBV3	2945	3239	0.16%	0.016%
60	17.957	2524	2528	2529	rBV4	2589	2776	0.14%	0.014%
61	18.392	2599	2602	2603	rBV3	2077	2345	0.12%	0.011%
62	18.669	2645	2649	2655	rBV8	5088	10146	0.51%	0.050%
63	19.186	2732	2737	2742	rBV5	17338	24338	1.23%	0.119%
64	19.263	2746	2750	2755	rVB2	14475	20202	1.02%	0.099%
65	19.616	2804	2810	2826	rBV	1490385	1973681	100.00%	9.635%
66	20.545	2965	2968	2972	rVB3	25160	27466	1.39%	0.134%
67	21.174	3073	3075	3080	rVB4	26636	28017	1.42%	0.137%
68	21.392	3107	3112	3121	rBV	844889	1166677	59.11%	5.695%
69	21.727	3166	3169	3174	rBV3	47955	64751	3.28%	0.316%
70	23.698	3498	3504	3513	rVB2	956689	1894173	95.97%	9.247%
71	23.868	3526	3533	3544	rVB	534392	1148085	58.17%	5.604%




Sum of corrected areas: 20485184

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111323\
Data File : BP018132.D
Acq On : 13 Nov 2023 15:44
Operator : MA/JU
Sample : PB157055BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK055

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

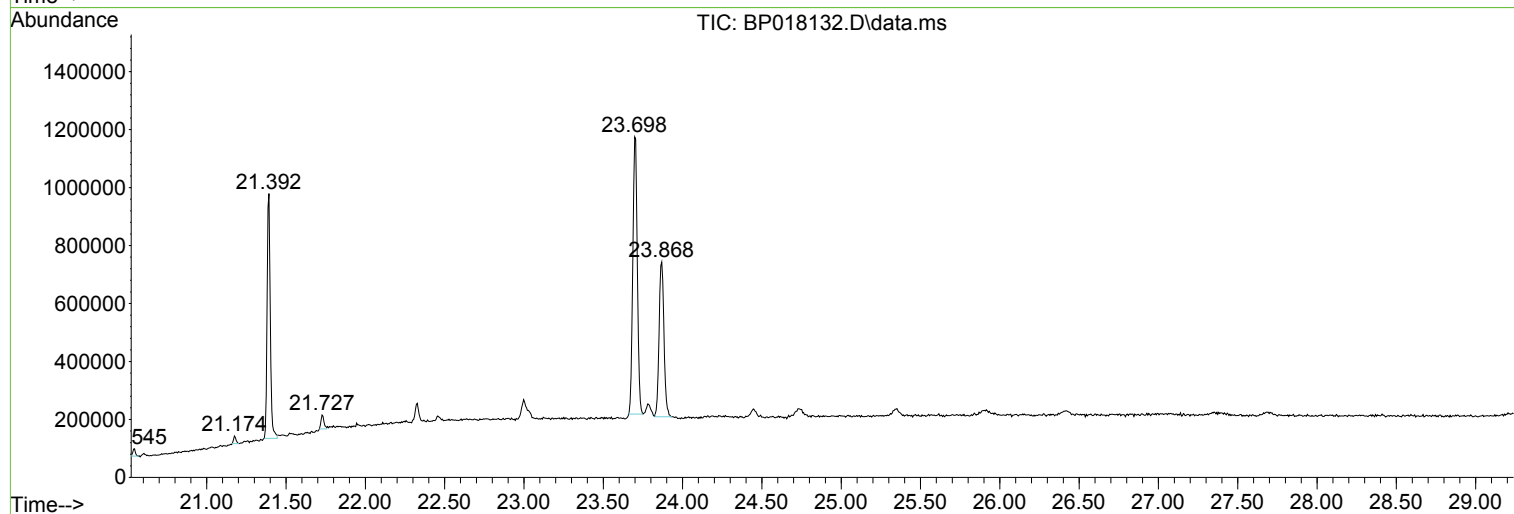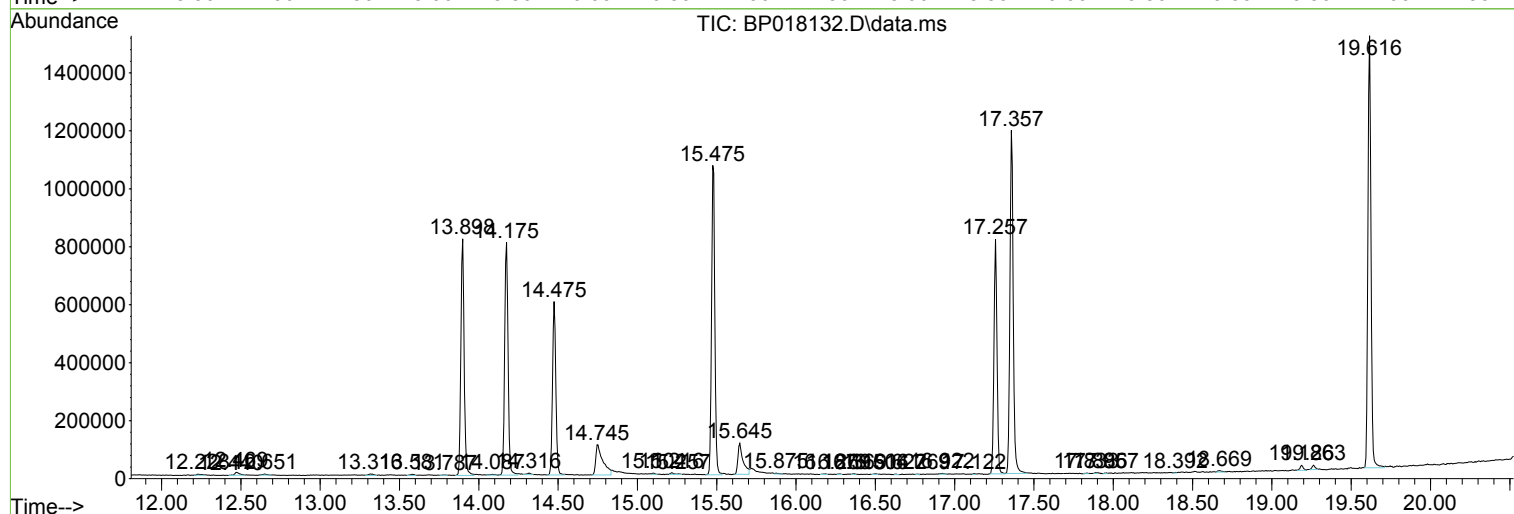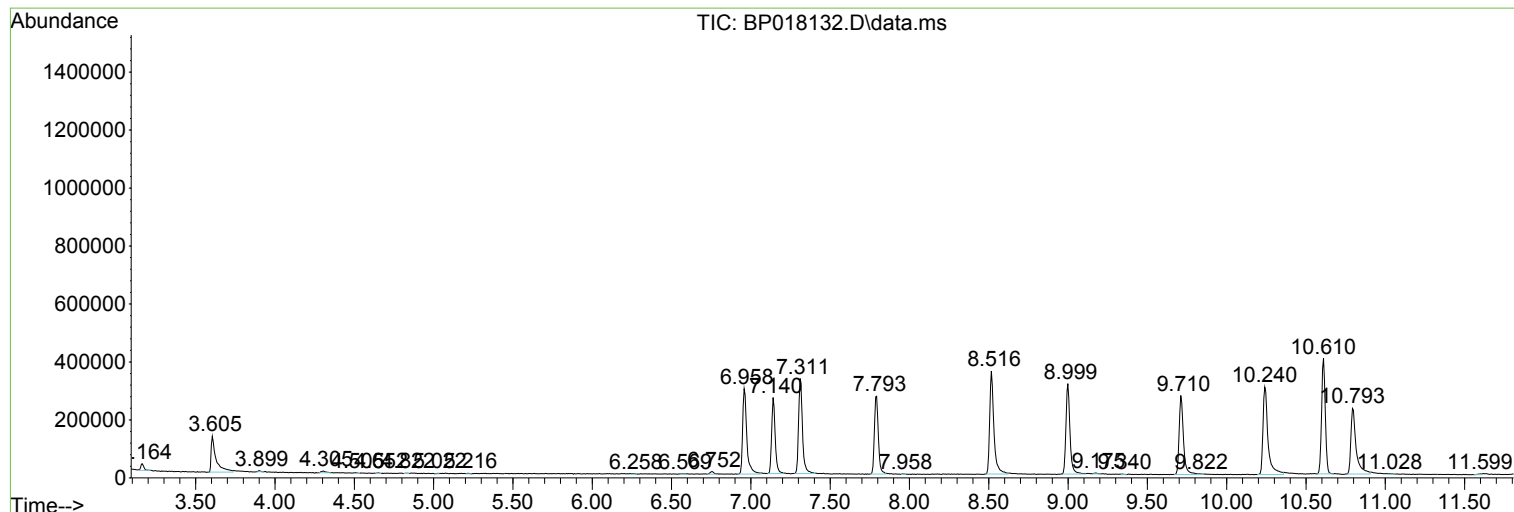

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111323\
Data File : BP018132.D
Acq On : 13 Nov 2023 15:44
Operator : MA/JU
Sample : PB157055BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK055

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111323\
Data File : BP018132.D
Acq On : 13 Nov 2023 15:44
Operator : MA/JU
Sample : PB157055BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK055

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc