

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111325\
Data File : BP026127.D
Acq On : 13 Nov 2025 14:05
Operator : RC/JU
Sample : PB170500BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB170500BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP026127.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.267	389	396	409	rBV	4742627	7039928	48.19%	10.944%
2	6.825	653	661	671	rBV	4277982	6792022	46.49%	10.559%
3	7.655	794	802	810	rVB	843660	1419178	9.71%	2.206%
4	8.796	988	996	1009	rBV	2820927	4342830	29.73%	6.751%
5	10.431	1266	1274	1288	rBV	1045855	1841560	12.61%	2.863%
6	12.913	1686	1696	1706	rBV	6109849	9721484	66.55%	15.113%
7	14.307	1921	1933	1940	rBV	1481896	2268796	15.53%	3.527%
8	15.831	2185	2192	2210	rBV	4937318	6817187	46.67%	10.598%
9	17.125	2405	2412	2424	rBV	1854541	2622267	17.95%	4.077%
10	19.878	2873	2880	2887	rBV	9331553	14608614	100.00%	22.710%
11	21.583	3164	3170	3182	rVB	2143526	3233181	22.13%	5.026%
12	24.924	3729	3738	3752	rVB	1354225	3619350	24.78%	5.627%




Sum of corrected areas: 64326397

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111325\
Data File : BP026127.D
Acq On : 13 Nov 2025 14:05
Operator : RC/JU
Sample : PB170500BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB170500BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

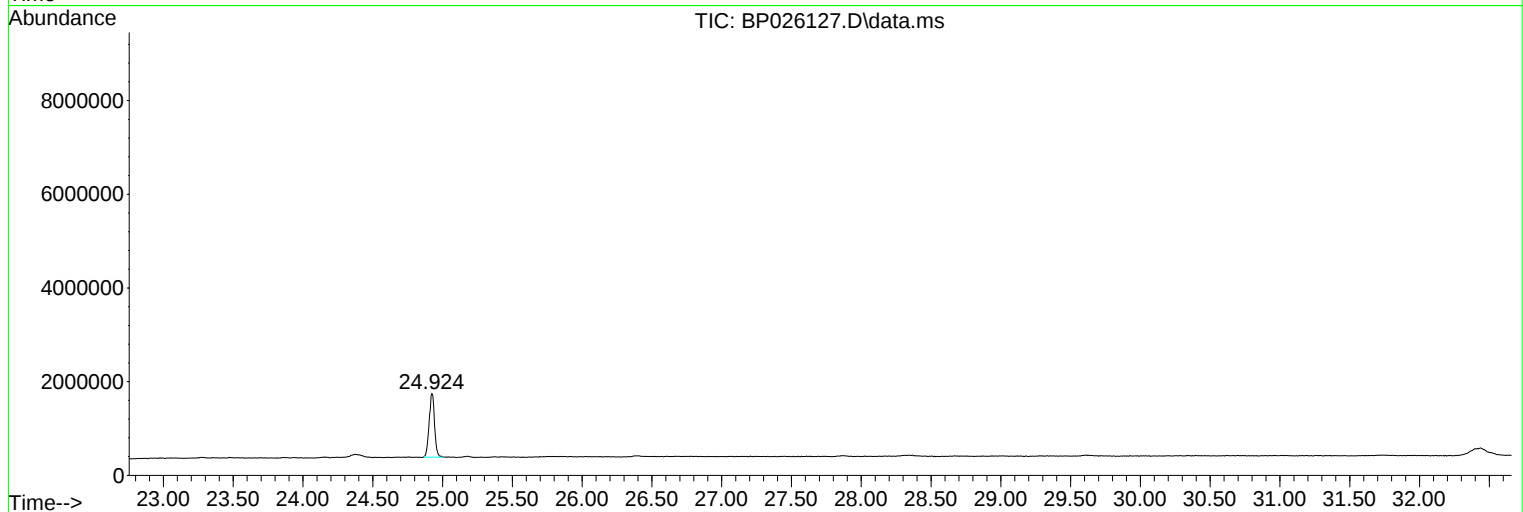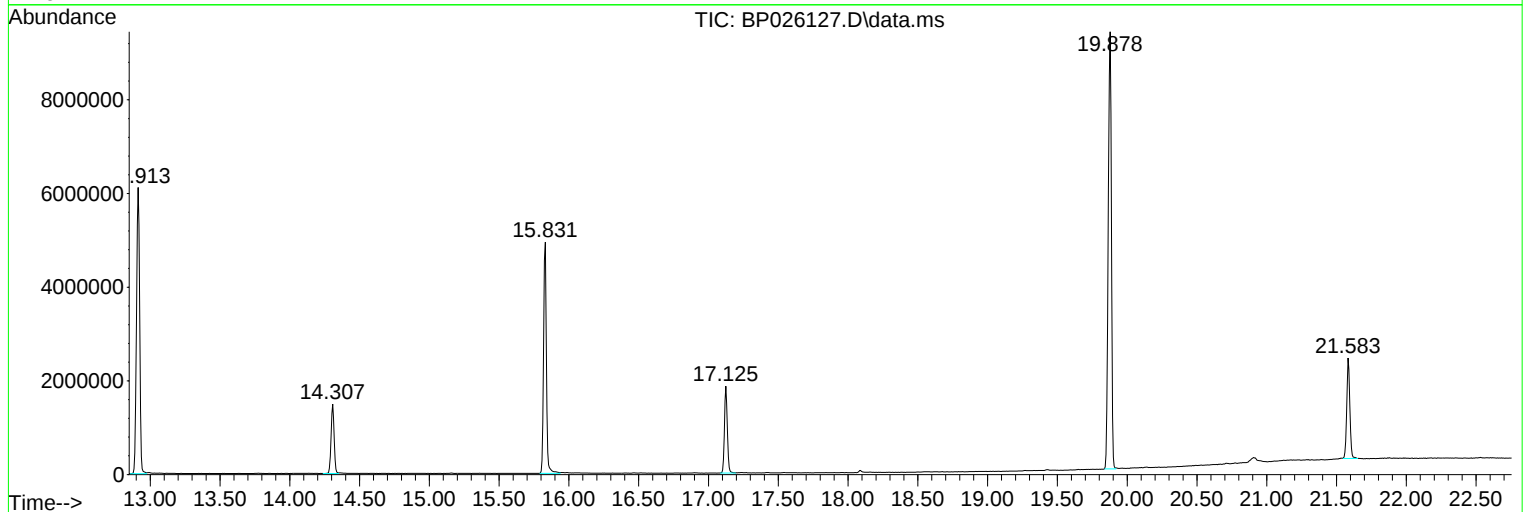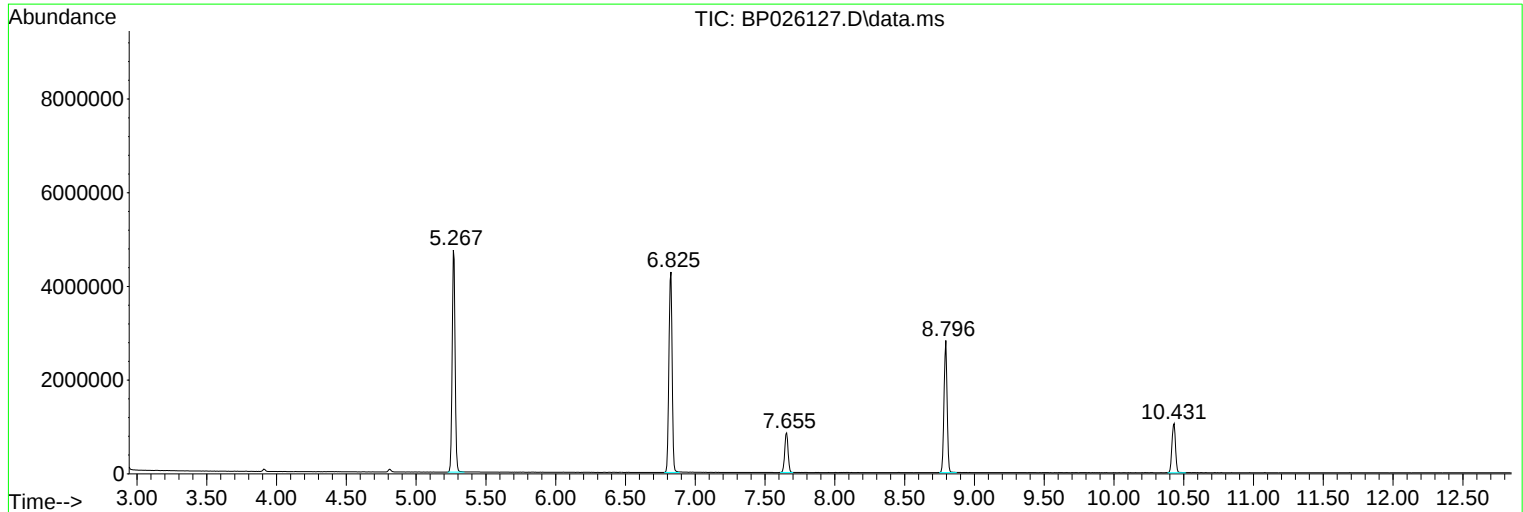

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111325\
Data File : BP026127.D
Acq On : 13 Nov 2025 14:05
Operator : RC/JU
Sample : PB170500BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB170500BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111325\
Data File : BP026127.D
Acq On : 13 Nov 2025 14:05
Operator : RC/JU
Sample : PB170500BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB170500BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------