




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111423\
 Data File : BP018158.D
 Acq On : 14 Nov 2023 16:43
 Operator : MA/JU
 Sample : PB157059BL
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK059

Manual IntegrationsAPPROVED

Quant Time: Nov 15 00:39:11 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 13 15:50:18 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/16/2023
 Supervised By :mohammad ahmed 11/16/2023

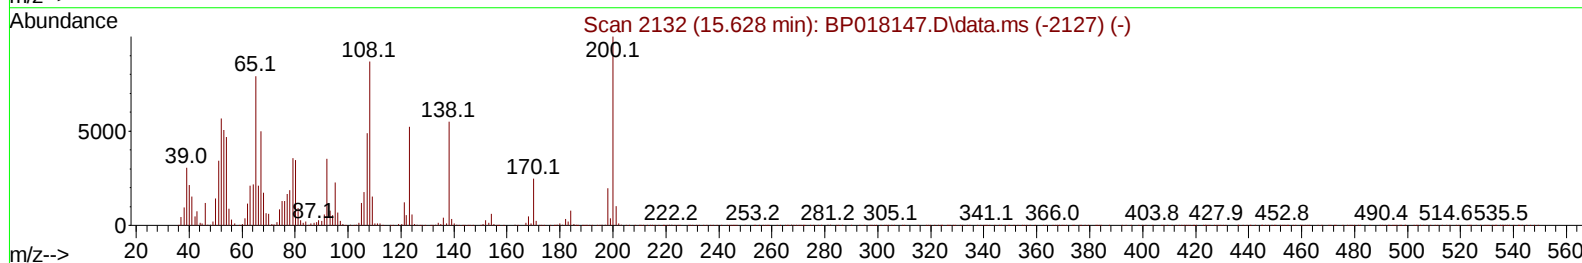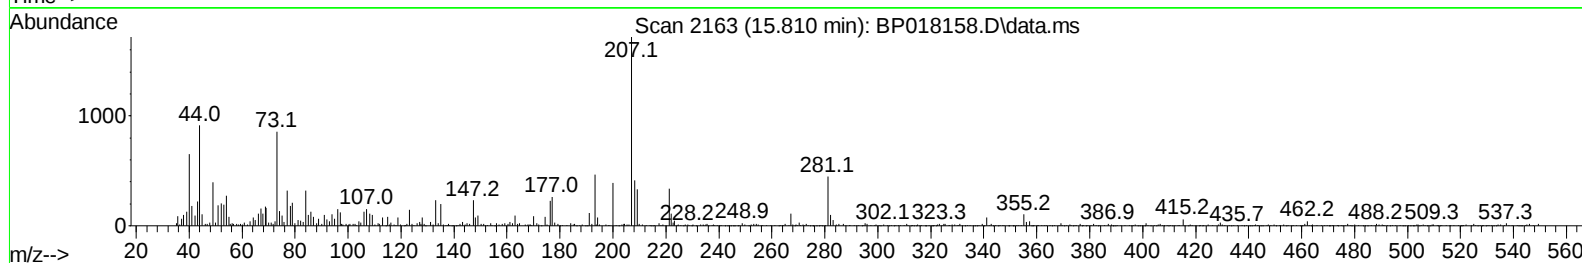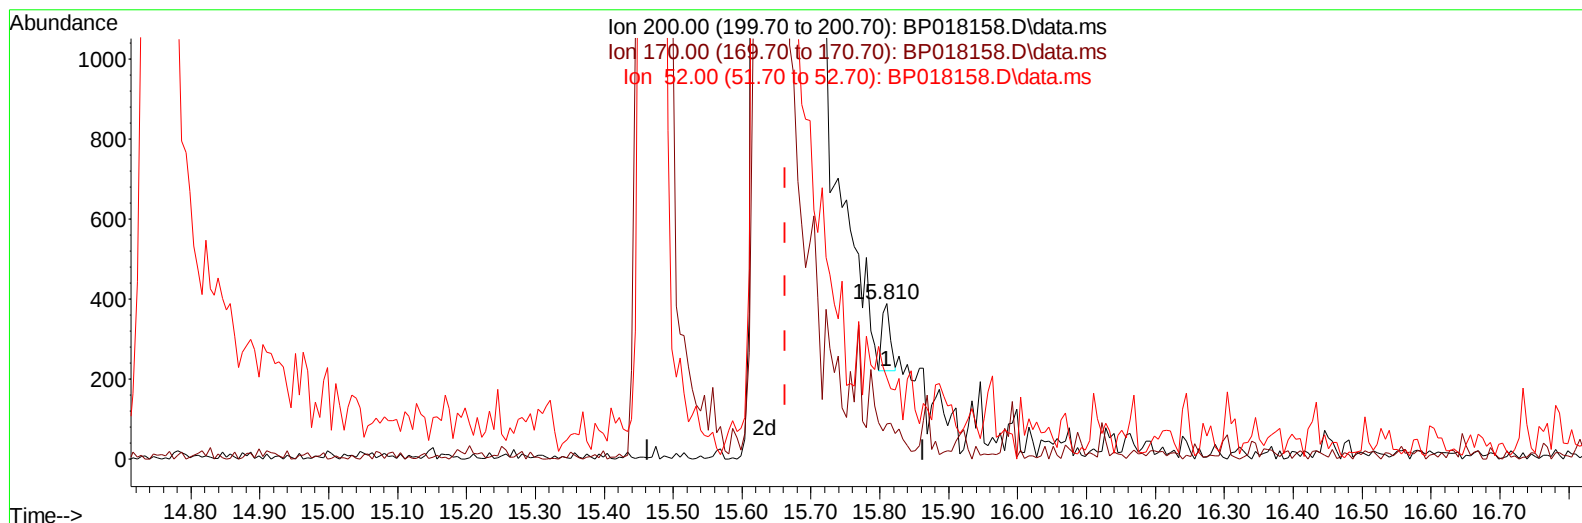

TIC: BP018158.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.810min (+ 0.147) 0.04 ng/ul

response 140

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	23.60	22.88
52.00	52.00	52.44
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111423\
 Data File : BP018158.D
 Acq On : 14 Nov 2023 16:43
 Operator : MA/JU
 Sample : PB157059BL
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK059

Manual IntegrationsAPPROVED

Quant Time: Nov 15 00:39:11 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 13 15:50:18 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/16/2023
 Supervised By :mohammad ahmed 11/16/2023

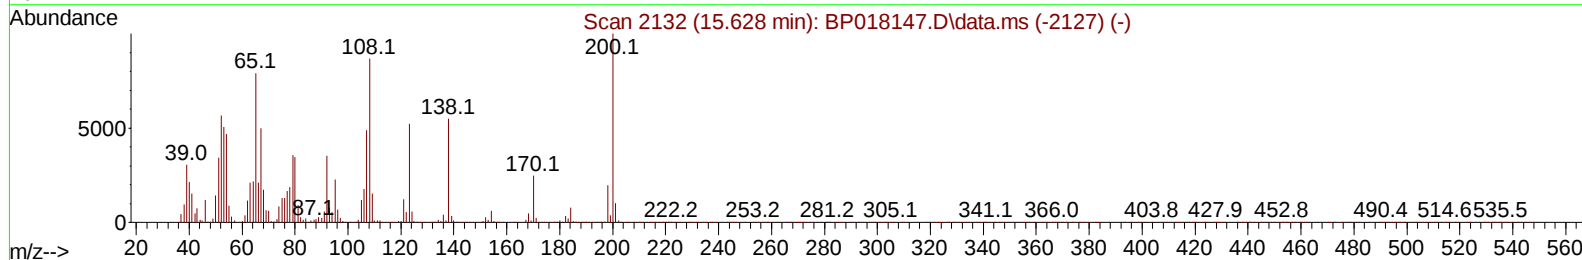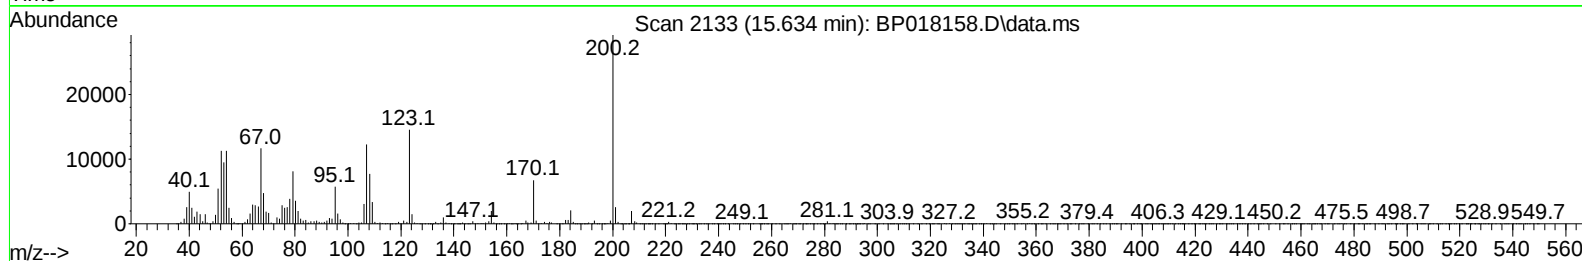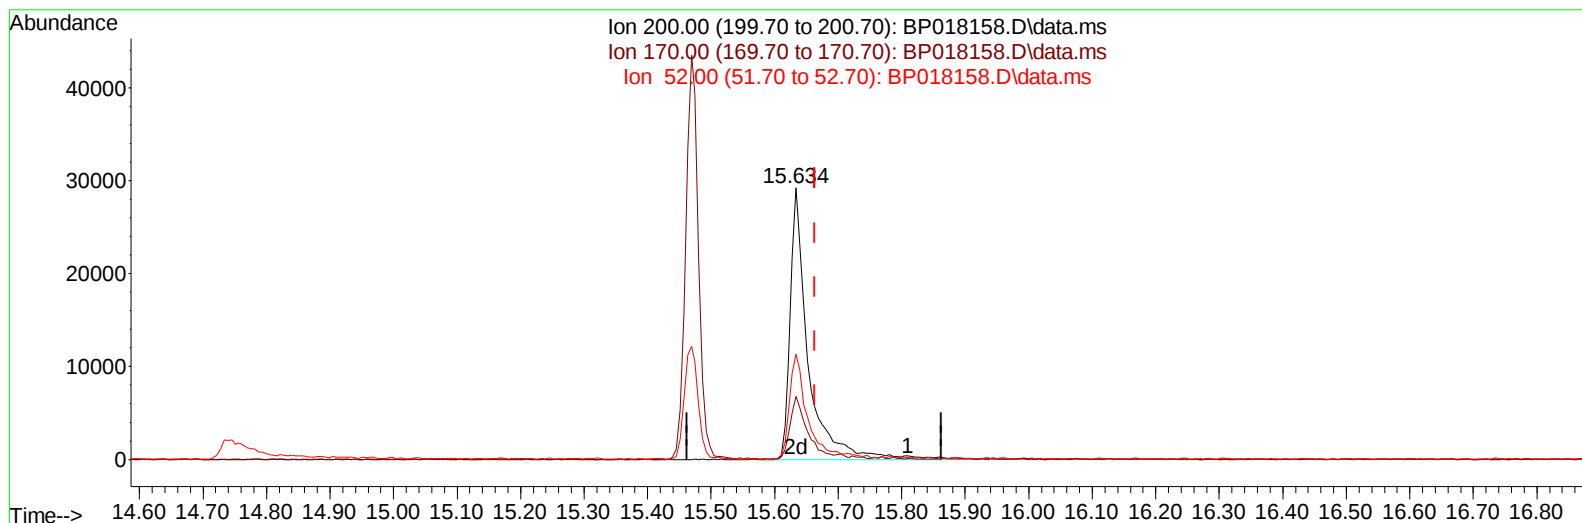

TIC: BP018158.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.634min (-0.029) 14.82 ng/ul m

response 57046

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	23.60	23.21
52.00	52.00	38.82#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111423\
 Data File : BP018158.D
 Acq On : 14 Nov 2023 16:43
 Operator : MA/JU
 Sample : PB157059BL
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK059

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/16/2023
 Supervised By :mohammad ahmed 11/16/2023

Quant Time: Nov 15 01:22:44 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 13 15:50:18 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.787	152	80234	20.000	ng/ul	0.00
20) Naphthalene-d8	10.604	136	378163	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.469	164	239839	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.245	188	532493	20.000	ng/ul	#-0.01
79) Chrysene-d12	21.380	240	462209	20.000	ng/ul	-0.01
88) Perylene-d12	23.851	264	479074	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	12680	5.575	ng/uL	0.00
4) Pyridine-d5	3.599	84	108798	18.346	ng/ul	0.00
7) Phenol-d5	6.952	99	189548	24.470	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.140	67	129817	28.518	ng/ul	0.00
11) 2-Chlorophenol-d4	7.311	132	153696	25.056	ng/ul	0.00
15) 4-Methylphenol-d8	8.510	113	153243	24.143	ng/ul	0.00
21) Nitrobenzene-d5	8.993	128	75961	22.295	ng/ul	0.00
24) 2-Nitrophenol-d4	9.710	143	94836	24.570	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.234	165	150335	21.853	ng/ul	0.00
31) 4-Chloroaniline-d4	10.793	131	180028	19.082	ng/ul	0.00
46) Dimethylphthalate-d6	13.893	166	598829	27.060	ng/ul	0.00
49) Acenaphthylene-d8	14.169	160	606353	25.157	ng/ul	0.00
54) 4-Nitrophenol-d4	14.740	143	43164	13.053	ng/ul	0.00
60) Fluorene-d10	15.469	176	489212	26.776	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.634	200	57046m	14.819	ng/ul	-0.03
73) Anthracene-d10	17.351	188	785087	27.261	ng/ul	0.00
81) Pyrene-d10	19.604	212	913559	29.590	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.686	264	786279	28.226	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111423\
Data File : BP018158.D
Acq On : 14 Nov 2023 16:43
Operator : MA/JU
Sample : PB157059BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK059

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/16/2023
Supervised By :mohammad ahmed 11/16/2023

Quant Time: Nov 15 01:22:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Nov 13 15:50:18 2023
Response via : Initial Calibration

