

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111423\
 Data File : BP018151.D
 Acq On : 14 Nov 2023 12:13
 Operator : MA/JU
 Sample : PB156906TB 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SLEB906

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018151.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.164	9	13	21	rVB	29815	39923	1.68%	0.176%
2	3.593	83	86	105	rBV	197906	374393	15.75%	1.653%
3	5.987	490	493	496	rBV5	1992	3210	0.14%	0.014%
4	6.128	513	517	520	rBV6	1510	2671	0.11%	0.012%
5	6.152	520	521	526	rVB5	2237	2761	0.12%	0.012%
6	6.952	651	657	675	rBV	365659	668344	28.12%	2.951%
7	7.140	683	689	701	rBV	326522	515755	21.70%	2.278%
8	7.310	711	718	730	rBV	399959	686849	28.90%	3.033%
9	7.534	754	756	761	rVB5	1967	3151	0.13%	0.014%
10	7.787	793	799	814	rBV	276584	467836	19.69%	2.066%
11	8.510	916	922	940	rBV	449082	824856	34.71%	3.642%
12	8.993	996	1004	1021	rBV	385880	688157	28.96%	3.039%
13	9.710	1119	1126	1144	rBV	281945	559898	23.56%	2.472%
14	10.234	1209	1215	1243	rBV	369793	803363	33.80%	3.548%
15	10.604	1271	1278	1289	rBV	392875	666568	28.05%	2.943%
16	10.787	1303	1309	1330	rBV	324623	736121	30.98%	3.251%
17	12.251	1554	1558	1559	rBV4	3648	5061	0.21%	0.022%
18	12.263	1559	1560	1565	rVB5	3799	4017	0.17%	0.018%
19	13.316	1737	1739	1746	rVB8	3438	4007	0.17%	0.018%
20	13.440	1755	1760	1763	rBV7	3087	4297	0.18%	0.019%
21	13.892	1829	1837	1852	rBV	784337	1172006	49.32%	5.175%
22	14.163	1877	1883	1903	rBV	808068	1233949	51.92%	5.449%
23	14.316	1907	1909	1913	rVB5	2070	2598	0.11%	0.011%
24	14.469	1928	1935	1948	rBV	500083	740762	31.17%	3.271%
25	14.739	1976	1981	2004	rBV2	81457	311049	13.09%	1.374%
26	14.881	2004	2005	2008	rVB3	3715	3232	0.14%	0.014%
27	15.469	2099	2105	2117	rBV	1100312	1569944	66.06%	6.933%
28	15.634	2128	2133	2146	rBV	166141	344161	14.48%	1.520%
29	17.251	2398	2408	2418	rBV	734734	1060203	44.61%	4.682%
30	17.351	2418	2425	2441	rVV	1354763	2011311	84.63%	8.882%
31	17.681	2480	2481	2485	rBV4	2135	2715	0.11%	0.012%
32	18.539	2626	2627	2632	rVB5	2994	3551	0.15%	0.016%
33	19.180	2732	2736	2740	rBV3	14911	19660	0.83%	0.087%
34	19.251	2744	2748	2757	rVV2	23209	39906	1.68%	0.176%
35	19.480	2783	2787	2791	rBV	49903	56476	2.38%	0.249%
36	19.604	2803	2808	2819	rBV	1786753	2312031	97.29%	10.210%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111423\
Data File : BP018151.D
Acq On : 14 Nov 2023 12:13
Operator : MA/JU
Sample : PB156906TB 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB906

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Title : SVOA CALIBRATION

37	20.510	2959	2962	2968	rBV2	39861	50100	2.11%	0.221%
38	21.380	3105	3110	3122	rBV	774547	1121098	47.17%	4.951%
39	23.686	3494	3502	3511	rBV2	1180940	2376498	100.00%	10.494%
40	23.851	3523	3530	3542	rVB	547894	1152958	48.51%	5.091%




Sum of corrected areas: 22645446

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111423\
Data File : BP018151.D
Acq On : 14 Nov 2023 12:13
Operator : MA/JU
Sample : PB156906TB 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB906

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

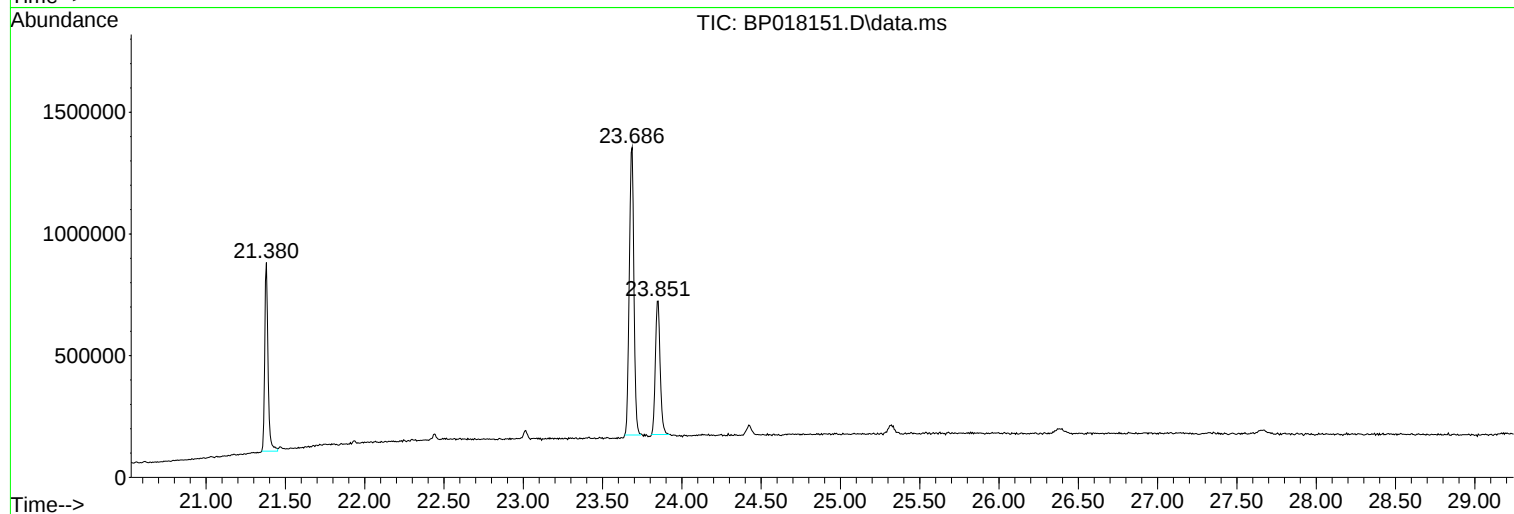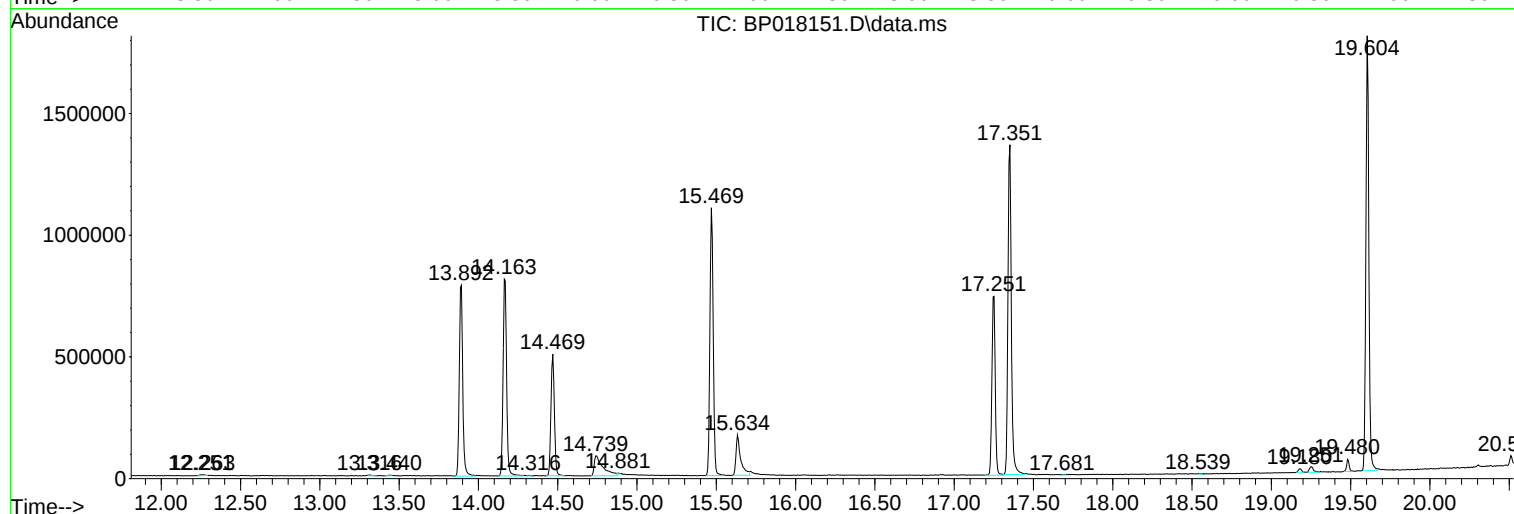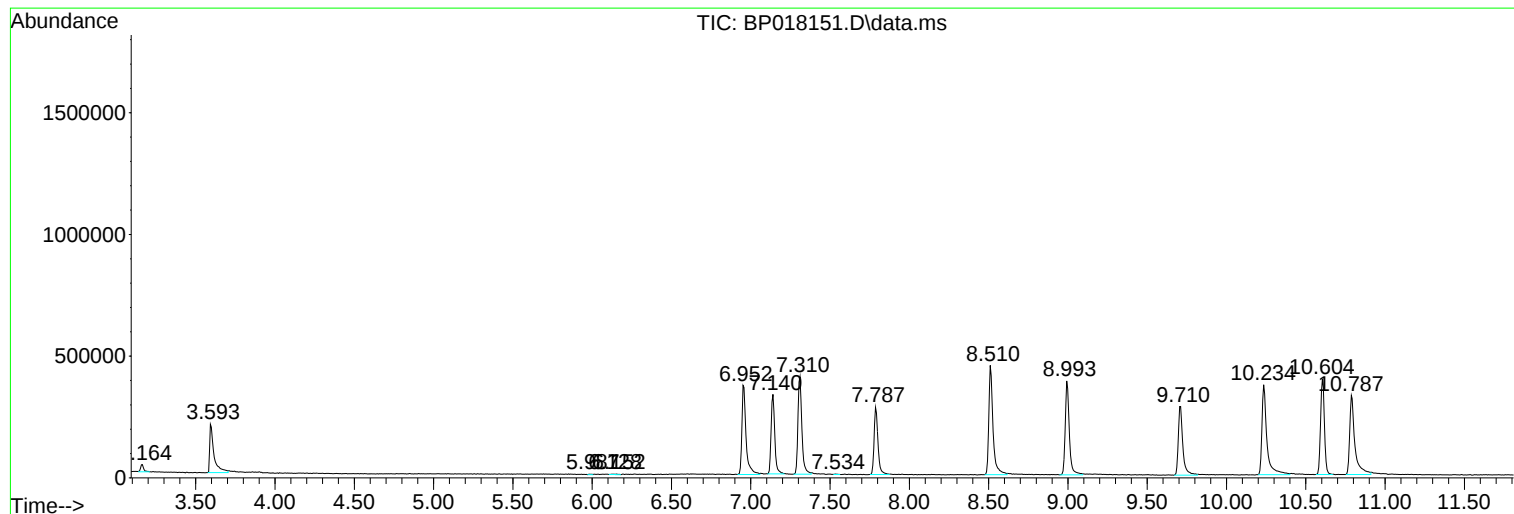

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111423\
Data File : BP018151.D
Acq On : 14 Nov 2023 12:13
Operator : MA/JU
Sample : PB156906TB 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB906

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111423\
Data File : BP018151.D
Acq On : 14 Nov 2023 12:13
Operator : MA/JU
Sample : PB156906TB 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB906

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc