

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111423\
 Data File : BP018152.D
 Acq On : 14 Nov 2023 12:47
 Operator : MA/JU
 Sample : PB156922BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK922

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018152.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.158	9	12	19	rVB	26788	33836	1.53%	0.157%
2	3.593	84	86	106	rBV	175117	356591	16.14%	1.655%
3	4.858	298	301	307	rVB8	1778	3564	0.16%	0.017%
4	6.905	646	649	652	rVB5	1876	2229	0.10%	0.010%
5	6.958	652	658	674	rBV	332891	626391	28.34%	2.907%
6	7.140	683	689	700	rBV	294753	464582	21.02%	2.156%
7	7.311	711	718	733	rBV	367080	641760	29.04%	2.978%
8	7.522	752	754	758	rVB5	2029	2771	0.13%	0.013%
9	7.787	793	799	815	rBV	252672	438756	19.85%	2.036%
10	8.510	916	922	940	rBV	405067	744441	33.68%	3.455%
11	8.993	996	1004	1022	rBV	343373	628677	28.45%	2.918%
12	9.363	1062	1067	1070	rBV7	1448	2389	0.11%	0.011%
13	9.599	1105	1107	1113	rVB7	1920	2376	0.11%	0.011%
14	9.710	1118	1126	1146	rVV	281025	540683	24.47%	2.509%
15	10.234	1205	1215	1234	rBV	325378	725110	32.81%	3.365%
16	10.605	1270	1278	1292	rVB	371163	604232	27.34%	2.804%
17	10.787	1303	1309	1327	rBV	287009	672837	30.44%	3.123%
18	11.881	1492	1495	1502	rVV9	1345	2889	0.13%	0.013%
19	12.263	1554	1560	1566	rBV7	3809	9666	0.44%	0.045%
20	13.316	1734	1739	1743	rVB8	3253	5590	0.25%	0.026%
21	13.410	1752	1755	1757	rBV4	2162	2251	0.10%	0.010%
22	13.451	1757	1762	1765	rVV6	2097	3541	0.16%	0.016%
23	13.681	1798	1801	1803	rBV3	1629	2223	0.10%	0.010%
24	13.893	1830	1837	1855	rBV	799670	1193589	54.01%	5.539%
25	14.169	1875	1884	1895	rBV	821821	1256619	56.86%	5.832%
26	14.469	1928	1935	1946	rBV	495023	721219	32.63%	3.347%
27	14.745	1976	1982	2002	rBV3	78717	305143	13.81%	1.416%
28	14.981	2020	2022	2028	rVB6	2383	3443	0.16%	0.016%
29	15.469	2099	2105	2116	rBV	1163111	1685032	76.25%	7.820%
30	15.634	2127	2133	2145	rBV	162210	340481	15.41%	1.580%
31	16.045	2201	2203	2206	rVB4	2077	2274	0.10%	0.011%
32	16.281	2242	2243	2246	rVB3	2608	2331	0.11%	0.011%
33	16.828	2329	2336	2339	rBV9	1225	3043	0.14%	0.014%
34	17.028	2367	2370	2372	rBV4	1826	2605	0.12%	0.012%
35	17.139	2385	2389	2391	rBV5	1650	2760	0.12%	0.013%
36	17.245	2399	2407	2418	rBV	687123	977191	44.22%	4.535%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111423\
 Data File : BP018152.D
 Acq On : 14 Nov 2023 12:47
 Operator : MA/JU
 Sample : PB156922BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK922

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

37	17.351	2418	2425	2443	rVV	1302195	1879037	85.02%	8.720%
38	17.892	2512	2517	2522	rVB9	1611	3315	0.15%	0.015%
39	18.128	2554	2557	2560	rBV5	2423	3824	0.17%	0.018%
40	18.169	2560	2564	2567	rVB6	2335	3661	0.17%	0.017%
41	18.275	2580	2582	2589	rVB8	2334	4321	0.20%	0.020%
42	18.510	2618	2622	2627	rVB7	1974	3742	0.17%	0.017%
43	19.181	2732	2736	2743	rBV4	15200	19667	0.89%	0.091%
44	19.251	2744	2748	2754	rVB4	17119	29146	1.32%	0.135%
45	19.410	2773	2775	2778	rVB4	3766	3594	0.16%	0.017%
46	19.486	2784	2788	2793	rBV2	33112	42703	1.93%	0.198%
47	19.604	2803	2808	2818	rBV	1684228	2194895	99.32%	10.186%
48	20.304	2925	2927	2930	rBV4	7390	7684	0.35%	0.036%
49	20.510	2959	2962	2966	rBV4	26459	30949	1.40%	0.144%
50	21.380	3105	3110	3121	rBV	725526	1031144	46.66%	4.785%
51	23.686	3494	3502	3511	rBV2	1108454	2210022	100.00%	10.256%
52	23.851	3523	3530	3541	rBV	489424	1066962	48.28%	4.952%




Sum of corrected areas: 21547781

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111423\
Data File : BP018152.D
Acq On : 14 Nov 2023 12:47
Operator : MA/JU
Sample : PB156922BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK922

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

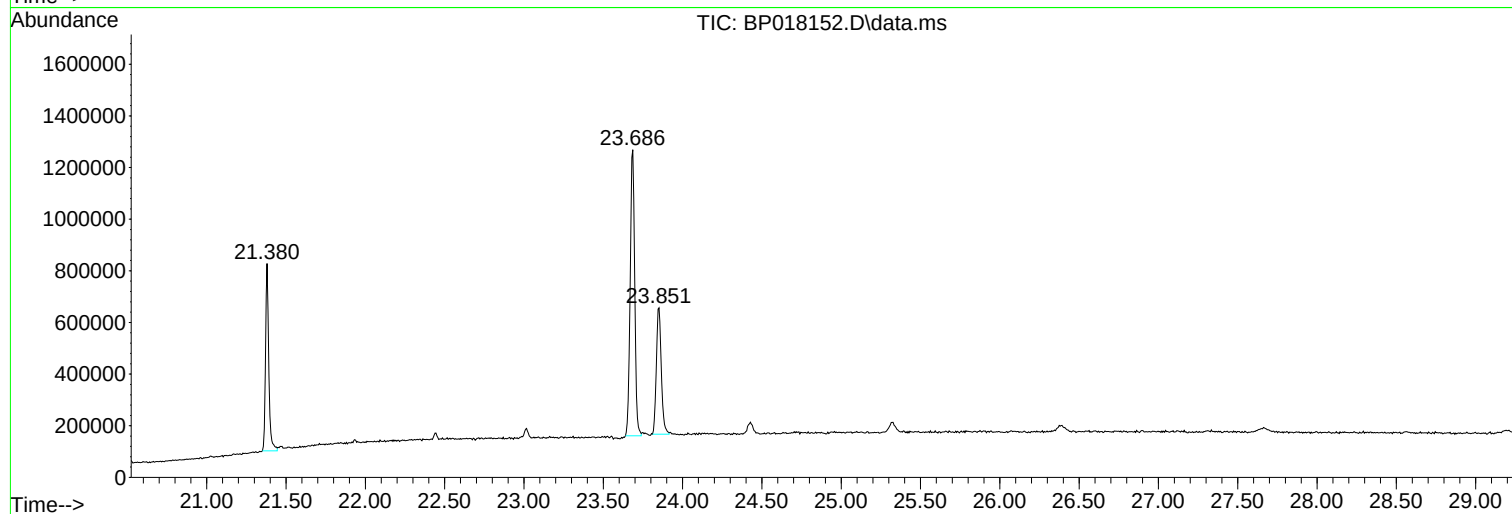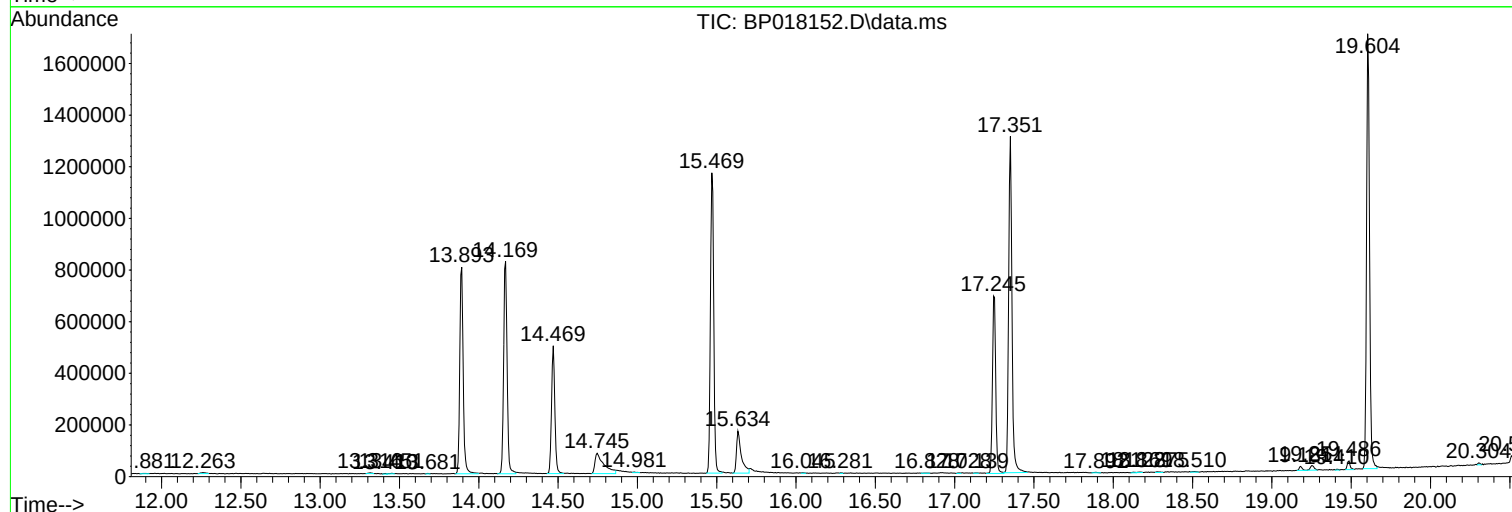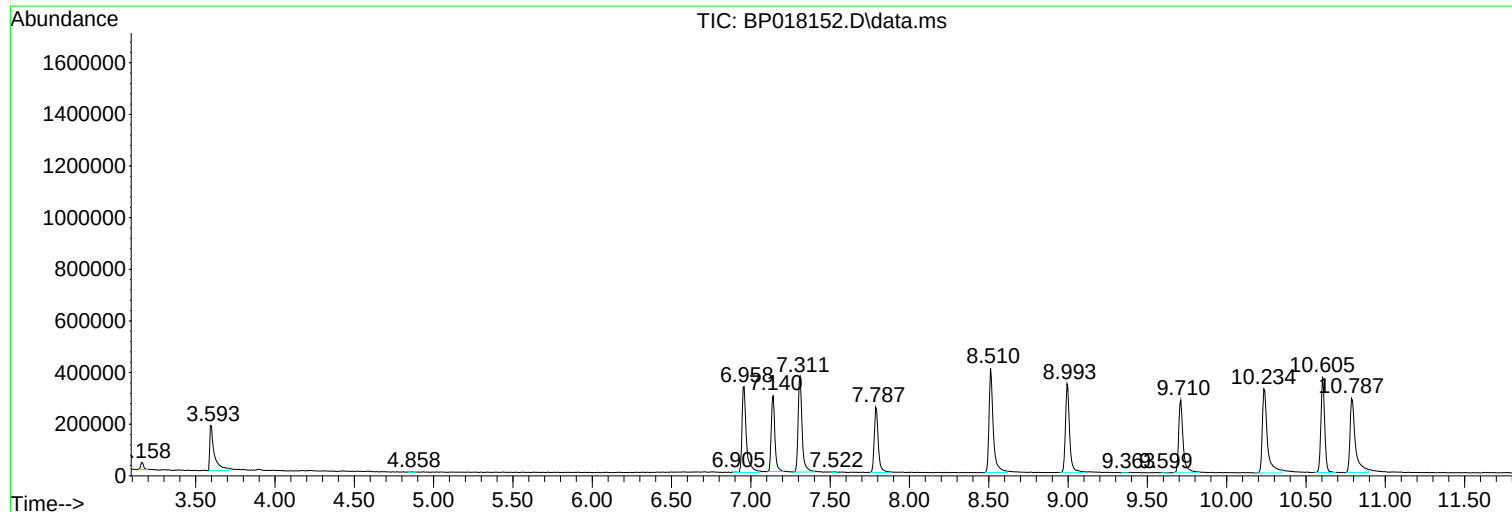

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111423\
Data File : BP018152.D
Acq On : 14 Nov 2023 12:47
Operator : MA/JU
Sample : PB156922BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK922

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111423\
Data File : BP018152.D
Acq On : 14 Nov 2023 12:47
Operator : MA/JU
Sample : PB156922BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK922

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc