

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111423\
 Data File : BP018155.D
 Acq On : 14 Nov 2023 15:02
 Operator : MA/JU
 Sample : 05337-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCDH8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018155.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.164	10	13	19	rVB2	19443	20550	0.60%	0.075%
2	3.640	89	94	101	rBV5	14129	34445	1.01%	0.125%
3	3.899	135	138	142	rBV2	5933	7342	0.21%	0.027%
4	5.034	323	331	338	rVB2	3725	9656	0.28%	0.035%
5	6.752	618	623	627	rVB8	3323	4581	0.13%	0.017%
6	6.963	653	659	675	rBV	46027	105489	3.09%	0.383%
7	7.140	681	689	701	rBV	293879	471979	13.81%	1.713%
8	7.310	712	718	733	rBV	263927	465323	13.61%	1.689%
9	7.787	790	799	814	rBV	356412	601659	17.60%	2.184%
10	8.516	916	923	939	rBV	174284	351256	10.28%	1.275%
11	8.993	998	1004	1019	rBV	388551	708254	20.72%	2.571%
12	9.169	1030	1034	1040	rVB8	5494	10484	0.31%	0.038%
13	9.710	1119	1126	1141	rBV	302185	591935	17.32%	2.149%
14	10.234	1209	1215	1243	rBV	341361	768979	22.49%	2.791%
15	10.604	1268	1278	1289	rBV	554910	928153	27.15%	3.369%
16	10.793	1302	1310	1333	rBV	184618	495897	14.51%	1.800%
17	11.157	1367	1372	1375	rBV7	2624	5361	0.16%	0.019%
18	11.651	1452	1456	1463	rVB7	3612	7294	0.21%	0.026%
19	12.234	1548	1555	1563	rVB8	6211	14711	0.43%	0.053%
20	13.310	1730	1738	1744	rBV3	16251	30536	0.89%	0.111%
21	13.892	1830	1837	1848	rBV	1062820	1538559	45.01%	5.585%
22	13.987	1848	1853	1864	rBV4	17567	65125	1.91%	0.236%
23	14.169	1877	1884	1896	rBV2	1070916	1599868	46.80%	5.808%
24	14.469	1928	1935	1945	rBV	819718	1201098	35.14%	4.360%
25	14.787	1983	1989	1999	rBV5	14720	49547	1.45%	0.180%
26	15.204	2057	2060	2065	rBV6	3744	5980	0.17%	0.022%
27	15.469	2099	2105	2114	rBV	1513355	2177313	63.69%	7.904%
28	15.534	2114	2116	2123	rVB8	6348	10883	0.32%	0.040%
29	15.628	2127	2132	2144	rBV	464023	714917	20.91%	2.595%
30	16.192	2222	2228	2236	rVB7	8114	14753	0.43%	0.054%
31	16.257	2236	2239	2240	rBV3	3311	3850	0.11%	0.014%
32	16.281	2240	2243	2247	rVV	14246	19063	0.56%	0.069%
33	16.339	2249	2253	2259	rVV4	18557	36609	1.07%	0.133%
34	16.404	2259	2264	2268	rVV3	14420	25437	0.74%	0.092%
35	16.451	2268	2272	2277	rVV5	11154	18292	0.54%	0.066%
36	16.504	2277	2281	2287	rVV4	8355	18705	0.55%	0.068%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111423\
 Data File : BP018155.D
 Acq On : 14 Nov 2023 15:02
 Operator : MA/JU
 Sample : 05337-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCDH8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

37	16.551	2287	2289	2293	rVV3	7917	9143	0.27%	0.033%
38	16.604	2293	2298	2306	rVV3	15084	32186	0.94%	0.117%
39	16.681	2306	2311	2316	rVV	13031	23741	0.69%	0.086%
40	16.751	2319	2323	2329	rVB5	8211	12880	0.38%	0.047%
41	16.922	2347	2352	2354	rVB5	3251	5518	0.16%	0.020%
42	17.051	2371	2374	2377	rBV5	3599	4577	0.13%	0.017%
43	17.122	2383	2386	2390	rVB5	2823	4128	0.12%	0.015%
44	17.245	2401	2407	2418	rBV	1066089	1466119	42.89%	5.322%
45	17.351	2418	2425	2444	rVV	1749058	2645389	77.39%	9.603%
46	17.510	2446	2452	2456	rVB6	5552	11980	0.35%	0.043%
47	17.586	2461	2465	2466	rBV4	3053	3447	0.10%	0.013%
48	17.880	2510	2515	2522	rBV4	39801	58564	1.71%	0.213%
49	18.098	2547	2552	2558	rBV5	27564	43934	1.29%	0.159%
50	18.192	2566	2568	2573	rVB	7929	10051	0.29%	0.036%
51	18.310	2584	2588	2594	rBV	23362	35581	1.04%	0.129%
52	18.663	2644	2648	2649	rBV4	3255	4385	0.13%	0.016%
53	19.175	2731	2735	2740	rBV3	24212	37150	1.09%	0.135%
54	19.233	2741	2745	2746	rBV3	25425	26234	0.77%	0.095%
55	19.345	2761	2764	2770	rVB5	18352	26592	0.78%	0.097%
56	19.480	2784	2787	2791	rBV5	11741	13597	0.40%	0.049%
57	19.604	2802	2808	2818	rBV	2429019	3135787	91.73%	11.383%
58	21.380	3105	3110	3121	rBV	1293262	1678866	49.11%	6.094%
59	23.686	3494	3502	3512	rBV2	1750439	3418472	100.00%	12.409%
60	23.845	3523	3529	3540	rVB	815168	1705478	49.89%	6.191%




Sum of corrected areas: 27547682

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111423\
Data File : BP018155.D
Acq On : 14 Nov 2023 15:02
Operator : MA/JU
Sample : 05337-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCDH8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

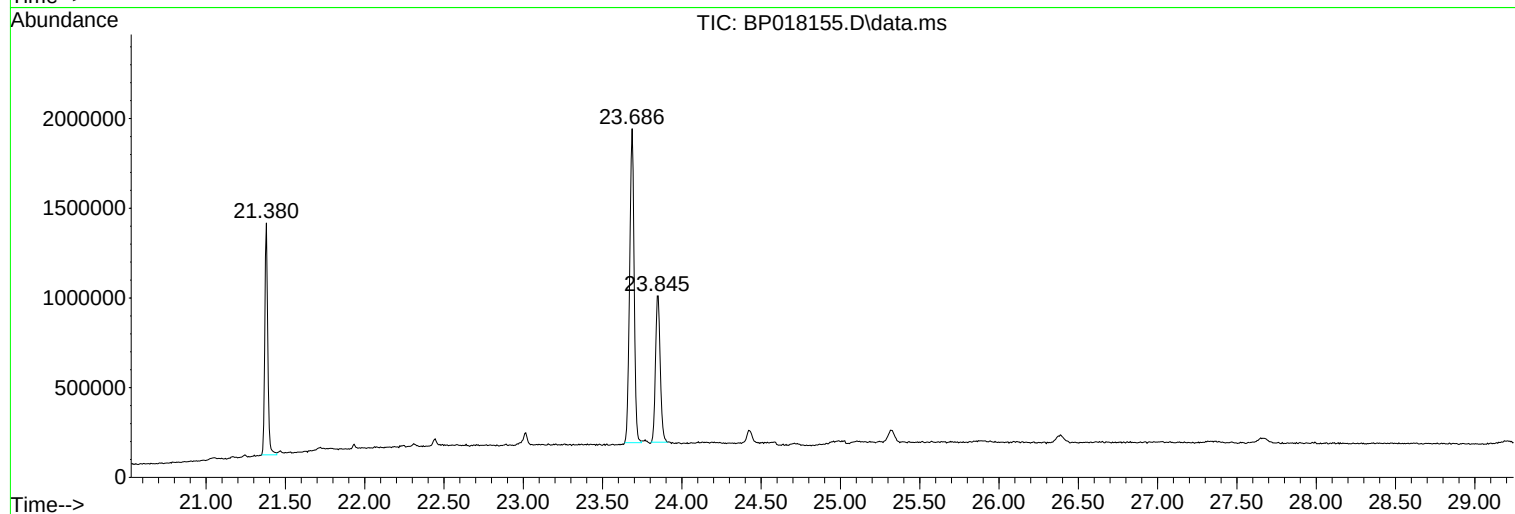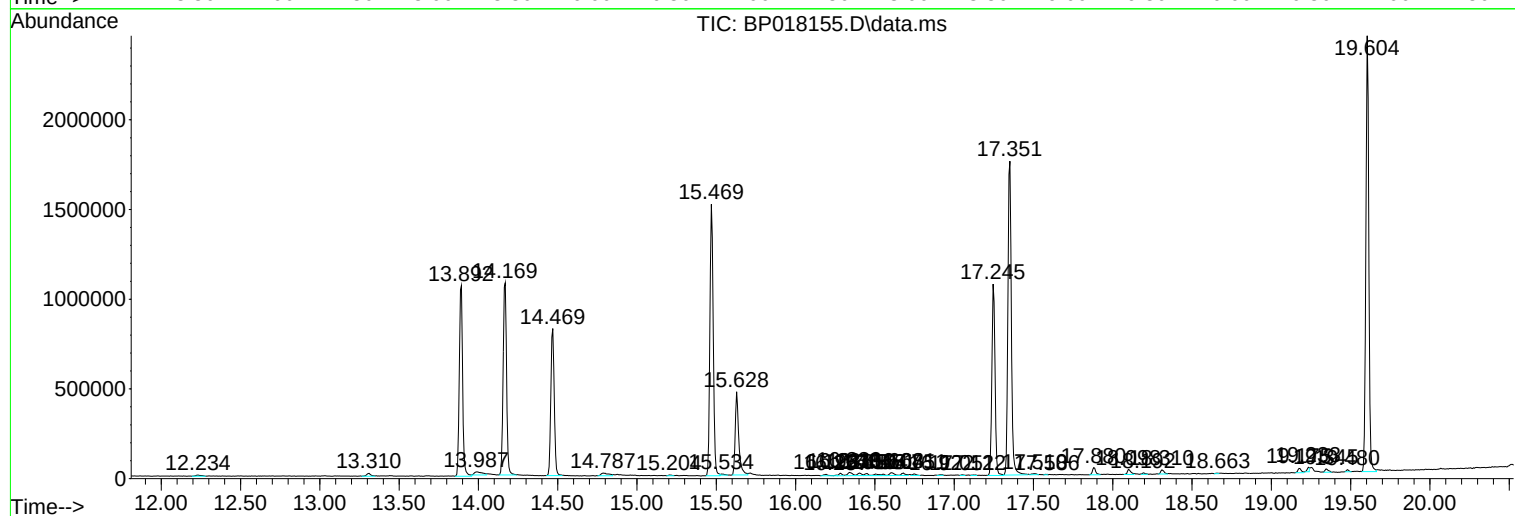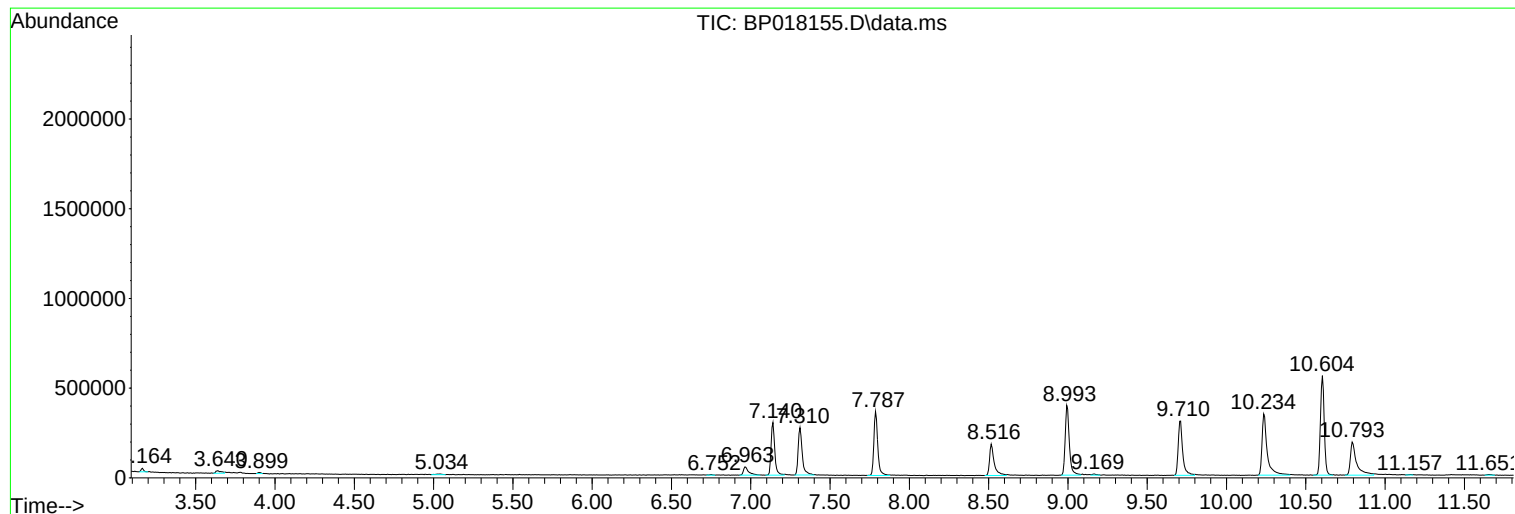

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111423\
Data File : BP018155.D
Acq On : 14 Nov 2023 15:02
Operator : MA/JU
Sample : 05337-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCDH8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111423\
Data File : BP018155.D
Acq On : 14 Nov 2023 15:02
Operator : MA/JU
Sample : 05337-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCDH8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc