

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111423\
 Data File : BP018158.D
 Acq On : 14 Nov 2023 16:43
 Operator : MA/JU
 Sample : PB157059BL
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK059

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018158.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.158	9	12	18	rVB	29544	35671	1.42%	0.143%
2	3.599	83	87	103	rBV	170883	329413	13.13%	1.318%
3	3.893	136	137	144	rVB6	5143	7276	0.29%	0.029%
4	4.387	220	221	225	rVB3	2693	3088	0.12%	0.012%
5	4.769	283	286	289	rBV4	2069	3295	0.13%	0.013%
6	6.952	651	657	674	rBV	318522	607505	24.22%	2.432%
7	7.140	682	689	701	rBV	293599	469039	18.70%	1.877%
8	7.311	711	718	731	rBV	356516	624770	24.90%	2.501%
9	7.787	791	799	813	rBV	314370	531087	21.17%	2.126%
10	8.510	914	922	941	rBV	391527	755302	30.11%	3.023%
11	8.993	992	1004	1020	rBV	347324	636234	25.36%	2.547%
12	9.216	1041	1042	1047	rVB5	2400	2779	0.11%	0.011%
13	9.710	1119	1126	1143	rBV	299383	587933	23.44%	2.353%
14	9.852	1148	1150	1154	rVB5	1995	2811	0.11%	0.011%
15	10.040	1179	1182	1185	rBV5	1961	2586	0.10%	0.010%
16	10.234	1209	1215	1235	rBV	361662	797955	31.81%	3.194%
17	10.604	1271	1278	1291	rVB	491373	825700	32.91%	3.305%
18	10.793	1303	1310	1340	rBV	278173	700881	27.94%	2.805%
19	11.640	1450	1454	1458	rBV7	1825	2861	0.11%	0.011%
20	12.257	1553	1559	1565	rBV7	4683	12182	0.49%	0.049%
21	13.228	1720	1724	1728	rVB6	1582	2850	0.11%	0.011%
22	13.310	1733	1738	1742	rBV8	3917	7297	0.29%	0.029%
23	13.893	1830	1837	1854	rBV	924667	1391269	55.46%	5.569%
24	14.169	1876	1884	1899	rBV	971036	1488290	59.33%	5.957%
25	14.469	1928	1935	1943	rBV	763586	1110340	44.26%	4.444%
26	14.740	1976	1981	2005	rBV	111219	399254	15.91%	1.598%
27	15.092	2039	2041	2047	rVB6	2271	3032	0.12%	0.012%
28	15.416	2094	2096	2098	rBV3	2207	2668	0.11%	0.011%
29	15.469	2098	2105	2119	rVV	1324551	1941888	77.41%	7.772%
30	15.634	2126	2133	2144	rBV	222419	417227	16.63%	1.670%
31	16.269	2238	2241	2246	rVB7	3124	3142	0.13%	0.013%
32	16.363	2252	2257	2260	rVB6	2485	3489	0.14%	0.014%
33	16.634	2301	2303	2312	rVB9	1754	3406	0.14%	0.014%
34	17.051	2368	2374	2377	rBV7	3248	5622	0.22%	0.023%
35	17.245	2401	2407	2416	rBV	970960	1371020	54.65%	5.487%
36	17.351	2418	2425	2446	rVB	1403624	2145545	85.52%	8.587%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111423\
Data File : BP018158.D
Acq On : 14 Nov 2023 16:43
Operator : MA/JU
Sample : PB157059BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK059

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Title : SVOA CALIBRATION

37	17.845	2503	2509	2511	rBV6	2243	3845	0.15%	0.015%
38	17.881	2511	2515	2517	rBV5	3112	3816	0.15%	0.015%
39	19.181	2732	2736	2741	rBV4	18575	27100	1.08%	0.108%
40	19.257	2745	2749	2758	rVB2	14398	24477	0.98%	0.098%
41	19.604	2802	2808	2821	rBV	1799014	2508685	100.00%	10.041%
42	21.380	3105	3110	3121	rBV	1043023	1441342	57.45%	5.769%
43	23.686	3495	3502	3513	rBV2	1217557	2346095	93.52%	9.390%
44	23.851	3523	3530	3542	rVB	658912	1394507	55.59%	5.581%




Sum of corrected areas: 24984574

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111423\
Data File : BP018158.D
Acq On : 14 Nov 2023 16:43
Operator : MA/JU
Sample : PB157059BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK059

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

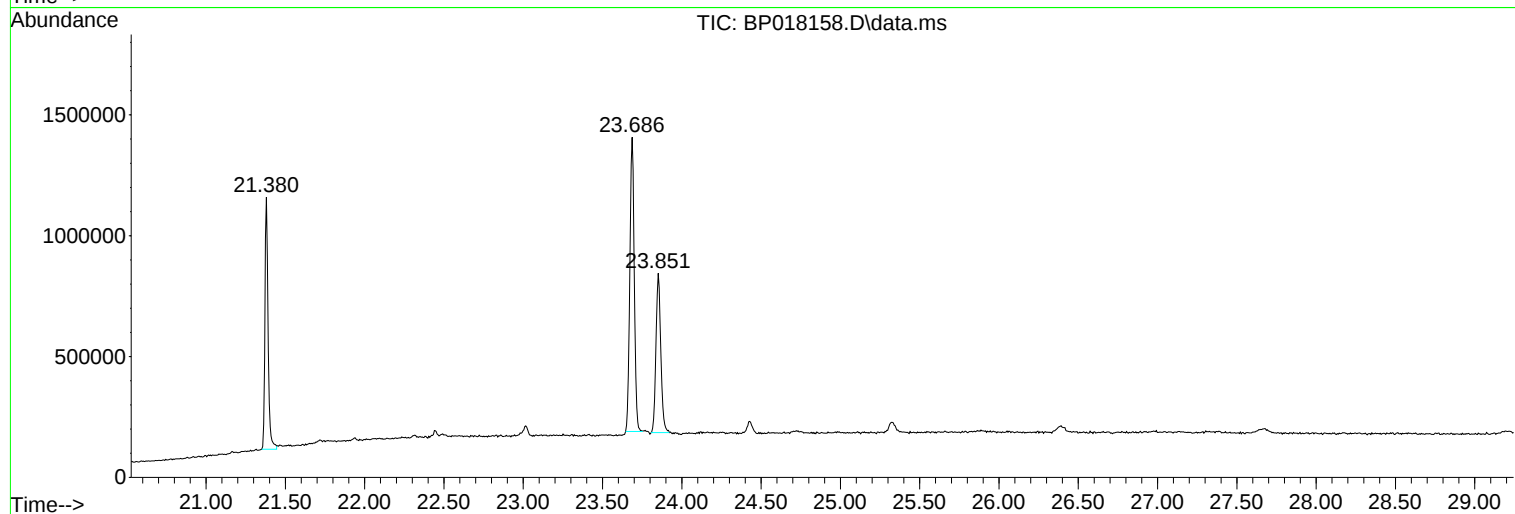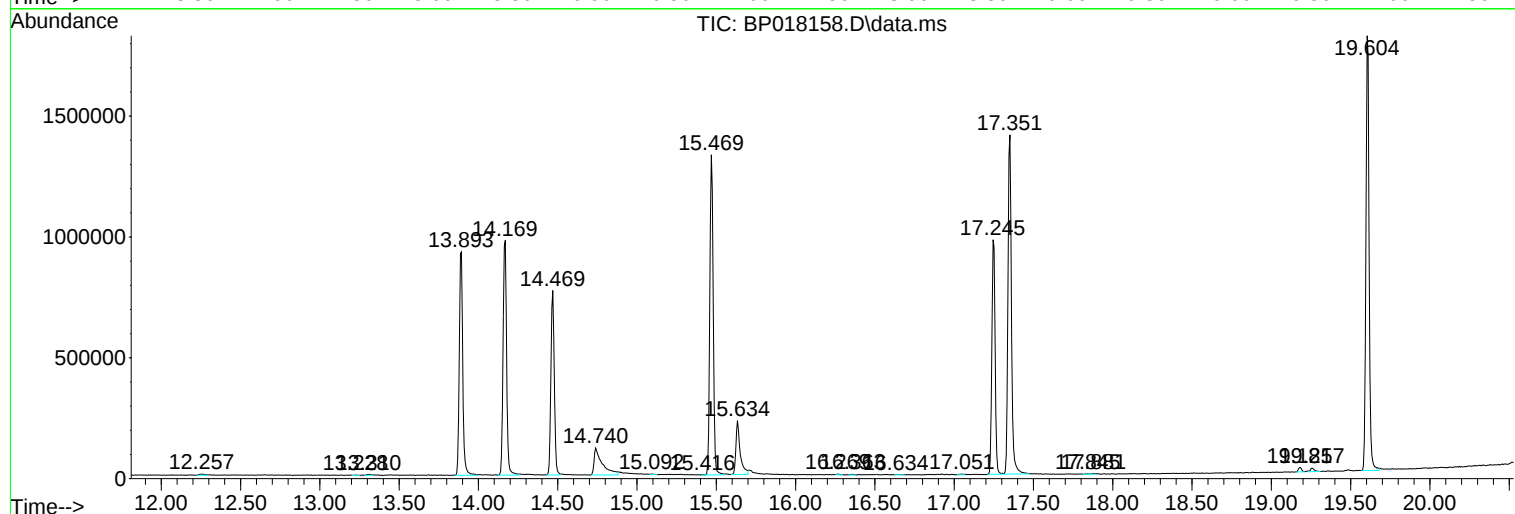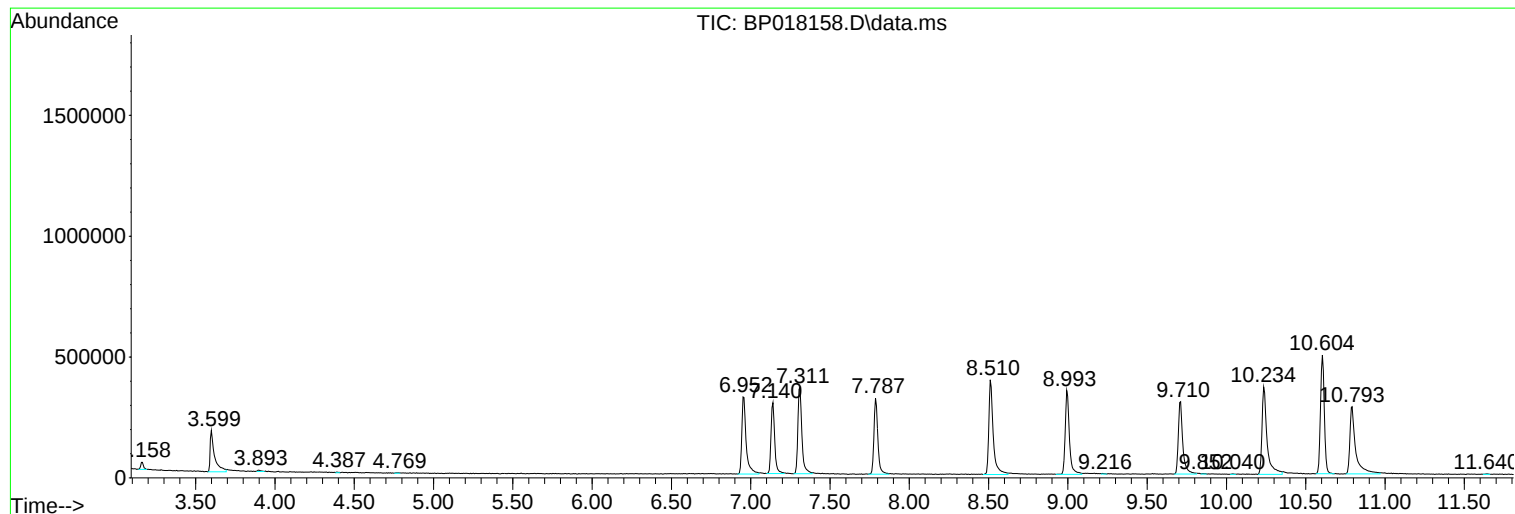

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111423\
Data File : BP018158.D
Acq On : 14 Nov 2023 16:43
Operator : MA/JU
Sample : PB157059BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK059

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111423\
Data File : BP018158.D
Acq On : 14 Nov 2023 16:43
Operator : MA/JU
Sample : PB157059BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK059

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------