


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111425\
Data File : BP026136.D
Acq On : 14 Nov 2025 11:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Oct 30 11:51:34 2025

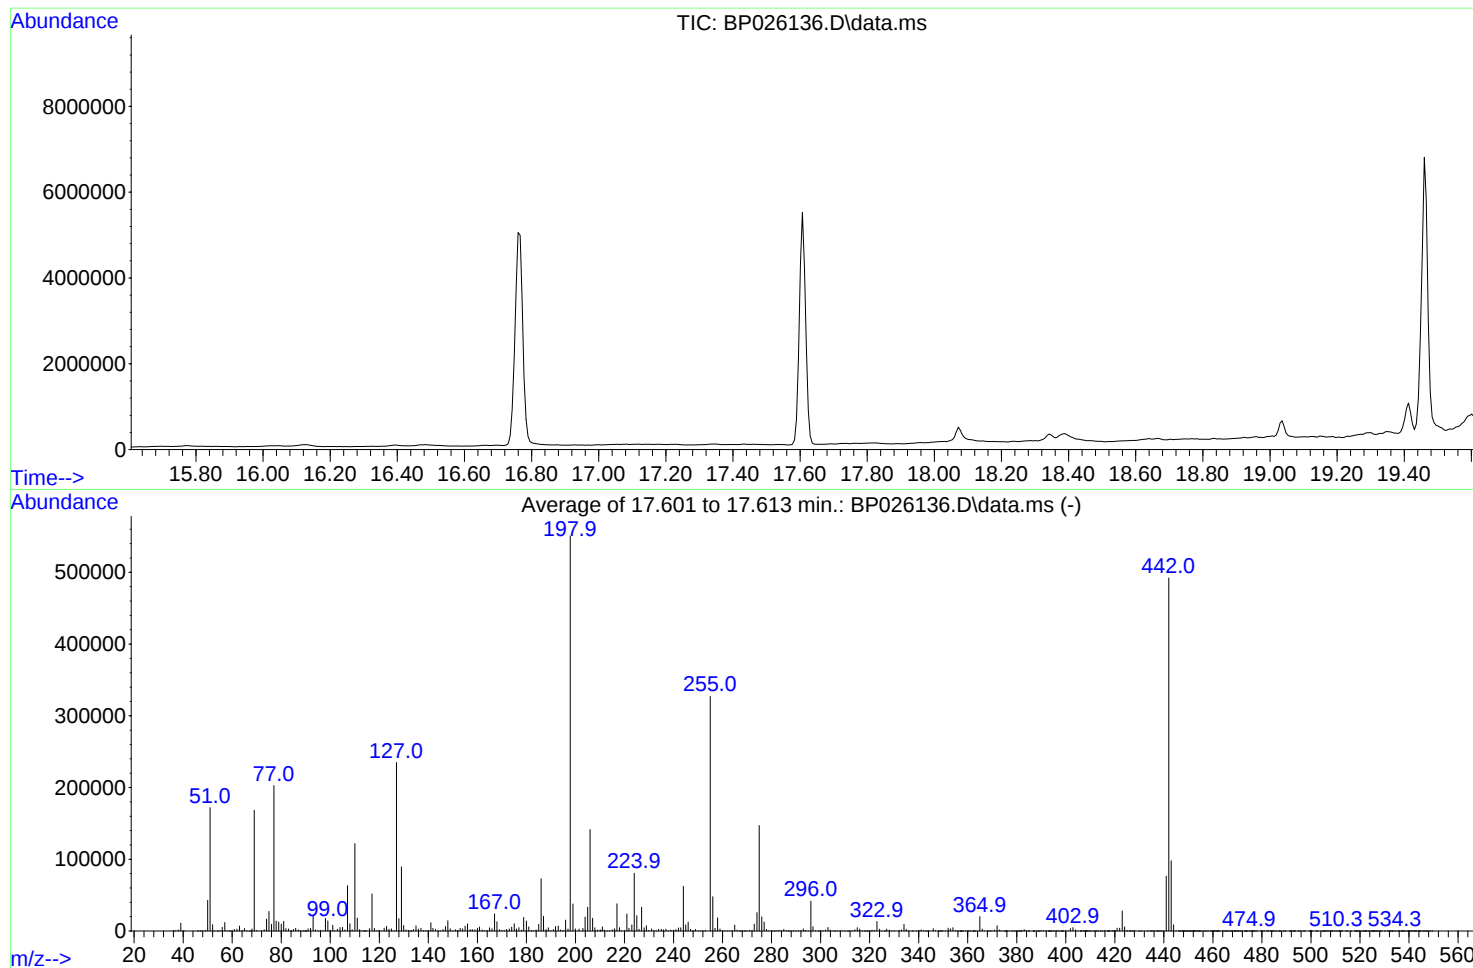

AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2484




Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.7	2840	PASS
69	69	100	100	100.0	168499	PASS
70	69	0.00	2	0.5	808	PASS
197	198	0.00	2	0.5	2943	PASS
198	198	100	100	100.0	550396	PASS
199	198	5	9	6.8	37661	PASS
365	198	1	100	3.7	20158	PASS
441	443	0.01	150	78.0	76443	PASS
442	442	100	100	100.0	492049	PASS
443	442	15	24	19.9	98021	PASS

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/14/2025	BNA_P	<u>BP026136.D</u>
Compound Name	Response	Retention Time
DDT	2258799	20.766
DDD	127705	20.301
DDE	7336	19.777
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
135041	2393840	5.64

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111425\
Data File : BP026136.D
Acq On : 14 Nov 2025 11:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 14 11:24:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 30 11:51:34 2025
Response via : Initial Calibration

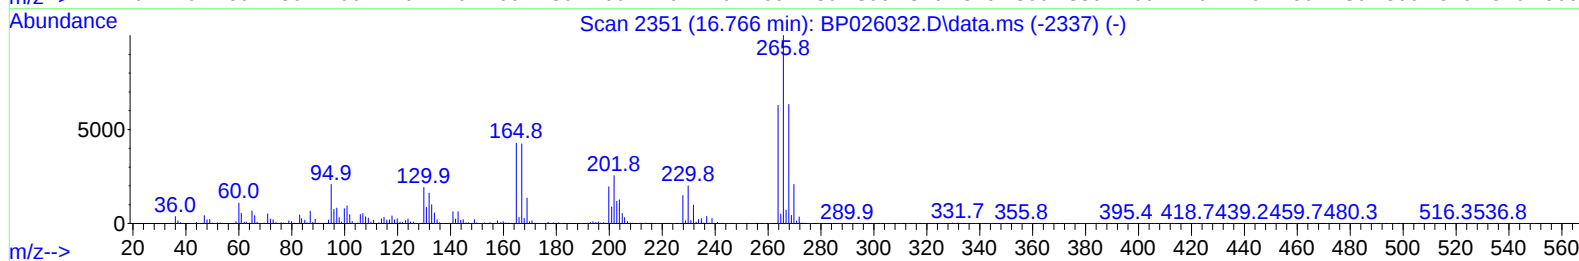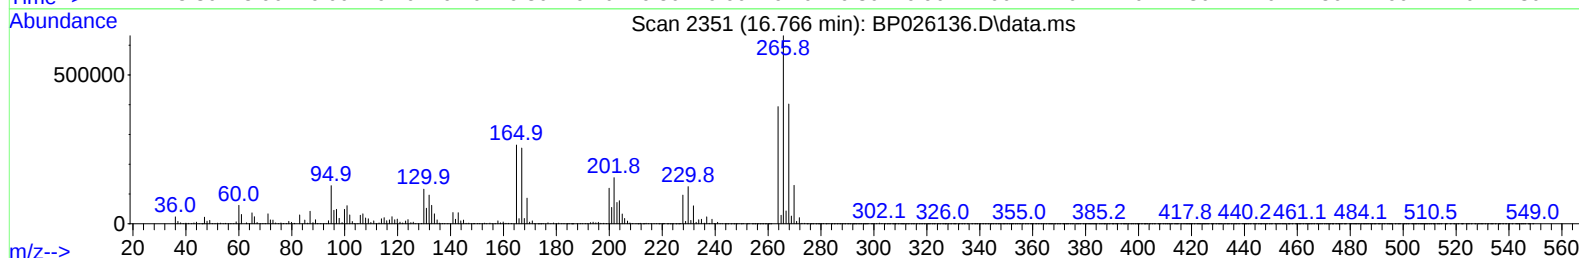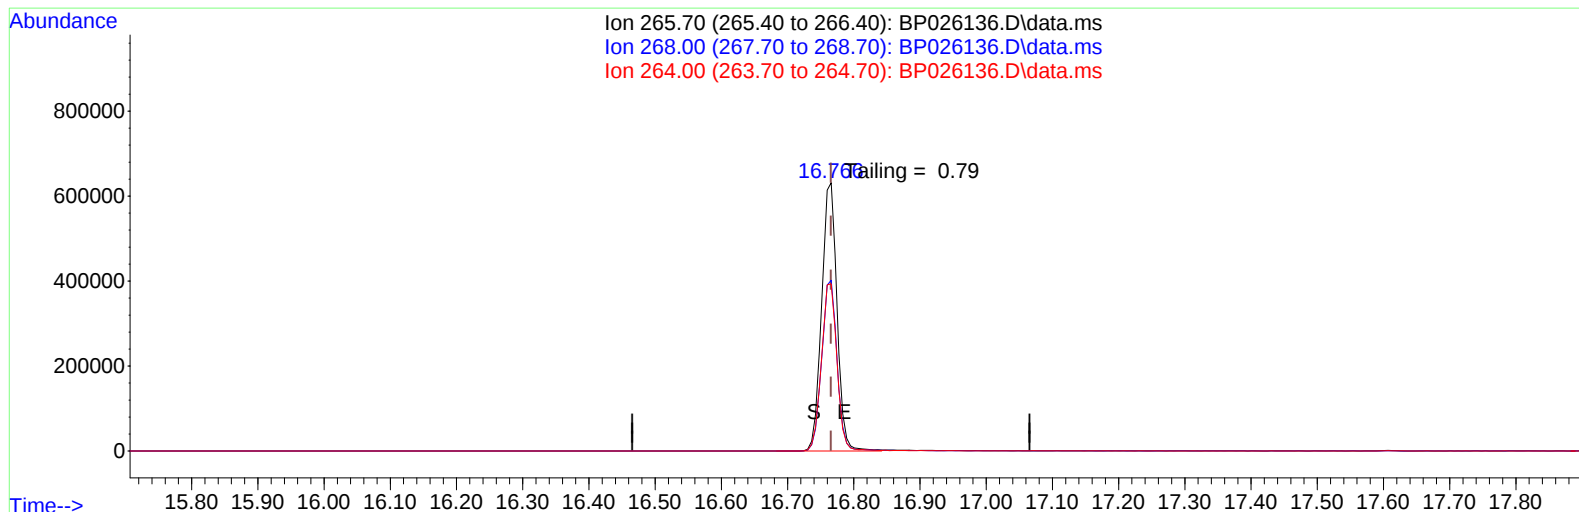

TIC: BP026136.D\data.ms

(70) Pentachlorophenol (C)




16.766min (+ 0.000) 1215921.03 ng

response 1022272

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	63.64
264.00	62.80	62.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111425\
Data File : BP026136.D
Acq On : 14 Nov 2025 11:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 14 11:24:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 30 11:51:34 2025
Response via : Initial Calibration

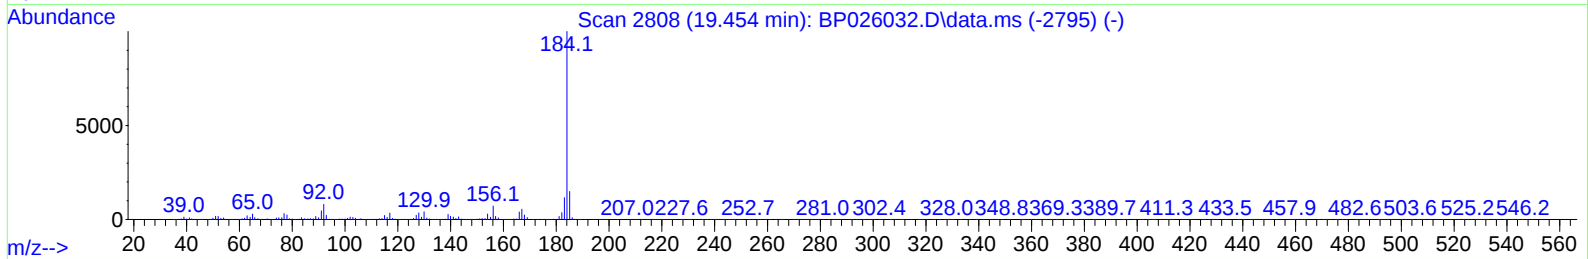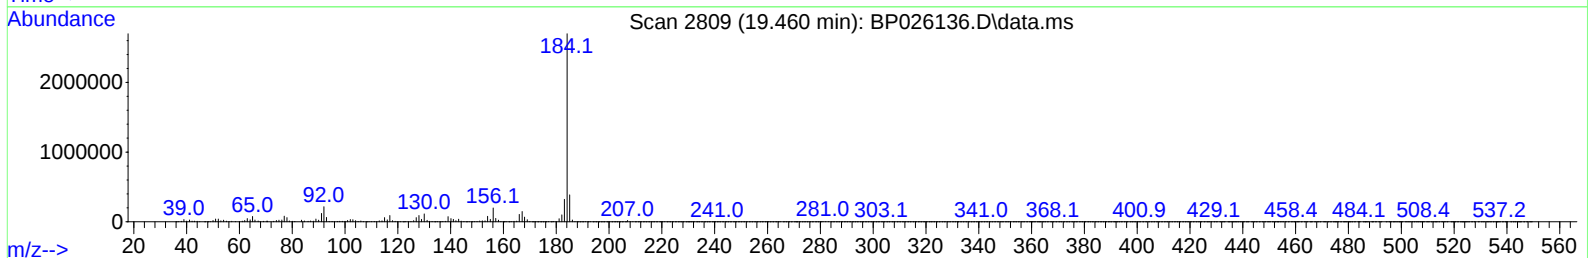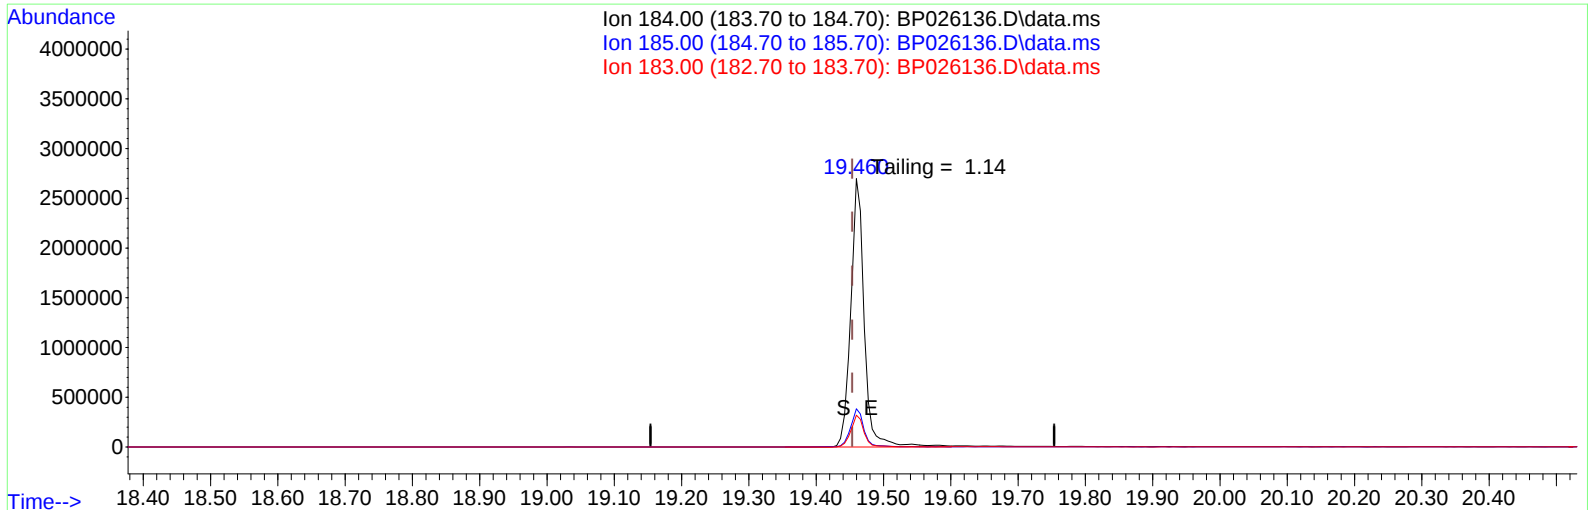

TIC: BP026136.D\data.ms

(77) Benzidine**19.460min (+ 0.006) 546345.61 ng****response 3688802**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.29
183.00	11.50	11.88
0.00	0.00	0.00