


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111425\
Data File : BP026136.D
Acq On : 14 Nov 2025 11:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Oct 30 11:51:34 2025

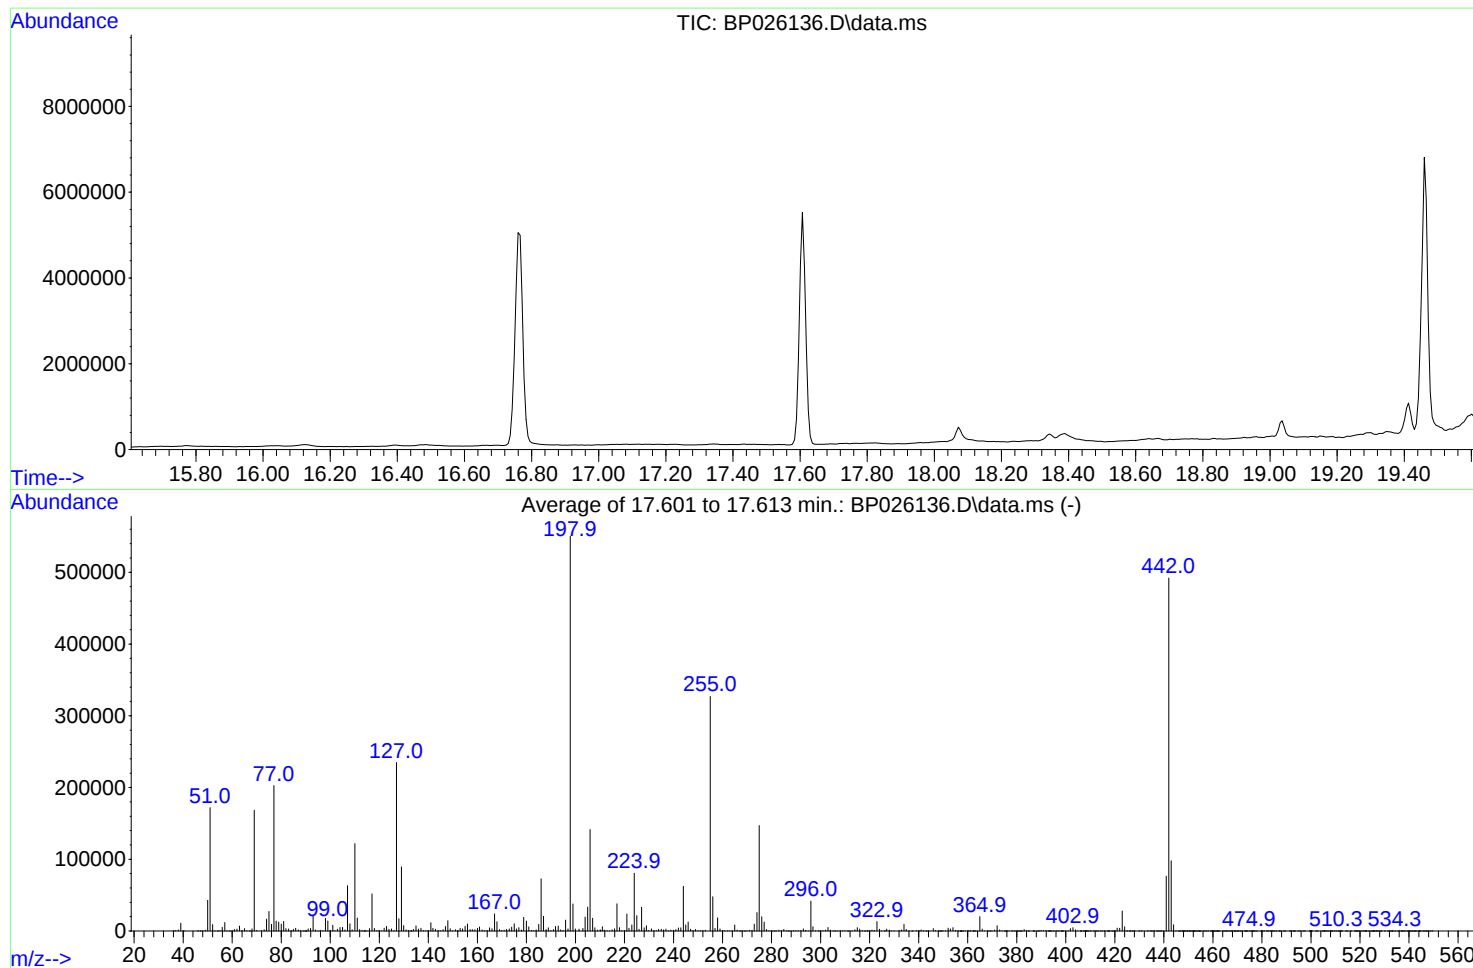

AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2484

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.7	2840	PASS
69	69	100	100	100.0	168499	PASS
70	69	0.00	2	0.5	808	PASS
197	198	0.00	2	0.5	2943	PASS
198	198	100	100	100.0	550396	PASS
199	198	5	9	6.8	37661	PASS
365	198	1	100	3.7	20158	PASS
441	443	0.01	150	78.0	76443	PASS
442	442	100	100	100.0	492049	PASS
443	442	15	24	19.9	98021	PASS