
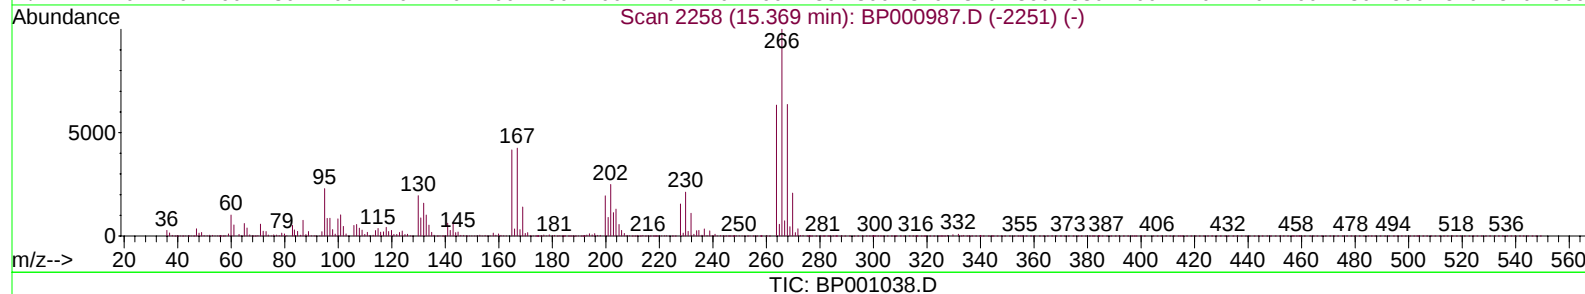
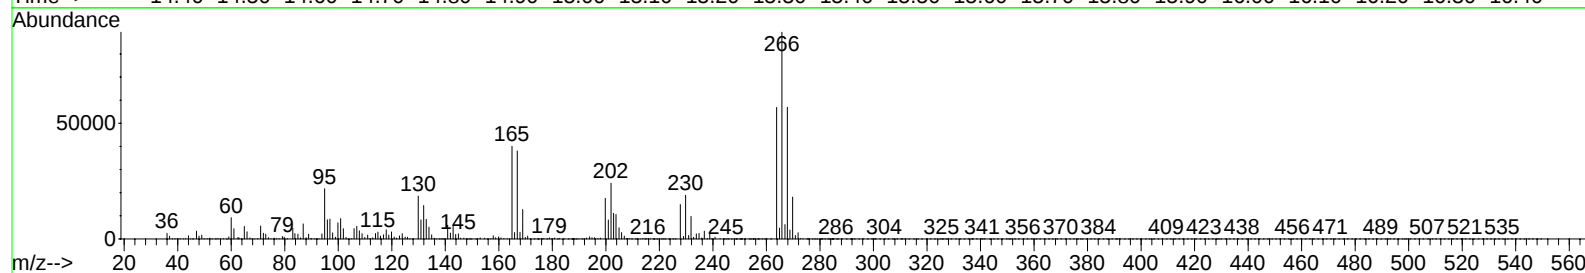


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP111519\
Data File : BP001038.D
Acq On : 15 Nov 2019 13:32
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 15 18:11:30 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP110619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 06 17:07:13 2019
Response via : Initial Calibration

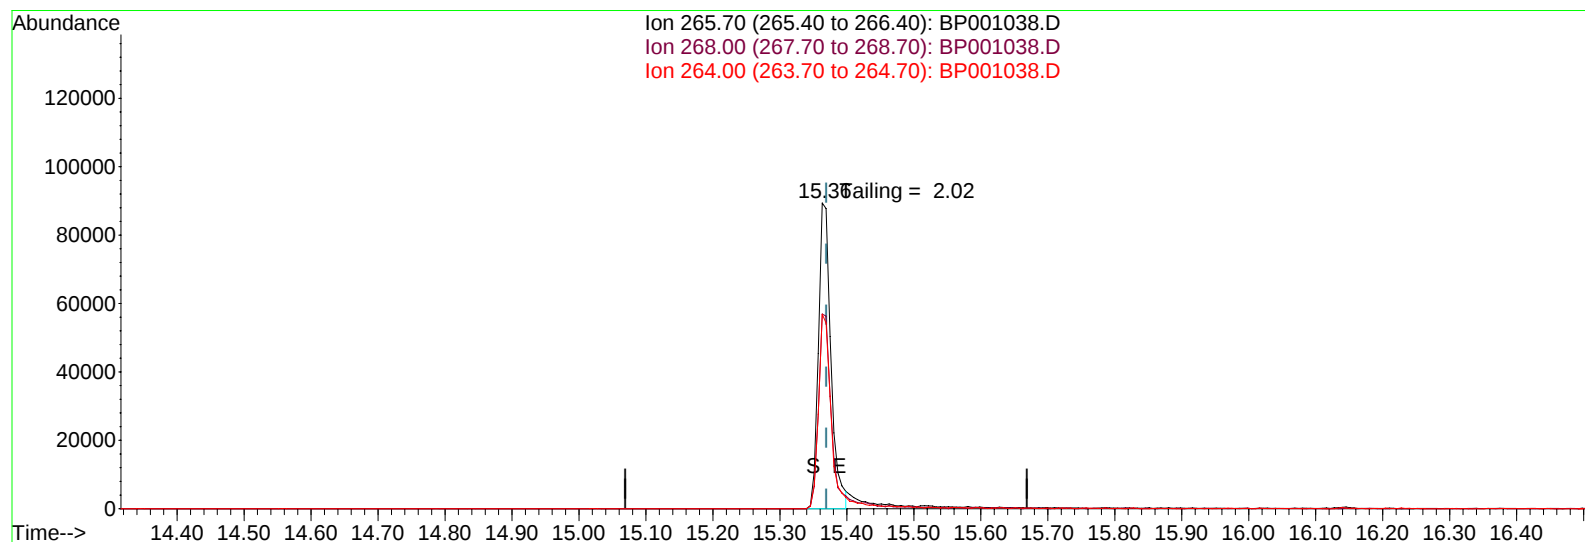

(70) Pentachlorophenol (C)




15.363min (-0.006) 483203.84ng

response 126175

Ion	Exp%	Act%
265.70	100	100
268.00	63.60	63.70
264.00	63.30	63.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP111519\
Data File : BP001038.D
Acq On : 15 Nov 2019 13:32
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 15 18:11:30 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP110619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 06 17:07:13 2019
Response via : Initial Calibration

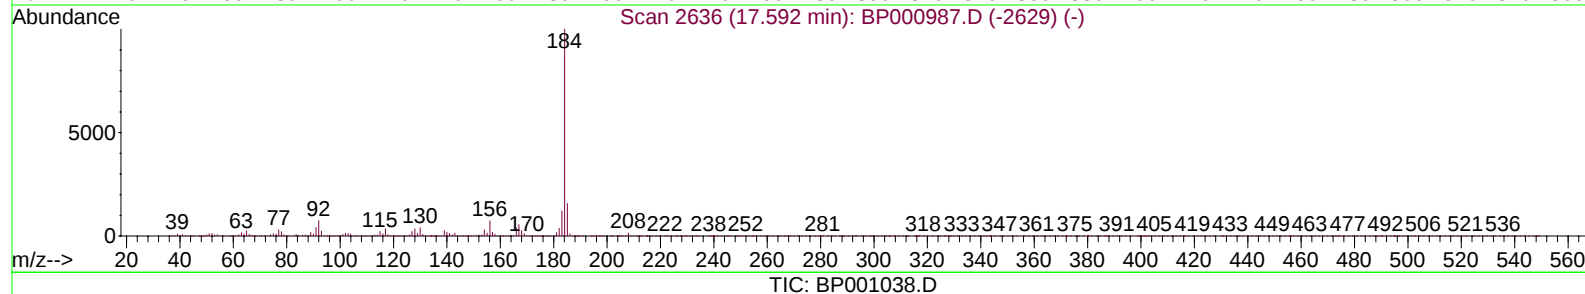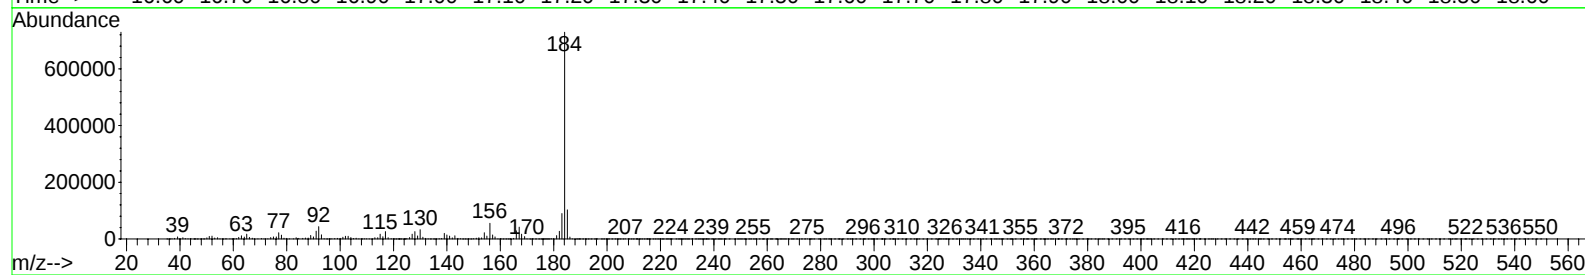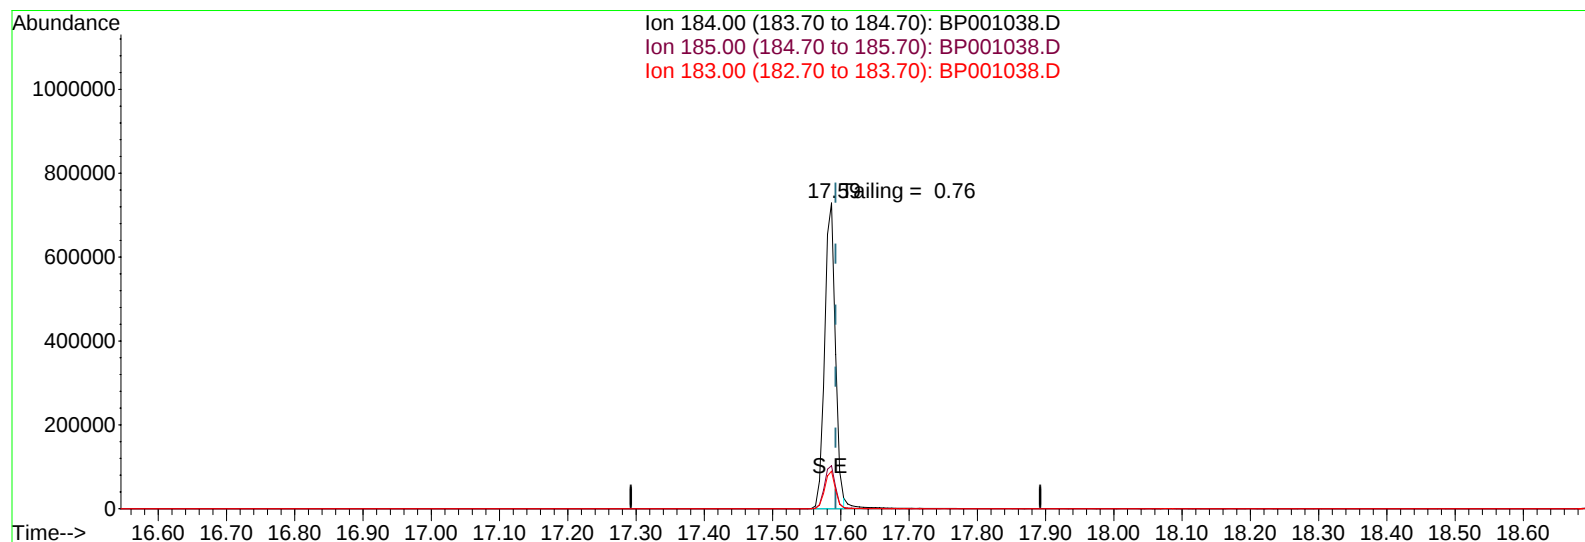

(77) Benzidine

17.586min (-0.006) 169461.43ng

response 805034

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.06
183.00	12.20	12.29
0.00	0.00	0.00