


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP111519\
 Data File : BP001038.D
 Acq On : 15 Nov 2019 13:32
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 06 17:07:13 2019

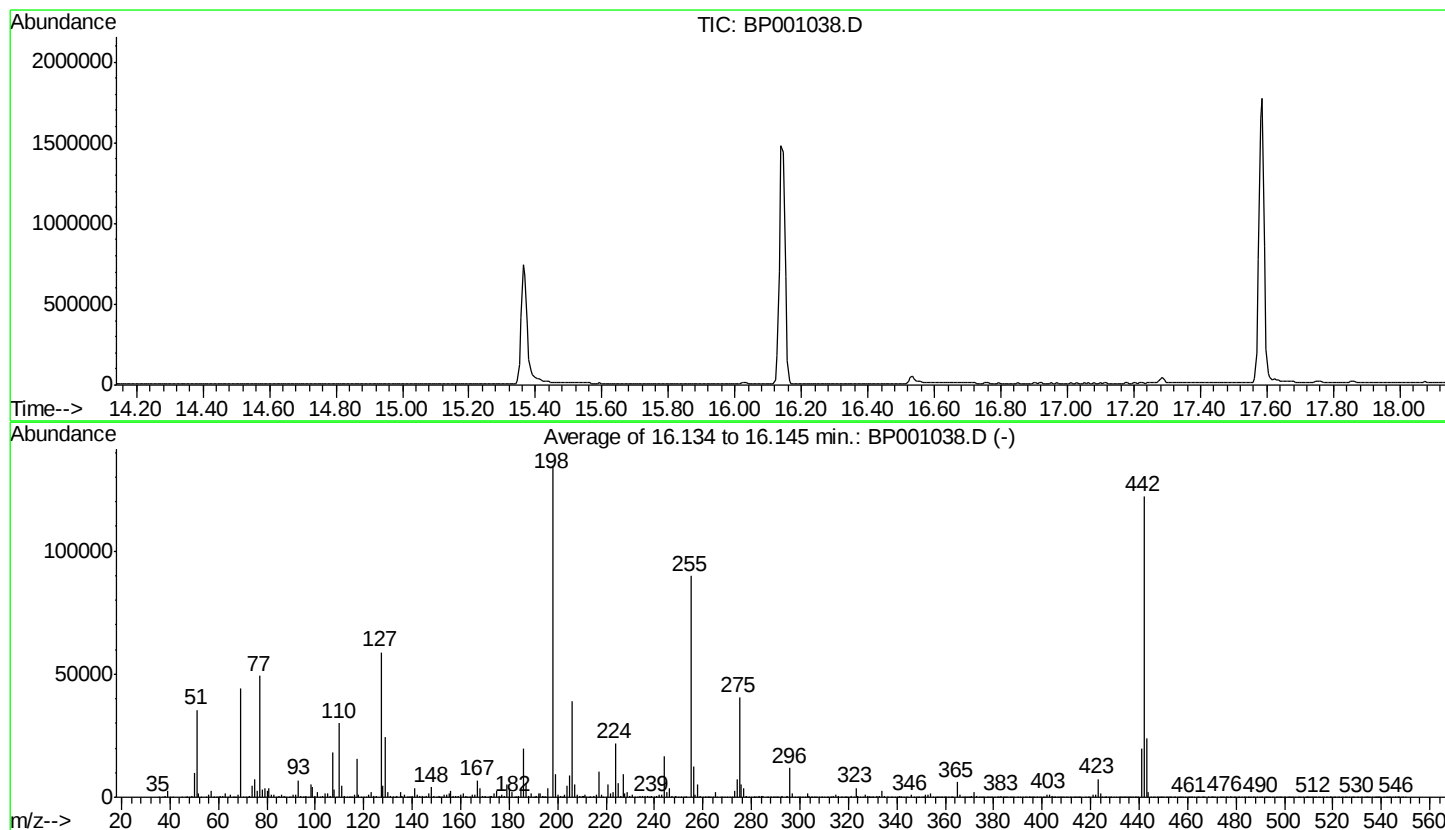

AutoFind: Scans 2388, 2389, 2390; Background Corrected with Scan 2381

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.4	35504	PASS
68	69	0.00	2	2.0	901	PASS
69	198	0.00	100	32.9	44312	PASS
70	69	0.00	2	0.5	212	PASS
127	198	10	80	43.7	58802	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	134668	PASS
199	198	5	9	6.9	9250	PASS
275	198	10	60	30.1	40511	PASS
365	198	1	100	4.5	6073	PASS
441	198	0.01	100	14.5	19577	PASS
442	198	50	100	90.7	122082	PASS
443	442	15	24	19.5	23861	PASS