




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
 Data File : BP018188.D
 Acq On : 15 Nov 2023 23:54
 Operator : MA/JU
 Sample : PB157169BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK169

Manual IntegrationsAPPROVED

Quant Time: Nov 16 00:53:22 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 15 18:13:37 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/16/2023
 Supervised By :mohammad ahmed 11/17/2023

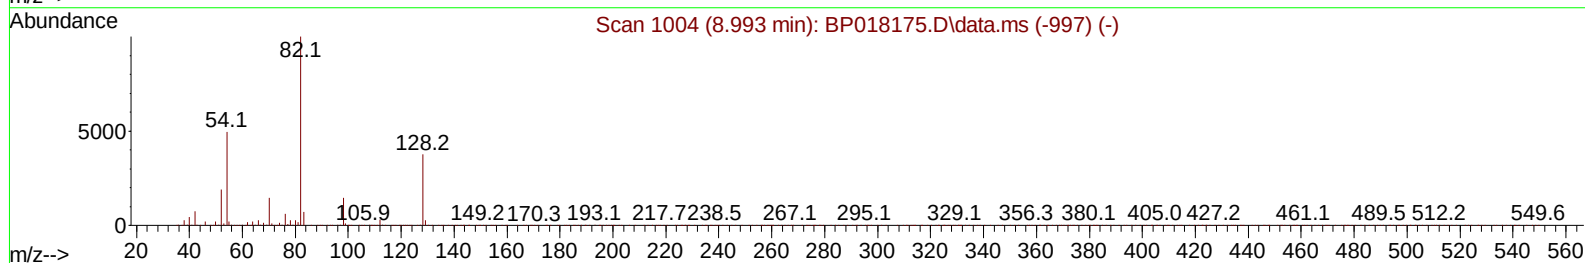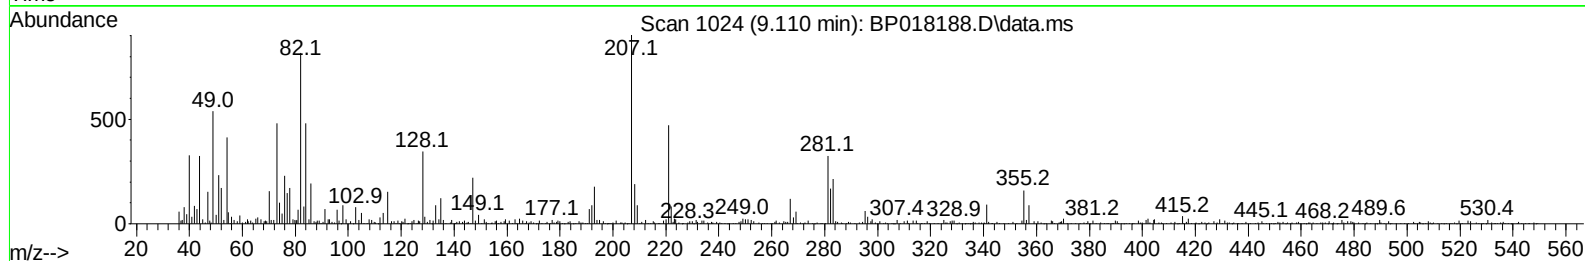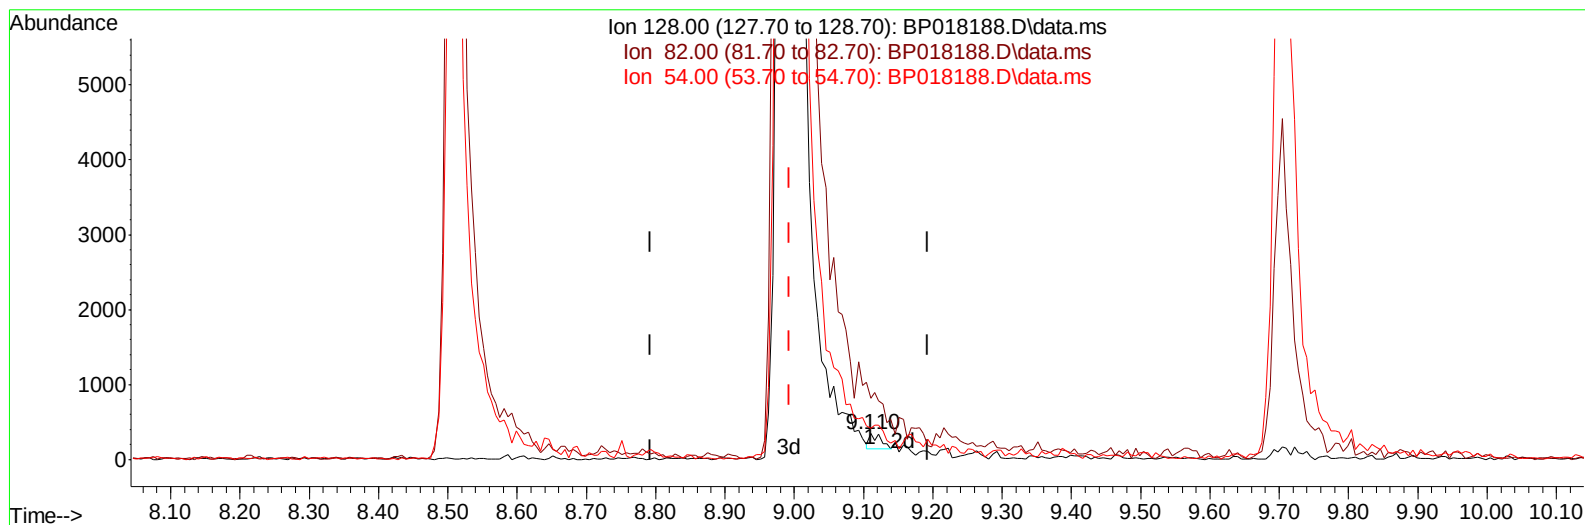

TIC: BP018188.D\data.ms

(21) Nitrobenzene-d5 (S)

9.110min (+ 0.118) 0.10 ng/u1

response 224

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	256.70	236.52
54.00	125.00	119.42
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
 Data File : BP018188.D
 Acq On : 15 Nov 2023 23:54
 Operator : MA/JU
 Sample : PB157169BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK169

Manual IntegrationsAPPROVED

Quant Time: Nov 16 00:53:22 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 15 18:13:37 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/16/2023
 Supervised By :mohammad ahmed 11/17/2023

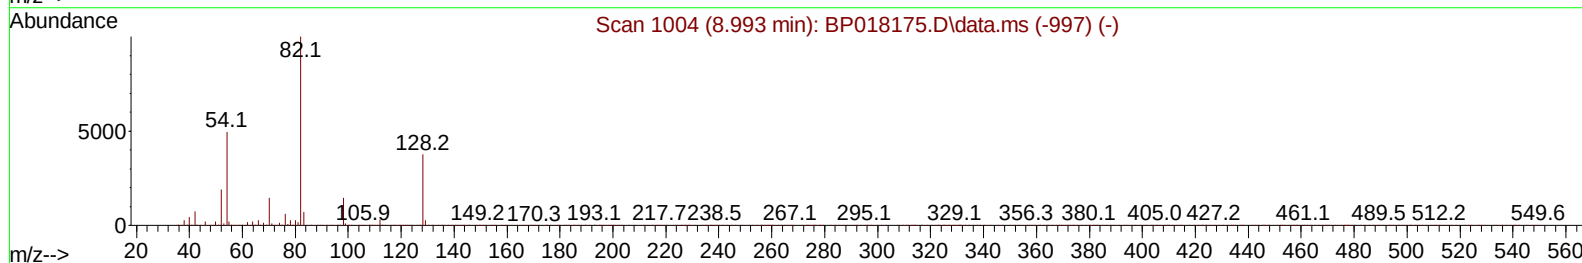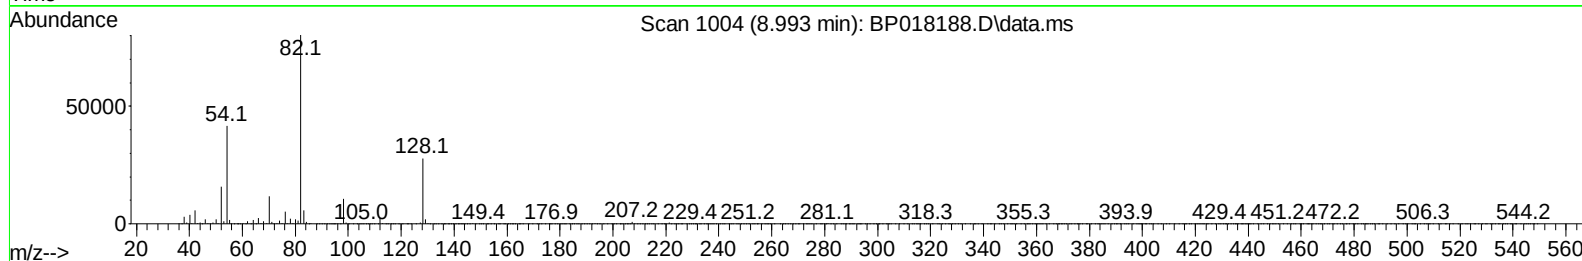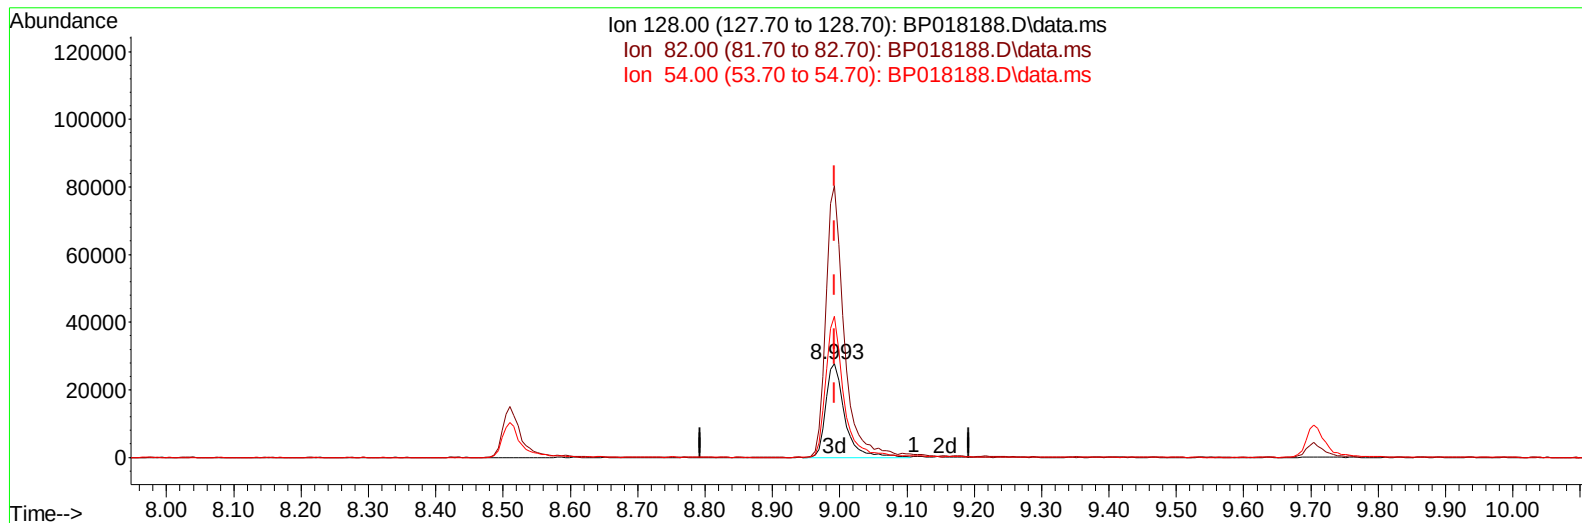

TIC: BP018188.D\data.ms

(21) Nitrobenzene-d5 (S)

8.993min (-0.000) 23.67 ng/ul m

response 54044

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	256.70	288.97
54.00	125.00	150.01#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
 Data File : BP018188.D
 Acq On : 15 Nov 2023 23:54
 Operator : MA/JU
 Sample : PB157169BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK169

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/16/2023
 Supervised By :mohammad ahmed 11/17/2023

Quant Time: Nov 16 00:55:53 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 15 18:13:37 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.781	152	66554	20.000	ng/ul	0.00
20) Naphthalene-d8	10.598	136	253458	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.463	164	145226	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.245	188	313459	20.000	ng/ul	0.00
79) Chrysene-d12	21.374	240	304184	20.000	ng/ul	0.00
88) Perylene-d12	23.845	264	364730	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.158	96	9524	5.048	ng/uL	0.00
4) Pyridine-d5	3.593	84	94544	19.219	ng/ul	0.00
7) Phenol-d5	6.952	99	141476	22.019	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.134	67	91964	24.355	ng/ul	0.00
11) 2-Chlorophenol-d4	7.304	132	118765	23.341	ng/ul	0.00
15) 4-Methylphenol-d8	8.510	113	109979	20.888	ng/ul	0.00
21) Nitrobenzene-d5	8.993	128	54044m	23.667	ng/ul	0.00
24) 2-Nitrophenol-d4	9.704	143	57729	22.315	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.234	165	96223	20.869	ng/ul	0.00
31) 4-Chloroaniline-d4	10.792	131	103066	16.300	ng/ul	0.00
46) Dimethylphthalate-d6	13.886	166	338454	25.258	ng/ul	0.00
49) Acenaphthylene-d8	14.163	160	344960	23.636	ng/ul	0.00
54) 4-Nitrophenol-d4	14.745	143	20624	10.300	ng/ul	0.01
60) Fluorene-d10	15.469	176	275181	24.874	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.633	200	38618	17.042	ng/ul	0.00
73) Anthracene-d10	17.345	188	434808	25.648	ng/ul	0.00
81) Pyrene-d10	19.604	212	528051	25.989	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.680	264	557105	26.269	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
Data File : BP018188.D
Acq On : 15 Nov 2023 23:54
Operator : MA/JU
Sample : PB157169BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK169

Manual IntegrationsAPPROVED

Quant Time: Nov 16 00:55:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 15 18:13:37 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/16/2023
Supervised By :mohammad ahmed 11/17/2023

