




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
Data File : BP018206.D
Acq On : 16 Nov 2023 10:36
Operator : MA/JU
Sample : PB157171BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK171

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/17/2023
Supervised By :mohammad ahmed 11/17/2023

Quant Time: Nov 16 21:38:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 15 18:13:37 2023
Response via : Initial Calibration

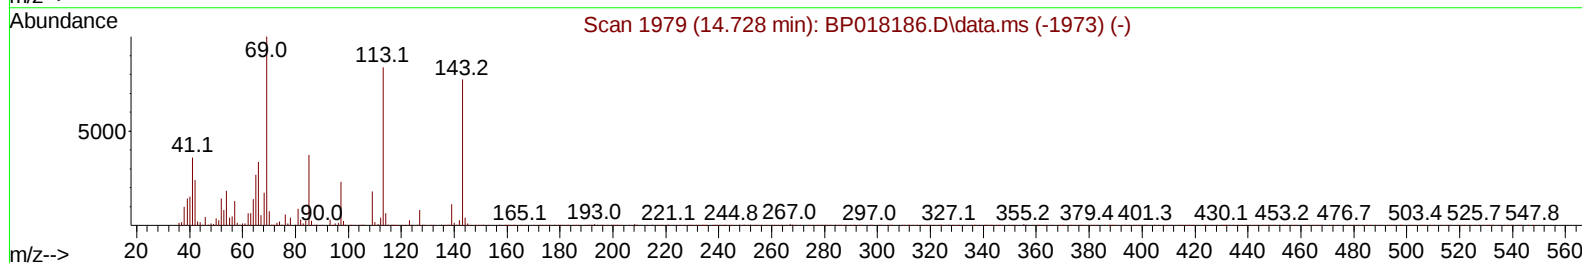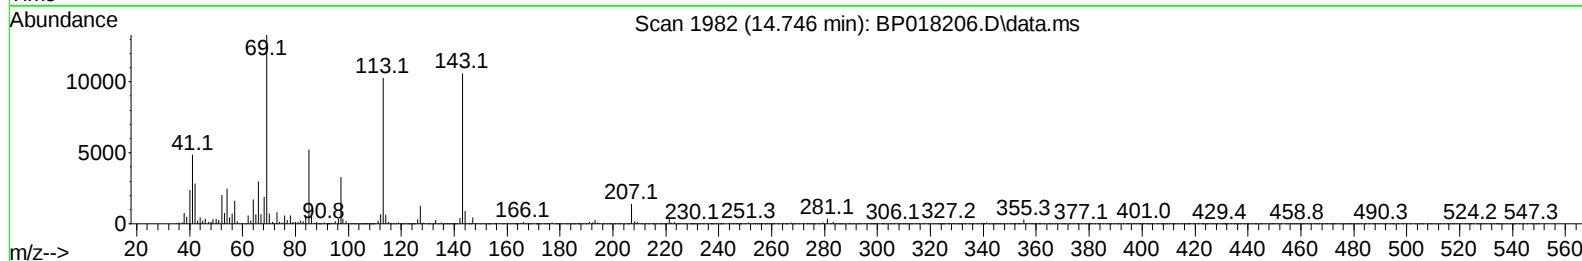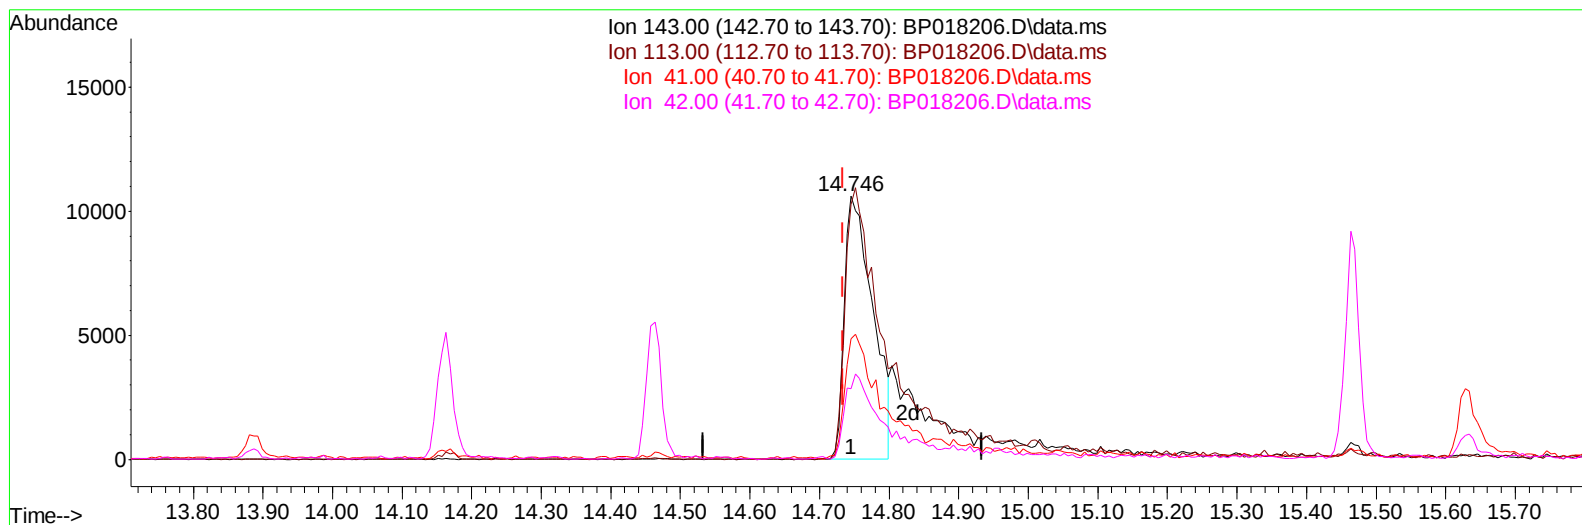

TIC: BP018206.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.746min (+ 0.012) 12.18 ng/u1

response 30056

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.00	96.80
41.00	47.70	45.84
42.00	30.10	26.93




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
Data File : BP018206.D
Acq On : 16 Nov 2023 10:36
Operator : MA/JU
Sample : PB157171BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK171

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/17/2023
Supervised By :mohammad ahmed 11/17/2023

Quant Time: Nov 16 21:38:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 15 18:13:37 2023
Response via : Initial Calibration

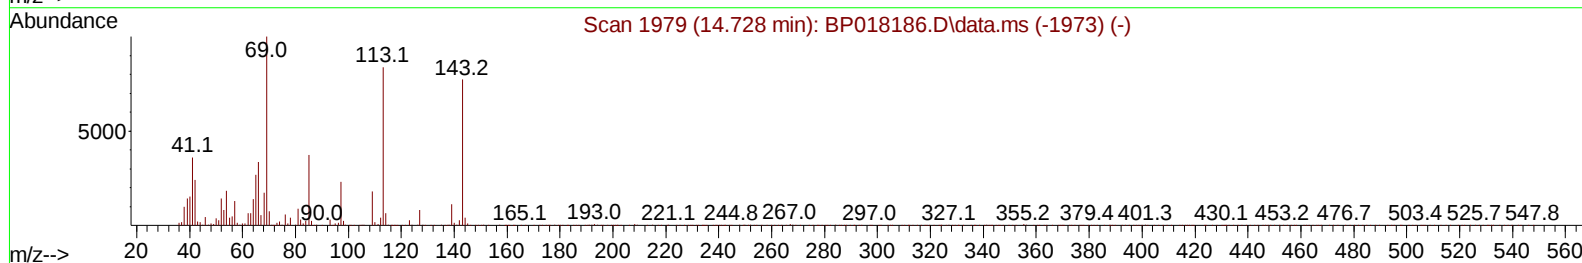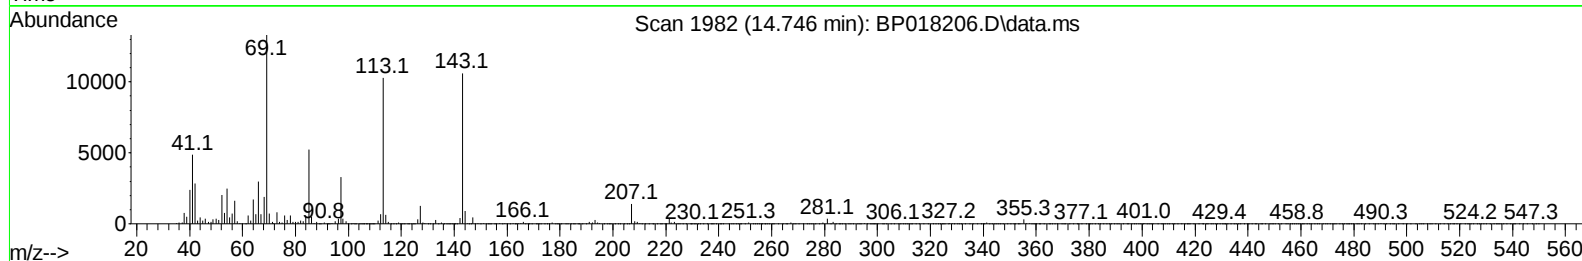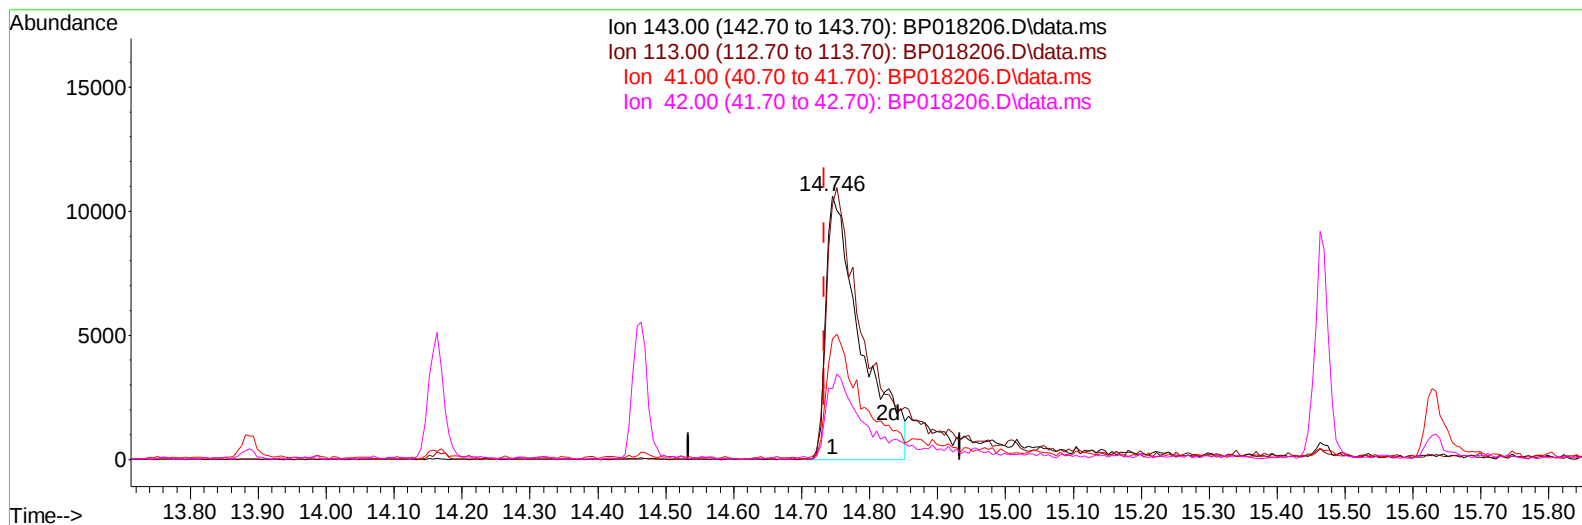

TIC: BP018206.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.746min (+ 0.012) 15.50 ng/ul m

response 38249

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.00	96.80
41.00	47.70	45.84
42.00	30.10	26.93

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
 Data File : BP018206.D
 Acq On : 16 Nov 2023 10:36
 Operator : MA/JU
 Sample : PB157171BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK171

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/17/2023
 Supervised By :mohammad ahmed 11/17/2023

Quant Time: Nov 16 22:01:57 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 15 18:13:37 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.781	152	74303	20.000	ng/ul	0.00
20) Naphthalene-d8	10.599	136	289415	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.463	164	178993	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.245	188	407611	20.000	ng/ul	0.00
79) Chrysene-d12	21.381	240	376081	20.000	ng/ul	0.00
88) Perylene-d12	23.851	264	405816	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	10690	5.075	ng/uL	0.00
4) Pyridine-d5	3.593	84	107069	19.496	ng/ul	0.00
7) Phenol-d5	6.952	99	159156	22.187	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.134	67	105502	25.026	ng/ul	0.00
11) 2-Chlorophenol-d4	7.305	132	132804	23.378	ng/ul	0.00
15) 4-Methylphenol-d8	8.511	113	127928	21.763	ng/ul	0.00
21) Nitrobenzene-d5	8.993	128	62495	23.968	ng/ul	0.00
24) 2-Nitrophenol-d4	9.705	143	68660	23.243	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.234	165	109950	20.883	ng/ul	0.00
31) 4-Chloroaniline-d4	10.793	131	126954	17.583	ng/ul	0.00
46) Dimethylphthalate-d6	13.887	166	422029	25.554	ng/ul	0.00
49) Acenaphthylene-d8	14.163	160	424907	23.622	ng/ul	0.00
54) 4-Nitrophenol-d4	14.746	143	38249m	15.499	ng/ul	0.01
60) Fluorene-d10	15.469	176	341982	25.081	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.628	200	54422	18.469	ng/ul	0.00
73) Anthracene-d10	17.345	188	558438	25.331	ng/ul	0.00
81) Pyrene-d10	19.604	212	671646	26.737	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.686	264	638974	27.079	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
Data File : BP018206.D
Acq On : 16 Nov 2023 10:36
Operator : MA/JU
Sample : PB157171BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK171

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/17/2023
Supervised By :mohammad ahmed 11/17/2023

Quant Time: Nov 16 22:01:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 15 18:13:37 2023
Response via : Initial Calibration

