

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
 Data File : BP018207.D
 Acq On : 16 Nov 2023 11:10
 Operator : MA/JU
 Sample : 05338-23
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCDM6

Quant Time: Nov 16 11:44:32 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 15 18:13:37 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.787	152	59643	20.000	ng/u1	0.00
20) Naphthalene-d8	10.599	136	208055	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.463	164	126885	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.245	188	257919	20.000	ng/u1	0.00
79) Chrysene-d12	21.380	240	242743	20.000	ng/u1	0.00
88) Perylene-d12	23.851	264	288307	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	11420	6.754	ng/uL	0.00
4) Pyridine-d5	3.593	84	126890	28.784	ng/u1	0.00
7) Phenol-d5	6.952	99	188853	32.798	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.134	67	124566	36.812	ng/u1	0.00
11) 2-Chlorophenol-d4	7.305	132	157348	34.507	ng/u1	0.00
15) 4-Methylphenol-d8	8.510	113	153363	32.503	ng/u1	0.00
21) Nitrobenzene-d5	8.993	128	73486	39.204	ng/u1	0.00
24) 2-Nitrophenol-d4	9.704	143	80952	38.120	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.234	165	134889	35.639	ng/u1	0.00
31) 4-Chloroaniline-d4	10.781	131	174100	33.542	ng/u1	0.00
46) Dimethylphthalate-d6	13.887	166	451450	38.561	ng/u1	0.00
49) Acenaphthylene-d8	14.163	160	473691	37.148	ng/u1	0.00
54) 4-Nitrophenol-d4	14.745	143	37889	21.658	ng/u1	0.01
60) Fluorene-d10	15.469	176	369007	38.177	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.628	200	53948	28.933	ng/u1	0.00
73) Anthracene-d10	17.345	188	561862	40.279	ng/u1	0.00
81) Pyrene-d10	19.604	212	663540	40.923	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.686	264	699964	41.753	ng/u1	0.00


Target Compounds				Qvalue	
2) 1,4-Dioxane	3.199	88	6786	3.678 ng/uL#	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
Data File : BP018207.D
Acq On : 16 Nov 2023 11:10
Operator : MA/JU
Sample : 05338-23
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCDM6

Quant Time: Nov 16 11:44:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 15 18:13:37 2023
Response via : Initial Calibration

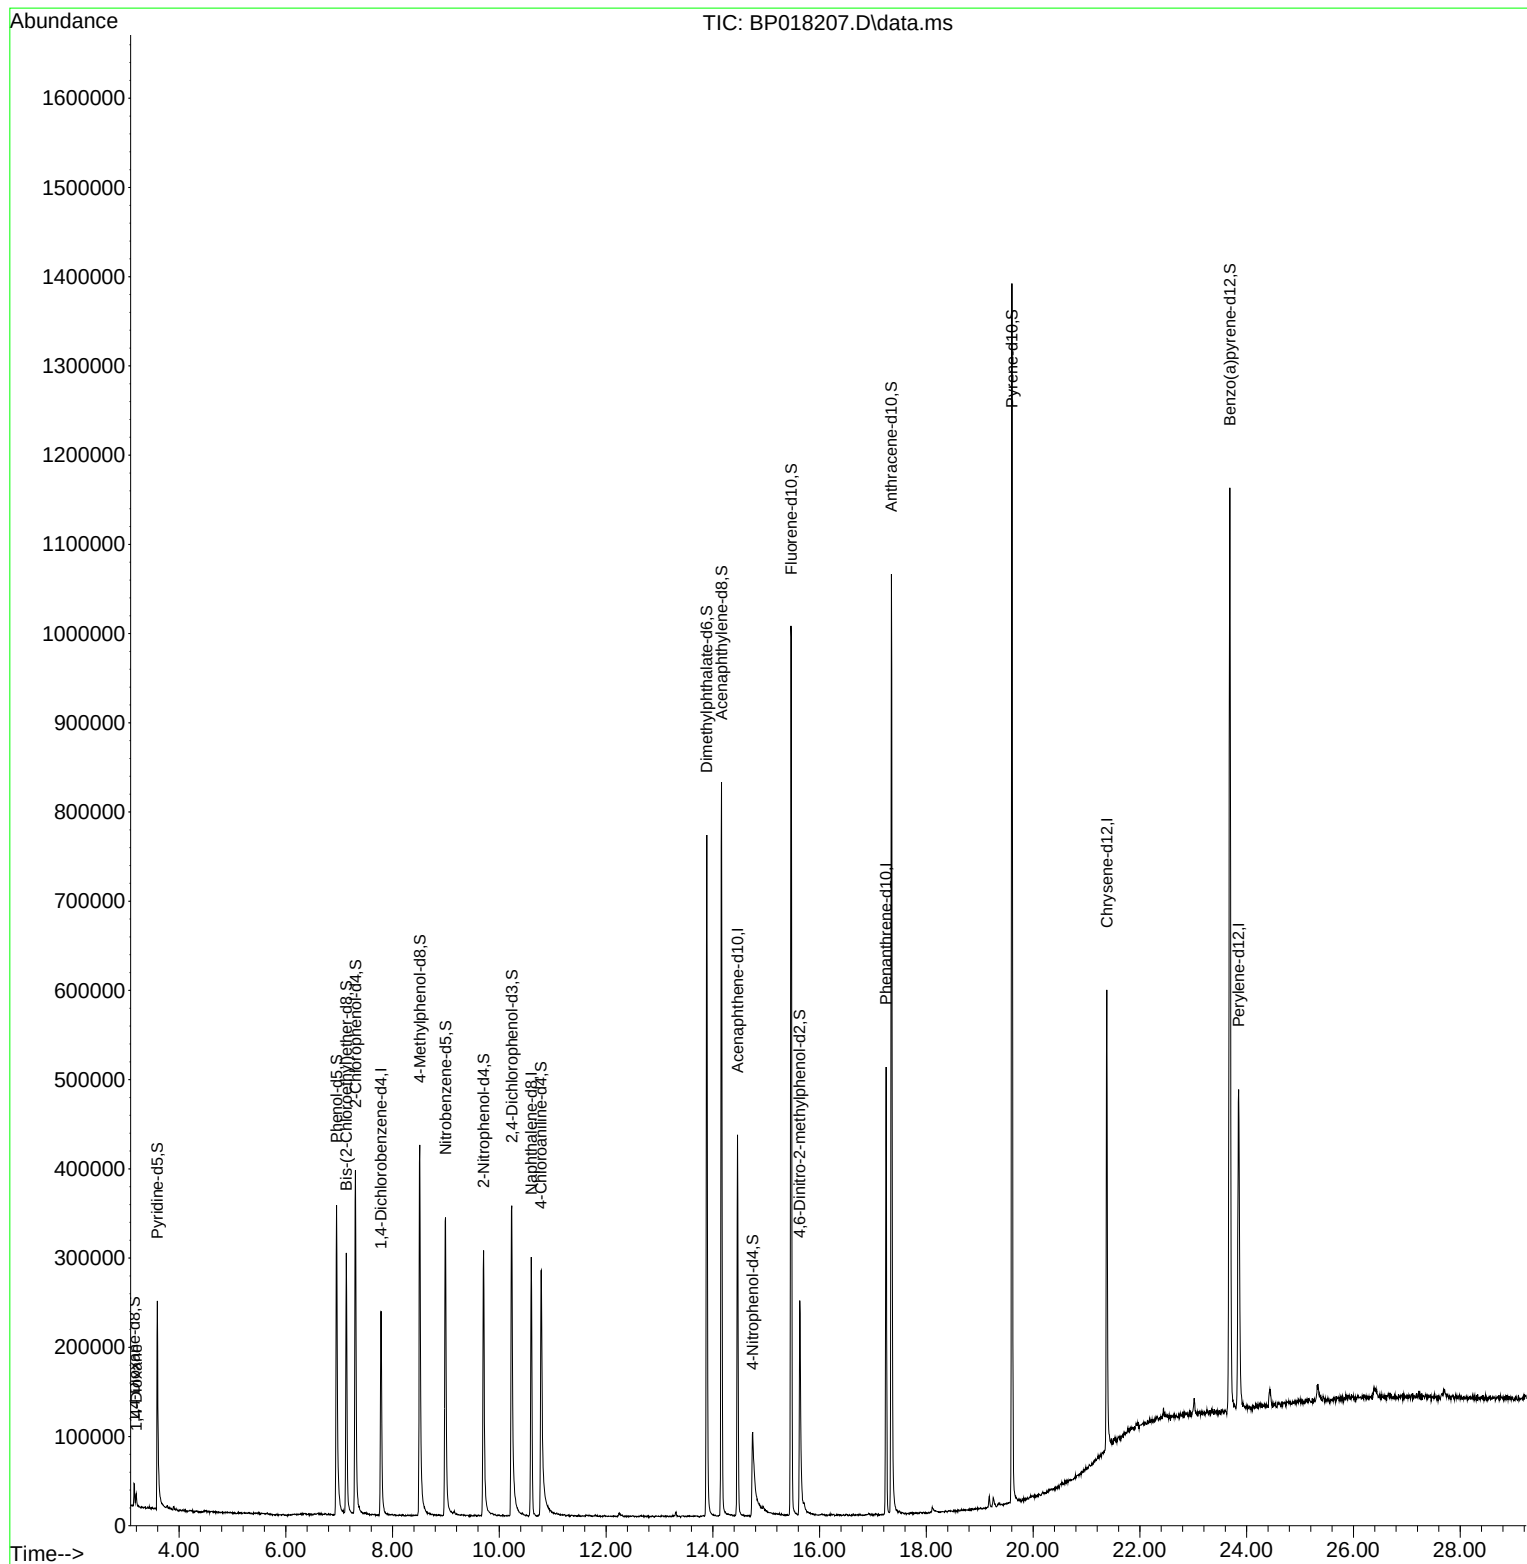

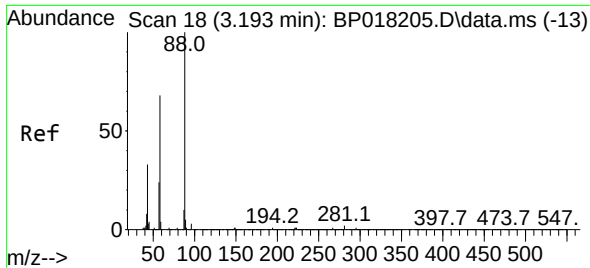

#2
 1,4-Dioxane
 Concen: 3.678 ng/uL
 RT: 3.199 min Scan# 19
 Delta R.T. 0.006 min
 Lab File: BP018207.D
 Acq: 16 Nov 2023 11:10

Instrument :
 BNA_P
 ClientSampleId :
 GCDM6

Tgt Ion: 88 Resp: 6786
 Ion Ratio Lower Upper
 88 100
 43 39.0 25.4 38.2#
 58 68.4 53.3 79.9

