

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
 Data File : BP018176.D
 Acq On : 15 Nov 2023 16:26
 Operator : MA/JU
 Sample : PB156922BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK922

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018176.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.158	9	12	18	rVB	28686	36222	1.93%	0.177%
2	3.593	82	86	97	rBV	238464	391376	20.81%	1.914%
3	3.899	135	138	141	rBV5	6477	8025	0.43%	0.039%
4	5.140	347	349	353	rBV5	1652	2148	0.11%	0.011%
5	5.405	392	394	398	rBV5	1382	2103	0.11%	0.010%
6	5.540	412	417	418	rBV5	1636	2244	0.12%	0.011%
7	5.646	432	435	437	rBV4	2209	2760	0.15%	0.013%
8	6.699	610	614	617	rVB6	2220	3180	0.17%	0.016%
9	6.952	651	657	675	rBV	334242	601832	32.00%	2.943%
10	7.134	682	688	706	rVB	271856	436600	23.22%	2.135%
11	7.305	711	717	737	rVB	366256	624283	33.20%	3.053%
12	7.499	748	750	753	rVB4	1966	1946	0.10%	0.010%
13	7.781	792	798	816	rBV	315766	554233	29.47%	2.710%
14	8.510	916	922	942	rBV	372018	723390	38.47%	3.538%
15	8.993	997	1004	1019	rBV	324741	595922	31.69%	2.914%
16	9.704	1119	1125	1137	rBV	280079	524421	27.89%	2.565%
17	10.010	1173	1177	1182	rVB8	1275	2341	0.12%	0.011%
18	10.234	1208	1215	1242	rBV	315973	719267	38.25%	3.517%
19	10.599	1270	1277	1292	rVB	427129	717042	38.13%	3.507%
20	10.787	1302	1309	1331	rBV	271950	641273	34.10%	3.136%
21	11.687	1459	1462	1468	rBV7	1473	2046	0.11%	0.010%
22	11.746	1468	1472	1475	rVB6	1456	2011	0.11%	0.010%
23	12.251	1553	1558	1559	rBV4	3656	4180	0.22%	0.020%
24	12.640	1620	1624	1626	rBV4	1384	2096	0.11%	0.010%
25	13.310	1732	1738	1742	rBV9	4357	8073	0.43%	0.039%
26	13.569	1778	1782	1784	rBV5	1857	2354	0.13%	0.012%
27	13.675	1797	1800	1803	rVV5	1677	2420	0.13%	0.012%
28	13.887	1829	1836	1851	rBV	715406	1058003	56.26%	5.174%
29	14.163	1877	1883	1902	rBV2	773176	1155773	61.46%	5.652%
30	14.287	1902	1904	1907	rVV4	2389	3262	0.17%	0.016%
31	14.463	1927	1934	1944	rBV	596310	883962	47.01%	4.323%
32	14.751	1975	1983	1999	rBV3	77195	290768	15.46%	1.422%
33	14.981	2020	2022	2025	rVB4	2198	2115	0.11%	0.010%
34	15.239	2064	2066	2069	rBV4	1722	1911	0.10%	0.009%
35	15.469	2098	2105	2121	rBV	1017072	1442526	76.71%	7.054%
36	15.634	2127	2133	2144	rBV	195400	363452	19.33%	1.777%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
 Data File : BP018176.D
 Acq On : 15 Nov 2023 16:26
 Operator : MA/JU
 Sample : PB156922BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK922

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

37	16.063	2201	2206	2211	rVB9	1705	2463	0.13%	0.012%
38	16.657	2305	2307	2309	rBV3	1627	1909	0.10%	0.009%
39	16.881	2342	2345	2347	rBV4	1668	2258	0.12%	0.011%
40	16.928	2350	2353	2354	rVV3	2613	2691	0.14%	0.013%
41	17.051	2370	2374	2378	rBV7	2352	4467	0.24%	0.022%
42	17.245	2400	2407	2417	rBV	738869	1031579	54.85%	5.045%
43	17.345	2418	2424	2443	rVV	976260	1482525	78.83%	7.250%
44	17.675	2478	2480	2487	rVB7	1658	2928	0.16%	0.014%
45	17.881	2513	2515	2518	rBV3	2141	2316	0.12%	0.011%
46	18.028	2536	2540	2544	rBV7	2063	3548	0.19%	0.017%
47	18.104	2549	2553	2565	rVV7	14987	35740	1.90%	0.175%
48	19.133	2726	2728	2730	rBV3	3335	3203	0.17%	0.016%
49	19.180	2732	2736	2742	rVV4	13221	20917	1.11%	0.102%
50	19.257	2743	2749	2754	rVV2	14969	30683	1.63%	0.150%
51	19.351	2762	2765	2771	rBV6	6330	11503	0.61%	0.056%
52	19.480	2783	2787	2791	rBV2	34390	39773	2.11%	0.195%
53	19.604	2802	2808	2821	rBV	1324096	1733935	92.20%	8.479%
54	20.304	2924	2927	2932	rBV7	7335	13248	0.70%	0.065%
55	20.510	2959	2962	2966	rBV3	23059	27782	1.48%	0.136%
56	21.380	3105	3110	3122	rBV	796201	1116321	59.36%	5.459%
57	23.686	3495	3502	3514	rVB2	941648	1880560	100.00%	9.197%
58	23.851	3523	3530	3545	rVB	534326	1182733	62.89%	5.784%




Sum of corrected areas: 20448642

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
Data File : BP018176.D
Acq On : 15 Nov 2023 16:26
Operator : MA/JU
Sample : PB156922BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK922

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

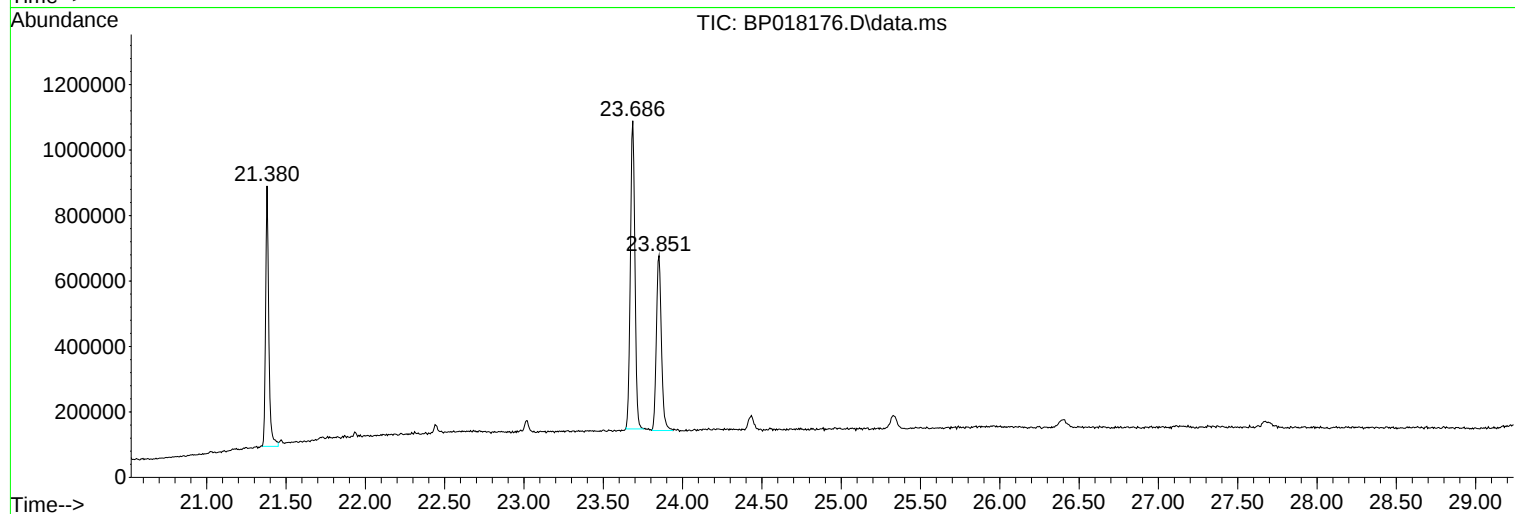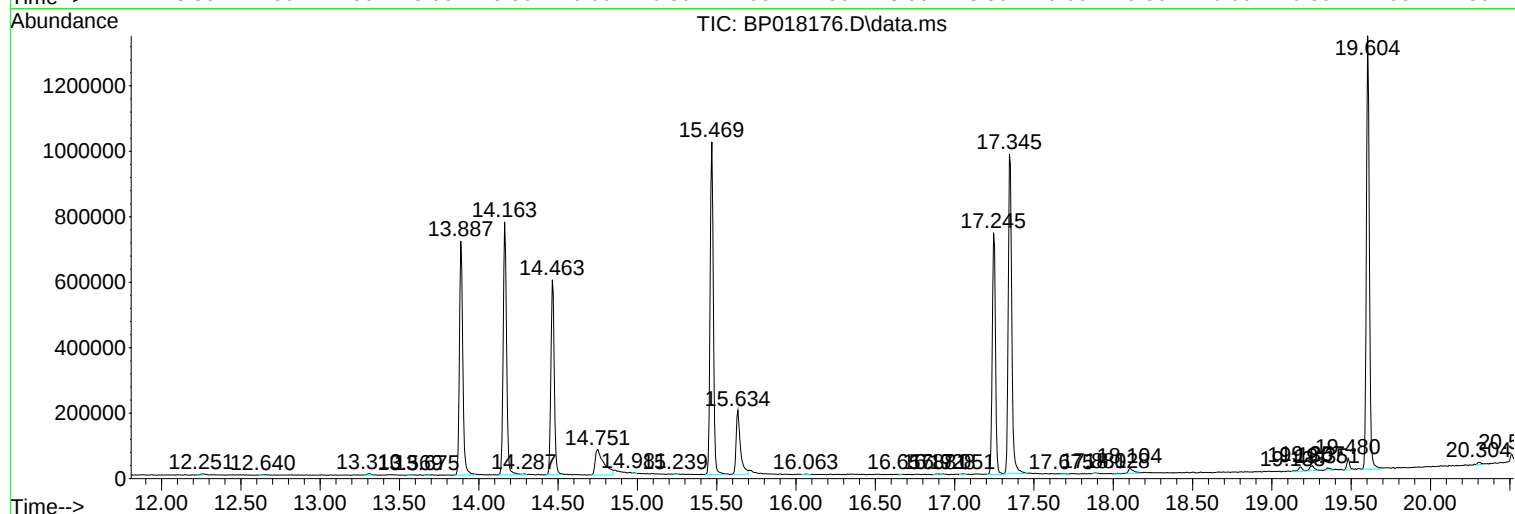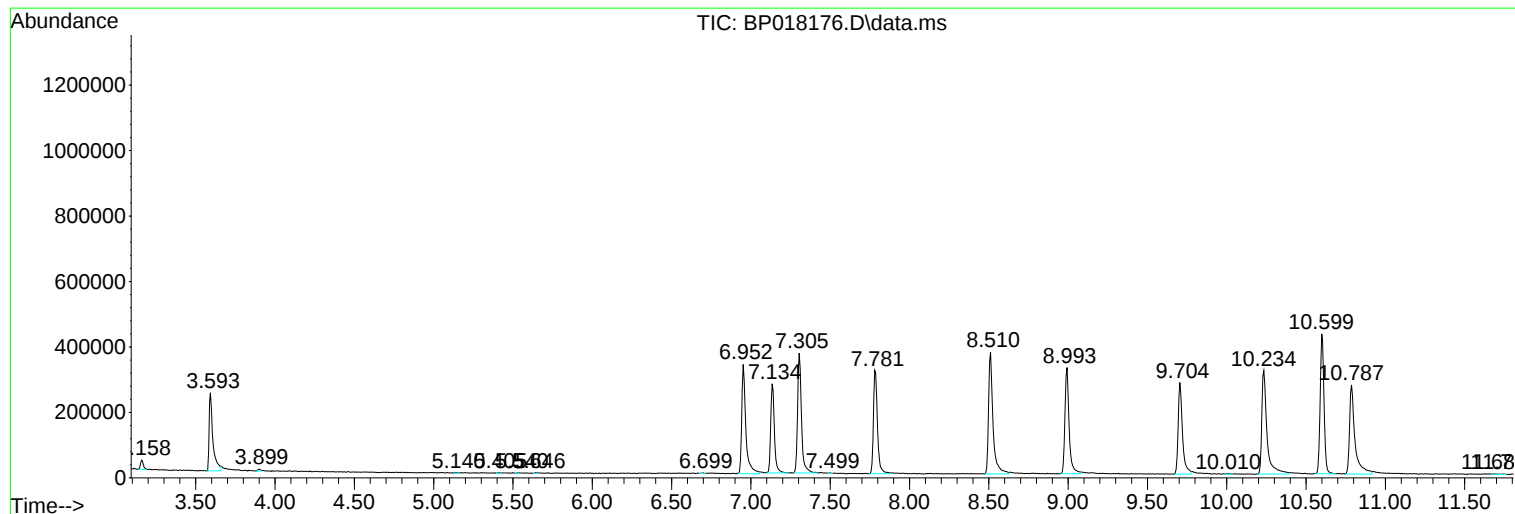

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
Data File : BP018176.D
Acq On : 15 Nov 2023 16:26
Operator : MA/JU
Sample : PB156922BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK922

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
Data File : BP018176.D
Acq On : 15 Nov 2023 16:26
Operator : MA/JU
Sample : PB156922BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK922

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------