

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
 Data File : BP018177.D
 Acq On : 15 Nov 2023 17:08
 Operator : MA/JU
 Sample : PB156906TB 10X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SLEB906

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018177.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.158	9	12	20	rBV	25730	32201	1.71%	0.170%
2	3.593	82	86	106	rBV	220545	379328	20.13%	2.007%
3	3.899	135	138	144	rVB3	4783	8193	0.43%	0.043%
4	4.605	254	258	259	rBV2	3268	2626	0.14%	0.014%
5	6.187	523	527	530	rVB5	1502	2064	0.11%	0.011%
6	6.952	651	657	673	rBV	305146	538993	28.60%	2.852%
7	7.134	680	688	706	rVB	252196	396739	21.05%	2.100%
8	7.305	711	717	733	rBV	341520	568559	30.17%	3.009%
9	7.787	792	799	814	rBV	284959	502302	26.65%	2.658%
10	8.511	915	922	944	rBV	331713	646003	34.28%	3.419%
11	8.993	997	1004	1018	rBV	283469	528715	28.06%	2.798%
12	9.705	1119	1125	1146	rBV	248976	481680	25.56%	2.549%
13	10.234	1208	1215	1230	rBV	292461	617410	32.76%	3.267%
14	10.446	1249	1251	1255	rVB5	1773	2281	0.12%	0.012%
15	10.605	1269	1278	1290	rBV	378659	636370	33.77%	3.368%
16	10.787	1303	1309	1333	rBV	239053	556512	29.53%	2.945%
17	11.622	1448	1451	1453	rVV4	2309	2992	0.16%	0.016%
18	12.252	1554	1558	1559	rBV3	3383	4345	0.23%	0.023%
19	12.269	1559	1561	1564	rVV4	3249	4216	0.22%	0.022%
20	13.057	1690	1695	1698	rBV6	1312	2223	0.12%	0.012%
21	13.310	1734	1738	1745	rBV9	4212	6488	0.34%	0.034%
22	13.675	1796	1800	1805	rVB8	1905	2952	0.16%	0.016%
23	13.893	1831	1837	1855	rVV	654620	954049	50.63%	5.049%
24	14.169	1877	1884	1899	rBV	664987	1016655	53.95%	5.380%
25	14.381	1917	1920	1924	rVB6	1846	2554	0.14%	0.014%
26	14.469	1928	1935	1947	rBV	536134	779172	41.35%	4.123%
27	14.581	1952	1954	1959	rVV6	1918	3191	0.17%	0.017%
28	14.751	1975	1983	2002	rBV2	78254	288373	15.30%	1.526%
29	15.098	2039	2042	2049	rVB9	2642	5037	0.27%	0.027%
30	15.469	2097	2105	2117	rBV	889875	1278492	67.84%	6.766%
31	15.634	2127	2133	2144	rBV	197617	347198	18.42%	1.837%
32	16.322	2246	2250	2252	rBV5	2290	3040	0.16%	0.016%
33	16.445	2266	2271	2272	rBV5	1501	1915	0.10%	0.010%
34	16.504	2278	2281	2285	rVV5	2081	2954	0.16%	0.016%
35	17.057	2370	2375	2380	rBV8	2086	4042	0.21%	0.021%
36	17.140	2388	2389	2396	rVB6	2126	3075	0.16%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
 Data File : BP018177.D
 Acq On : 15 Nov 2023 17:08
 Operator : MA/JU
 Sample : PB156906TB 10X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SLEB906

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

37	17.251	2402	2408	2419	rBV	679263	939688	49.86%	4.973%
38	17.351	2419	2425	2440	rVV2	922035	1361046	72.22%	7.203%
39	17.451	2440	2442	2445	rVV4	3932	5203	0.28%	0.028%
40	17.722	2483	2488	2490	rBV6	1207	1917	0.10%	0.010%
41	17.881	2509	2515	2520	rBV9	3938	7867	0.42%	0.042%
42	18.104	2548	2553	2561	rBV5	23945	50528	2.68%	0.267%
43	18.557	2626	2630	2632	rBV5	1561	2075	0.11%	0.011%
44	18.663	2645	2648	2651	rBV5	2934	4565	0.24%	0.024%
45	19.181	2733	2736	2741	rVB4	11089	13376	0.71%	0.071%
46	19.251	2744	2748	2754	rVV3	13081	23429	1.24%	0.124%
47	19.351	2762	2765	2770	rBV6	11672	18527	0.98%	0.098%
48	19.481	2783	2787	2792	rBV3	34072	41683	2.21%	0.221%
49	19.610	2803	2809	2819	rBV	1237446	1657392	87.95%	8.771%
50	20.516	2959	2963	2969	rBV4	27261	42108	2.23%	0.223%
51	21.380	3105	3110	3121	rBV	751673	1068743	56.71%	5.656%
52	23.692	3495	3503	3512	rBV	967260	1884523	100.00%	9.973%
53	23.857	3524	3531	3546	rVB	537966	1160886	61.60%	6.143%




Sum of corrected areas: 18896495

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
Data File : BP018177.D
Acq On : 15 Nov 2023 17:08
Operator : MA/JU
Sample : PB156906TB 10X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB906

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

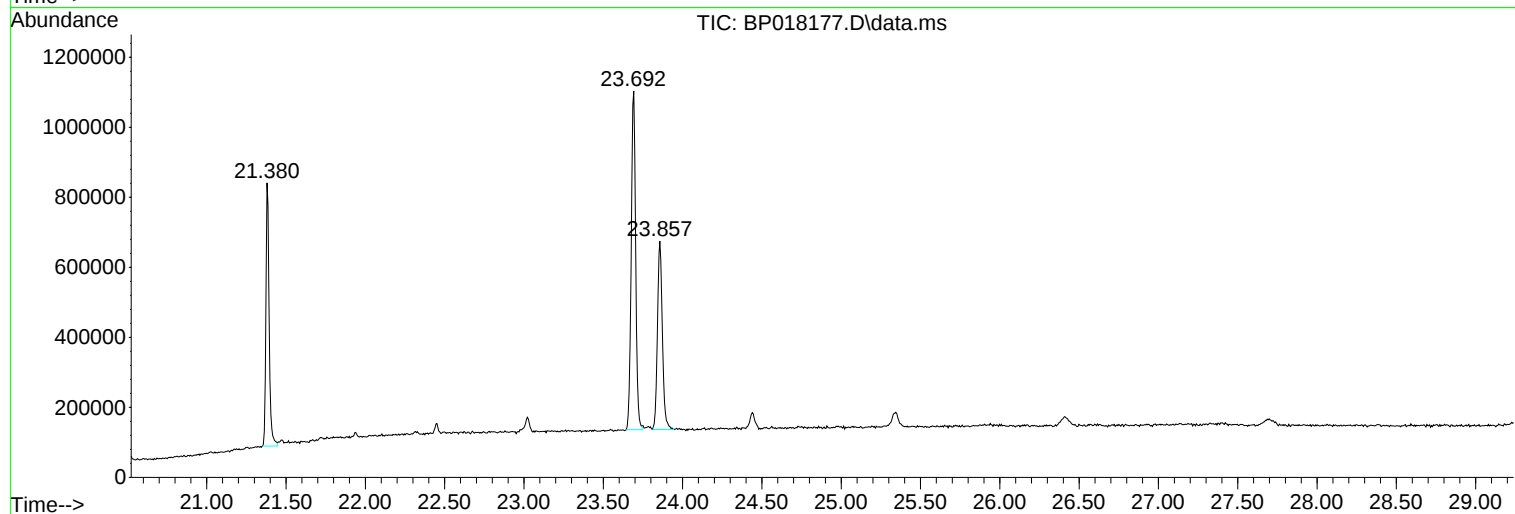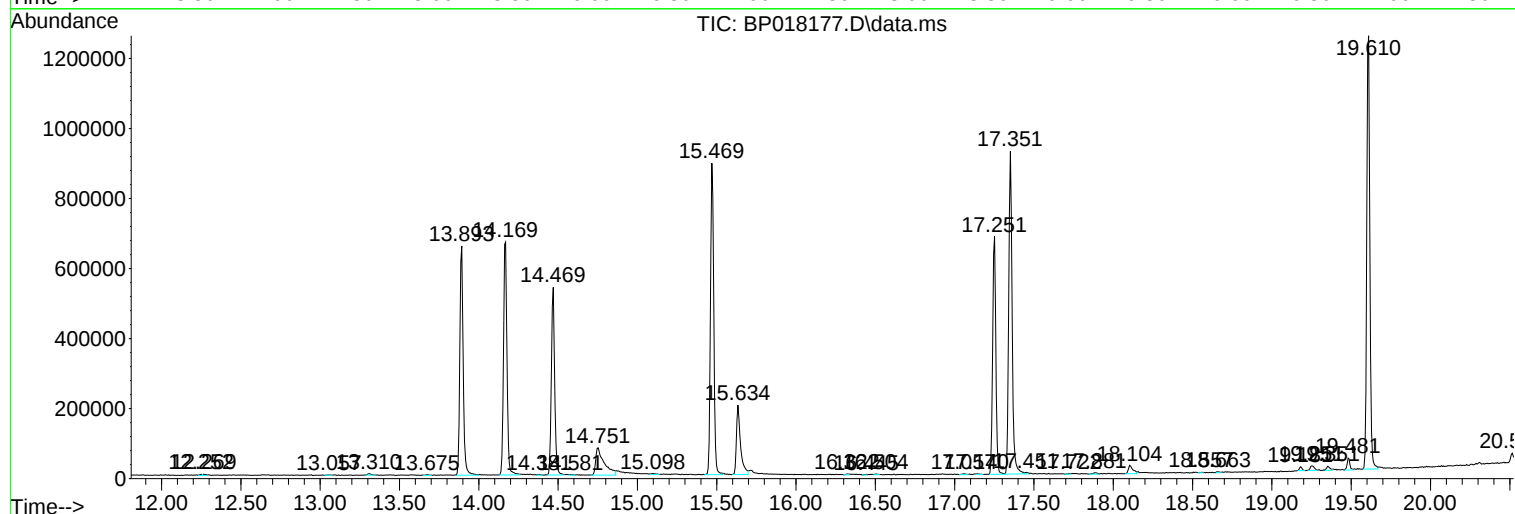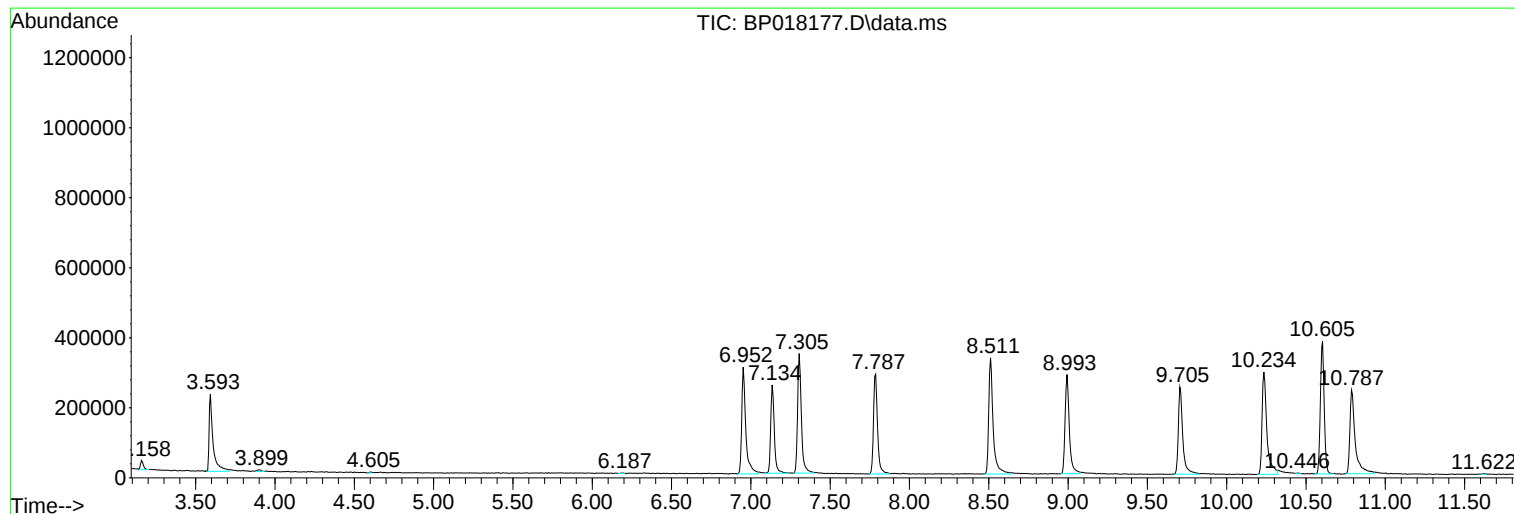

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
Data File : BP018177.D
Acq On : 15 Nov 2023 17:08
Operator : MA/JU
Sample : PB156906TB 10X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB906

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
Data File : BP018177.D
Acq On : 15 Nov 2023 17:08
Operator : MA/JU
Sample : PB156906TB 10X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB906

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc