

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
 Data File : BP018185.D
 Acq On : 15 Nov 2023 21:38
 Operator : MA/JU
 Sample : PB157123BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK123

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018185.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.158	9	12	19	rVB	22778	30341	2.03%	0.201%
2	3.381	48	50	52	rBV3	2156	1606	0.11%	0.011%
3	3.593	83	86	101	rBV	155722	274862	18.41%	1.821%
4	3.758	112	114	117	rVB4	2127	1796	0.12%	0.012%
5	3.899	136	138	142	rVB5	3994	4519	0.30%	0.030%
6	4.093	169	171	175	rVB5	2361	1794	0.12%	0.012%
7	4.128	175	177	180	rVB4	2082	1991	0.13%	0.013%
8	4.170	182	184	189	rVB6	1899	2523	0.17%	0.017%
9	4.222	191	193	196	rBV3	2197	1984	0.13%	0.013%
10	4.664	266	268	271	rVB4	2050	1942	0.13%	0.013%
11	4.687	271	272	275	rBV3	1749	1635	0.11%	0.011%
12	5.105	342	343	350	rVB6	1956	2032	0.14%	0.013%
13	6.128	515	517	522	rVV6	1204	1728	0.12%	0.011%
14	6.322	548	550	553	rBV4	1416	1859	0.12%	0.012%
15	6.952	649	657	681	rBV	226276	455504	30.50%	3.017%
16	7.134	682	688	703	rVB	204037	331055	22.17%	2.193%
17	7.305	710	717	731	rBV	273222	479966	32.14%	3.179%
18	7.558	757	760	764	rVV6	1254	1960	0.13%	0.013%
19	7.787	792	799	817	rVV	207971	381693	25.56%	2.528%
20	8.146	859	860	865	rVB5	1407	1748	0.12%	0.012%
21	8.510	915	922	939	rBV	271515	537032	35.96%	3.557%
22	8.781	965	968	970	rVB4	1494	1565	0.10%	0.010%
23	8.993	998	1004	1017	rBV	234007	448000	30.00%	2.967%
24	9.599	1105	1107	1111	rVB5	1456	1540	0.10%	0.010%
25	9.705	1119	1125	1147	rBV	195764	401874	26.91%	2.662%
26	10.234	1207	1215	1240	rVV	217999	536675	35.94%	3.555%
27	10.405	1242	1244	1248	rVB4	3428	4610	0.31%	0.031%
28	10.599	1271	1277	1295	rVB	274569	481953	32.28%	3.192%
29	10.793	1303	1310	1330	rBV	143737	391870	26.24%	2.595%
30	11.216	1379	1382	1385	rVB5	2257	2831	0.19%	0.019%
31	11.322	1399	1400	1404	rVB4	1702	1726	0.12%	0.011%
32	11.969	1508	1510	1513	rVB4	1577	1584	0.11%	0.010%
33	12.016	1513	1518	1519	rBV5	1329	1779	0.12%	0.012%
34	12.257	1555	1559	1560	rBV4	2257	2341	0.16%	0.016%
35	12.457	1590	1593	1596	rVB5	1670	2115	0.14%	0.014%
36	12.516	1600	1603	1609	rVB8	1506	2857	0.19%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
 Data File : BP018185.D
 Acq On : 15 Nov 2023 21:38
 Operator : MA/JU
 Sample : PB157123BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK123

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

37	12.675	1627	1630	1633	rBV5	1332	1524	0.10%	0.010%
38	12.763	1644	1645	1650	rVB5	1166	1504	0.10%	0.010%
39	13.051	1690	1694	1700	rVB9	1216	2635	0.18%	0.017%
40	13.104	1700	1703	1706	rBV5	1135	1628	0.11%	0.011%
41	13.234	1721	1725	1727	rVB5	1339	1930	0.13%	0.013%
42	13.275	1727	1732	1733	rBV4	1244	1658	0.11%	0.011%
43	13.304	1733	1737	1744	rVV9	4577	8153	0.55%	0.054%
44	13.446	1757	1761	1763	rVB5	1428	1625	0.11%	0.011%
45	13.887	1830	1836	1853	rVV	548313	819606	54.89%	5.429%
46	14.163	1874	1883	1892	rBV2	591401	871821	58.38%	5.774%
47	14.463	1926	1934	1948	rBV	400786	589643	39.49%	3.905%
48	14.757	1977	1984	1996	rBV2	48023	175976	11.78%	1.166%
49	15.469	2097	2105	2121	rBV	740902	1102858	73.86%	7.305%
50	15.634	2127	2133	2144	rBV	140571	273165	18.29%	1.809%
51	15.981	2190	2192	2195	rVB4	1353	1537	0.10%	0.010%
52	16.022	2195	2199	2202	rVB5	1589	2327	0.16%	0.015%
53	16.045	2202	2203	2206	rBV3	1666	1847	0.12%	0.012%
54	16.104	2212	2213	2218	rBV5	1872	2198	0.15%	0.015%
55	16.757	2322	2324	2327	rVB4	1578	1884	0.13%	0.012%
56	16.881	2341	2345	2347	rBV5	1232	1783	0.12%	0.012%
57	17.128	2382	2387	2389	rBV6	1709	2598	0.17%	0.017%
58	17.245	2401	2407	2418	rBV	493739	691775	46.33%	4.582%
59	17.345	2418	2424	2442	rVV	779463	1185410	79.38%	7.851%
60	17.569	2460	2462	2466	rBV4	1281	1538	0.10%	0.010%
61	17.757	2491	2494	2498	rVB6	1943	2484	0.17%	0.016%
62	17.881	2513	2515	2522	rVB8	1954	3163	0.21%	0.021%
63	17.945	2524	2526	2529	rVB4	1489	1566	0.10%	0.010%
64	17.986	2530	2533	2536	rBV5	1277	1764	0.12%	0.012%
65	18.110	2548	2554	2561	rBV10	9026	24163	1.62%	0.160%
66	18.404	2602	2604	2609	rBV6	2287	3032	0.20%	0.020%
67	18.645	2643	2645	2647	rBV3	2472	2611	0.17%	0.017%
68	18.933	2692	2694	2696	rBV3	2183	2592	0.17%	0.017%
69	19.175	2732	2735	2739	rVB4	9197	13265	0.89%	0.088%
70	19.257	2746	2749	2754	rVB4	6502	9503	0.64%	0.063%
71	19.357	2762	2766	2769	rBV5	4569	7762	0.52%	0.051%
72	19.604	2802	2808	2824	rBV	1048284	1420621	95.14%	9.409%
73	21.380	3105	3110	3121	rBV	519075	768356	51.45%	5.089%
74	23.680	3494	3501	3514	rVB	781886	1493265	100.00%	9.890%
75	23.851	3523	3530	3541	rVB	358371	794397	53.20%	5.262%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
Data File : BP018185.D
Acq On : 15 Nov 2023 21:38
Operator : MA/JU
Sample : PB157123BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK123

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 15098057

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
Data File : BP018185.D
Acq On : 15 Nov 2023 21:38
Operator : MA/JU
Sample : PB157123BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK123

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

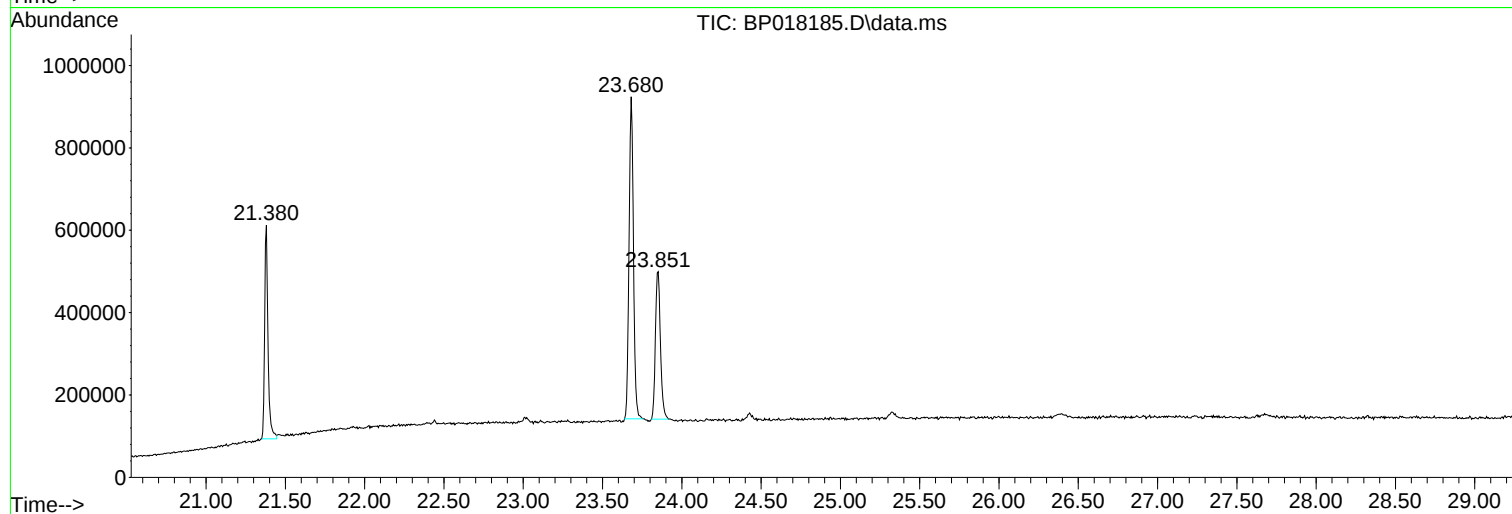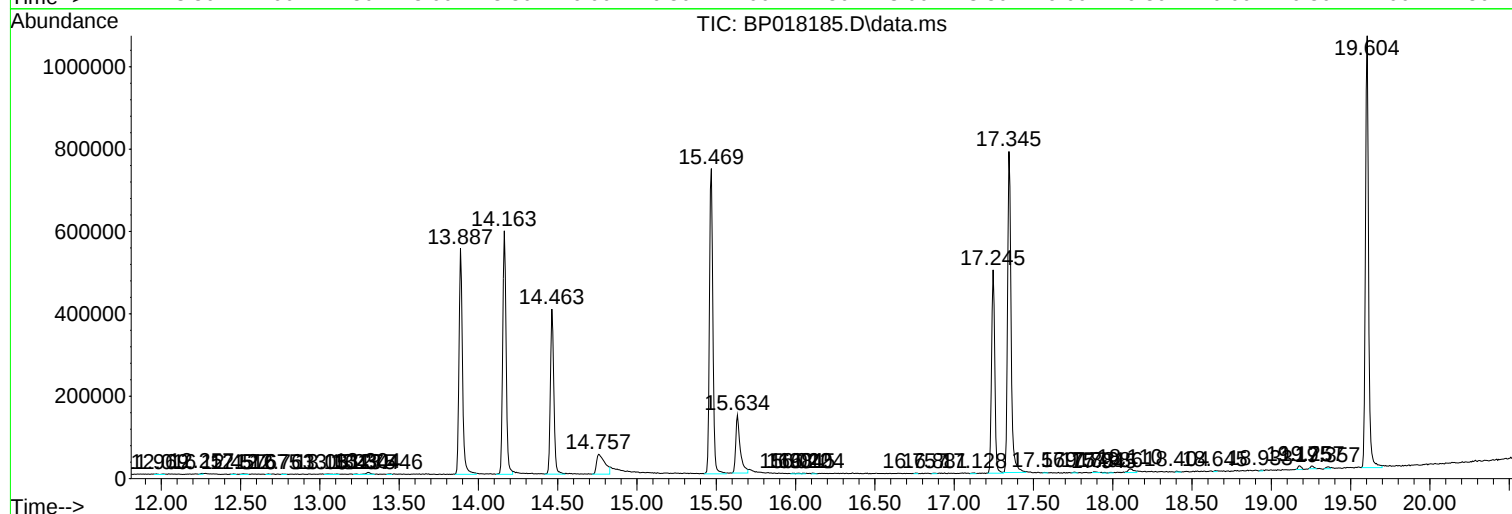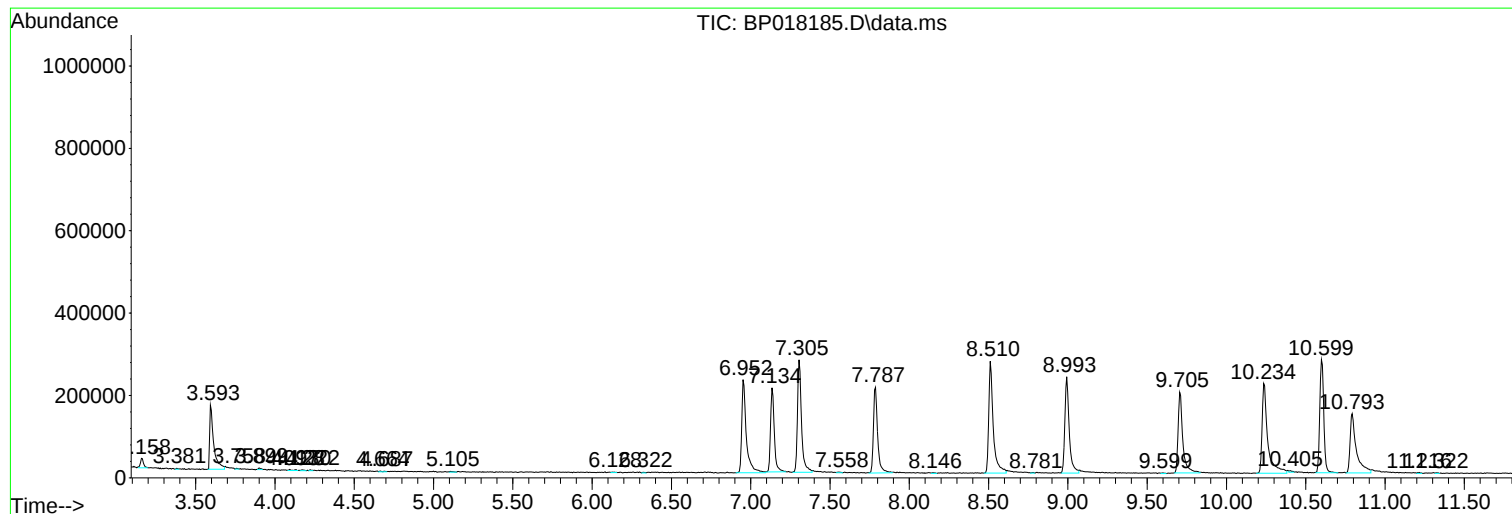

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
Data File : BP018185.D
Acq On : 15 Nov 2023 21:38
Operator : MA/JU
Sample : PB157123BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK123

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
Data File : BP018185.D
Acq On : 15 Nov 2023 21:38
Operator : MA/JU
Sample : PB157123BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK123

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------