

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
 Data File : BP018187.D
 Acq On : 15 Nov 2023 23:20
 Operator : MA/JU
 Sample : PB157167BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK167

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018187.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.158	9	12	17	rBV	32024	38470	1.83%	0.171%
2	3.593	82	86	103	rBV	288732	493461	23.47%	2.193%
3	3.905	135	139	143	rVB6	5932	8639	0.41%	0.038%
4	5.681	436	441	444	rBV6	1388	2476	0.12%	0.011%
5	6.493	573	579	584	rVB10	1928	4501	0.21%	0.020%
6	6.758	621	624	628	rVB5	2315	4422	0.21%	0.020%
7	6.840	634	638	641	rVB6	1806	2641	0.13%	0.012%
8	6.952	651	657	678	rVV	376030	674231	32.07%	2.996%
9	7.134	682	688	704	rVV	316584	492567	23.43%	2.189%
10	7.305	710	717	731	rBV	425955	710000	33.78%	3.155%
11	7.781	791	798	814	rBV	326914	574501	27.33%	2.553%
12	8.510	914	922	940	rBV	412866	801157	38.11%	3.560%
13	8.710	954	956	962	rVB6	2038	2436	0.12%	0.011%
14	8.993	997	1004	1021	rBV	355729	671232	31.93%	2.983%
15	9.704	1117	1125	1146	rBV	306355	595575	28.33%	2.647%
16	9.834	1146	1147	1152	rVB5	1796	2263	0.11%	0.010%
17	10.228	1207	1214	1234	rBV	369450	805946	38.34%	3.582%
18	10.599	1270	1277	1289	rBV	432017	725515	34.51%	3.224%
19	10.781	1302	1308	1330	rBV	315744	723959	34.44%	3.217%
20	10.957	1336	1338	1346	rVB9	3431	6608	0.31%	0.029%
21	11.098	1359	1362	1365	rVV4	1721	2113	0.10%	0.009%
22	11.240	1382	1386	1388	rBV5	1757	2242	0.11%	0.010%
23	11.563	1436	1441	1443	rBV5	1458	2174	0.10%	0.010%
24	12.263	1551	1560	1565	rBV5	3831	11266	0.54%	0.050%
25	12.704	1632	1635	1638	rBV4	1799	2372	0.11%	0.011%
26	13.304	1732	1737	1741	rBV6	6479	10990	0.52%	0.049%
27	13.887	1830	1836	1850	rBV	830272	1173831	55.84%	5.216%
28	13.981	1850	1852	1857	rVB6	2237	3162	0.15%	0.014%
29	14.163	1875	1883	1900	rBV	847686	1293136	61.52%	5.747%
30	14.463	1927	1934	1950	rVV	607079	888186	42.25%	3.947%
31	14.739	1974	1981	2005	rBV2	99944	377336	17.95%	1.677%
32	15.028	2028	2030	2035	rVB6	1987	3308	0.16%	0.015%
33	15.363	2084	2087	2090	rBV5	1514	2300	0.11%	0.010%
34	15.469	2098	2105	2115	rBV	1093729	1577706	75.05%	7.011%
35	15.628	2126	2132	2144	rBV	249946	451622	21.48%	2.007%
36	15.828	2164	2166	2170	rVB5	2242	2232	0.11%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
 Data File : BP018187.D
 Acq On : 15 Nov 2023 23:20
 Operator : MA/JU
 Sample : PB157167BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK167

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

37	16.257	2235	2239	2247	rVB10	2854	6563	0.31%	0.029%
38	16.334	2247	2252	2254	rBV6	2681	4582	0.22%	0.020%
39	16.828	2334	2336	2343	rVB8	1548	2369	0.11%	0.011%
40	16.910	2347	2350	2355	rBV7	1601	2806	0.13%	0.012%
41	17.245	2401	2407	2418	rBV	746874	1049318	49.92%	4.663%
42	17.345	2418	2424	2444	rVV	1155872	1714003	81.54%	7.617%
43	18.110	2549	2554	2556	rBV5	9424	13876	0.66%	0.062%
44	18.780	2666	2668	2672	rBV5	1521	2247	0.11%	0.010%
45	19.175	2730	2735	2740	rBV2	14598	19463	0.93%	0.086%
46	19.257	2745	2749	2758	rVB2	10905	19283	0.92%	0.086%
47	19.351	2763	2765	2768	rBV4	3194	4182	0.20%	0.019%
48	19.604	2802	2808	2823	rBV	1529131	2024822	96.32%	8.998%
49	21.374	3104	3109	3122	rBV	843105	1193022	56.75%	5.302%
50	23.680	3494	3501	3513	rBV	1066759	2102097	100.00%	9.341%
51	23.845	3522	3529	3544	rVB	543084	1199573	57.07%	5.331%




Sum of corrected areas: 22502782

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
Data File : BP018187.D
Acq On : 15 Nov 2023 23:20
Operator : MA/JU
Sample : PB157167BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK167

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

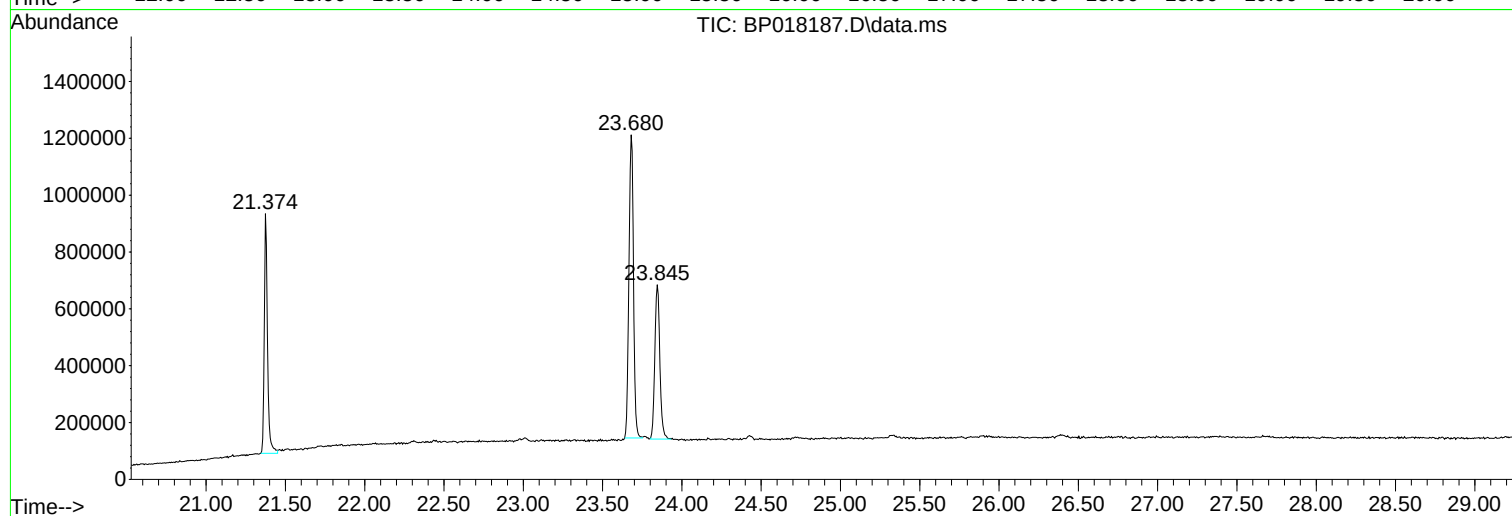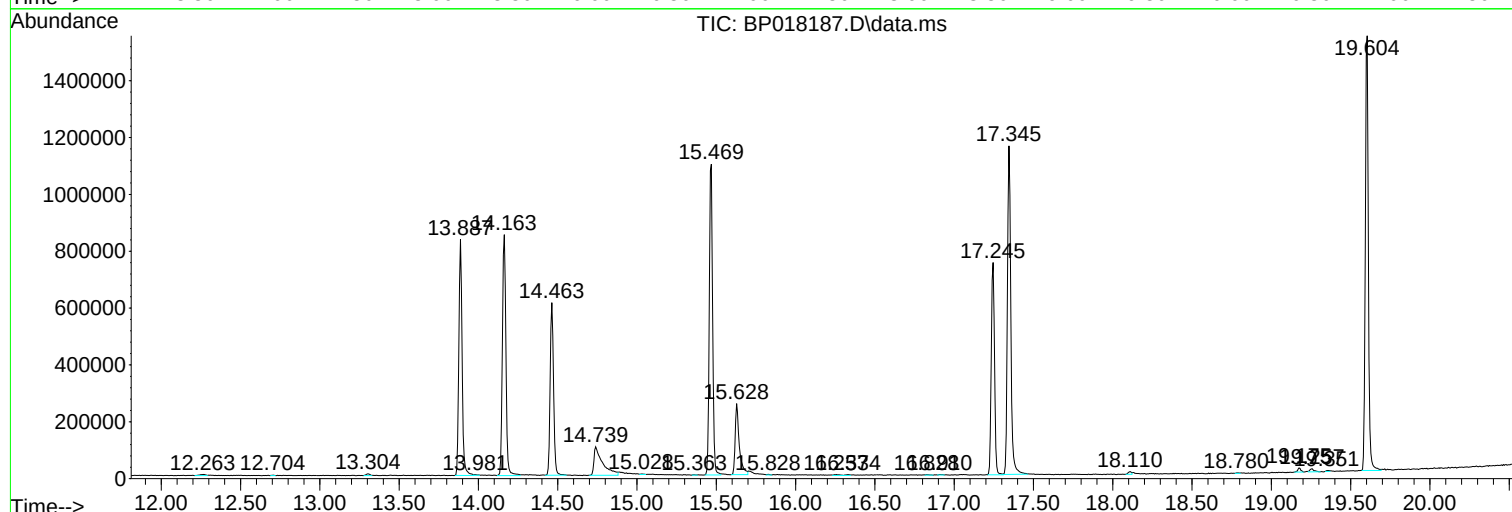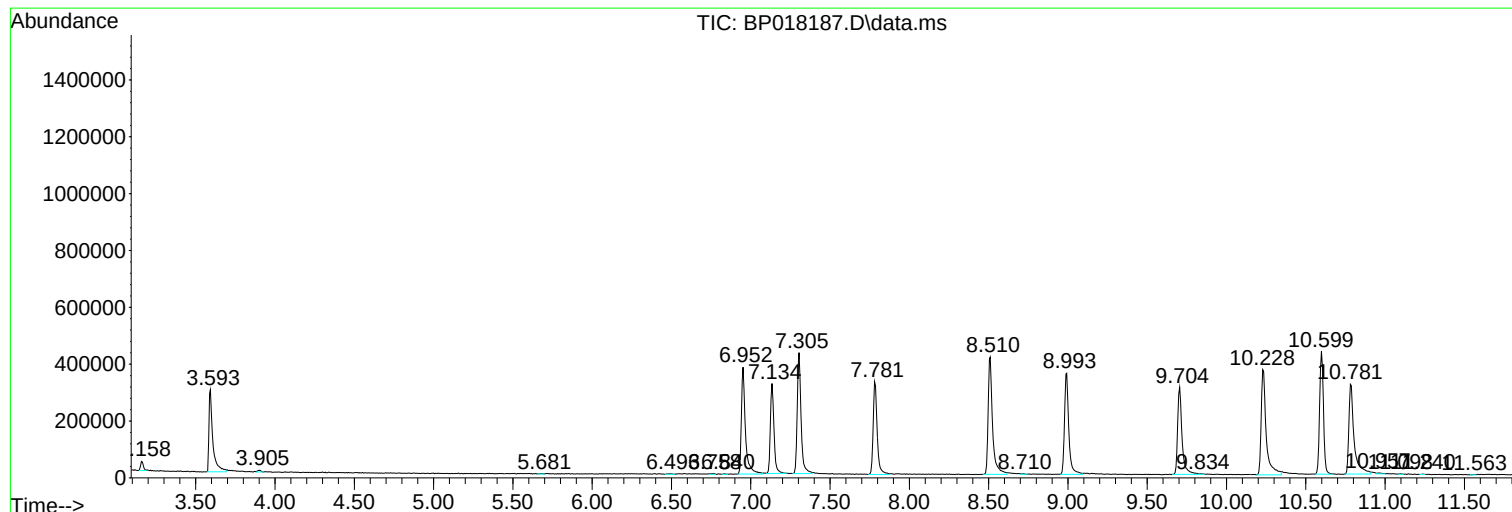

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
Data File : BP018187.D
Acq On : 15 Nov 2023 23:20
Operator : MA/JU
Sample : PB157167BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK167

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
Data File : BP018187.D
Acq On : 15 Nov 2023 23:20
Operator : MA/JU
Sample : PB157167BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK167

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------