

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
 Data File : BP018188.D
 Acq On : 15 Nov 2023 23:54
 Operator : MA/JU
 Sample : PB157169BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK169

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018188.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.158	9	12	17	rBV	21673	28844	1.84%	0.178%
2	3.593	83	86	101	rBV	166247	271842	17.30%	1.675%
3	3.899	135	138	141	rBV4	4727	5754	0.37%	0.035%
4	4.905	307	309	312	rBV4	1210	1690	0.11%	0.010%
5	4.940	314	315	320	rVV5	1842	1898	0.12%	0.012%
6	5.193	356	358	362	rBV4	1724	1867	0.12%	0.012%
7	5.275	369	372	376	rVB6	1931	2428	0.15%	0.015%
8	5.399	390	393	396	rVB5	1375	1702	0.11%	0.010%
9	5.640	432	434	437	rVB4	1824	1611	0.10%	0.010%
10	5.869	472	473	478	rVB4	2103	2185	0.14%	0.013%
11	5.905	478	479	484	rBV5	1781	2376	0.15%	0.015%
12	6.428	566	568	574	rVB7	1245	2016	0.13%	0.012%
13	6.757	621	624	626	rVB4	1547	2101	0.13%	0.013%
14	6.952	649	657	672	rBV	241696	460773	29.33%	2.839%
15	7.134	682	688	709	rVB	209788	341143	21.72%	2.102%
16	7.304	711	717	734	rVV	286735	498934	31.76%	3.075%
17	7.781	792	798	813	rBV	264371	466976	29.73%	2.878%
18	8.199	865	869	871	rVB5	1479	2009	0.13%	0.012%
19	8.510	916	922	942	rBV	280560	552658	35.18%	3.406%
20	8.881	981	985	988	rBV5	1304	1884	0.12%	0.012%
21	8.993	997	1004	1017	rBV	240152	453910	28.89%	2.797%
22	9.234	1041	1045	1050	rVB8	1678	3167	0.20%	0.020%
23	9.293	1053	1055	1057	rVB2	2006	1596	0.10%	0.010%
24	9.328	1057	1061	1062	rBB3	1758	1991	0.13%	0.012%
25	9.704	1118	1125	1146	rBV	204484	418447	26.64%	2.579%
26	10.234	1207	1215	1241	rBV	240465	565185	35.98%	3.483%
27	10.598	1271	1277	1286	rBV	350622	577664	36.77%	3.560%
28	10.787	1299	1309	1328	rBV	155589	404896	25.77%	2.495%
29	11.392	1407	1412	1415	rBV7	1591	2558	0.16%	0.016%
30	11.598	1442	1447	1448	rBV5	1721	2032	0.13%	0.013%
31	12.216	1549	1552	1554	rBV4	1606	1585	0.10%	0.010%
32	12.257	1556	1559	1560	rBV2	1911	2072	0.13%	0.013%
33	12.492	1597	1599	1604	rVB6	1498	2117	0.13%	0.013%
34	12.639	1622	1624	1628	rBV5	1657	2227	0.14%	0.014%
35	13.228	1721	1724	1726	rBV4	1497	1689	0.11%	0.010%
36	13.304	1731	1737	1741	rVV5	6271	10780	0.69%	0.066%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
 Data File : BP018188.D
 Acq On : 15 Nov 2023 23:54
 Operator : MA/JU
 Sample : PB157169BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK169

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

37	13.798	1816	1821	1822	rBV5	1212	1829	0.12%	0.011%
38	13.839	1824	1828	1830	rBV5	1456	2271	0.14%	0.014%
39	13.886	1830	1836	1853	rVV	564963	829147	52.78%	5.110%
40	14.163	1875	1883	1896	rBV2	586591	875255	55.71%	5.394%
41	14.463	1927	1934	1946	rBV	480051	703882	44.81%	4.338%
42	14.751	1977	1983	2001	rBV2	56797	220407	14.03%	1.358%
43	15.469	2098	2105	2116	rBV	733125	1107666	70.51%	6.826%
44	15.569	2120	2122	2127	rVB6	1362	2083	0.13%	0.013%
45	15.628	2127	2132	2143	rBV	158768	303362	19.31%	1.869%
46	16.216	2231	2232	2237	rVB5	1266	1583	0.10%	0.010%
47	16.269	2237	2241	2243	rBV5	2047	2854	0.18%	0.018%
48	16.333	2248	2252	2255	rBV6	1535	3078	0.20%	0.019%
49	16.910	2346	2350	2355	rBV8	1410	2783	0.18%	0.017%
50	17.245	2401	2407	2416	rVV	601947	821477	52.29%	5.062%
51	17.345	2418	2424	2442	rVV	805983	1212628	77.19%	7.473%
52	17.739	2487	2491	2495	rBV6	1840	3052	0.19%	0.019%
53	17.810	2500	2503	2504	rBV3	1545	1593	0.10%	0.010%
54	17.880	2513	2515	2518	rBV4	2536	2742	0.17%	0.017%
55	18.110	2549	2554	2561	rVV9	8219	21354	1.36%	0.132%
56	18.339	2589	2593	2595	rBV5	2001	3467	0.22%	0.021%
57	18.498	2617	2620	2622	rBV4	1876	2628	0.17%	0.016%
58	18.827	2673	2676	2677	rBV3	2046	1666	0.11%	0.010%
59	18.963	2697	2699	2702	rBV4	2041	1993	0.13%	0.012%
60	19.174	2732	2735	2739	rVV5	10546	13414	0.85%	0.083%
61	19.257	2743	2749	2755	rBV2	8507	17331	1.10%	0.107%
62	19.357	2762	2766	2768	rBV5	3935	5930	0.38%	0.037%
63	19.604	2802	2808	2821	rBV	1064395	1441306	91.75%	8.882%
64	21.374	3104	3109	3122	rBV	635345	954398	60.75%	5.881%
65	23.680	3494	3501	3511	rBV	793978	1570985	100.00%	9.681%
66	23.845	3522	3529	3539	rBV	464483	992501	63.18%	6.116%




Sum of corrected areas: 16227272

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
Data File : BP018188.D
Acq On : 15 Nov 2023 23:54
Operator : MA/JU
Sample : PB157169BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK169

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

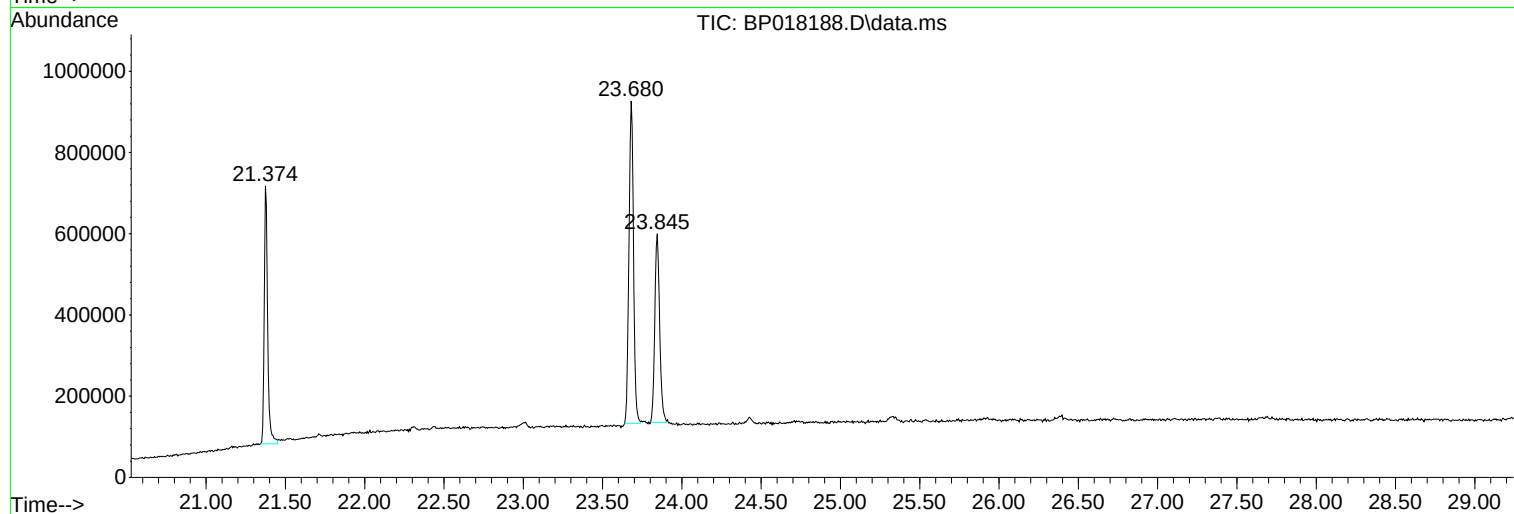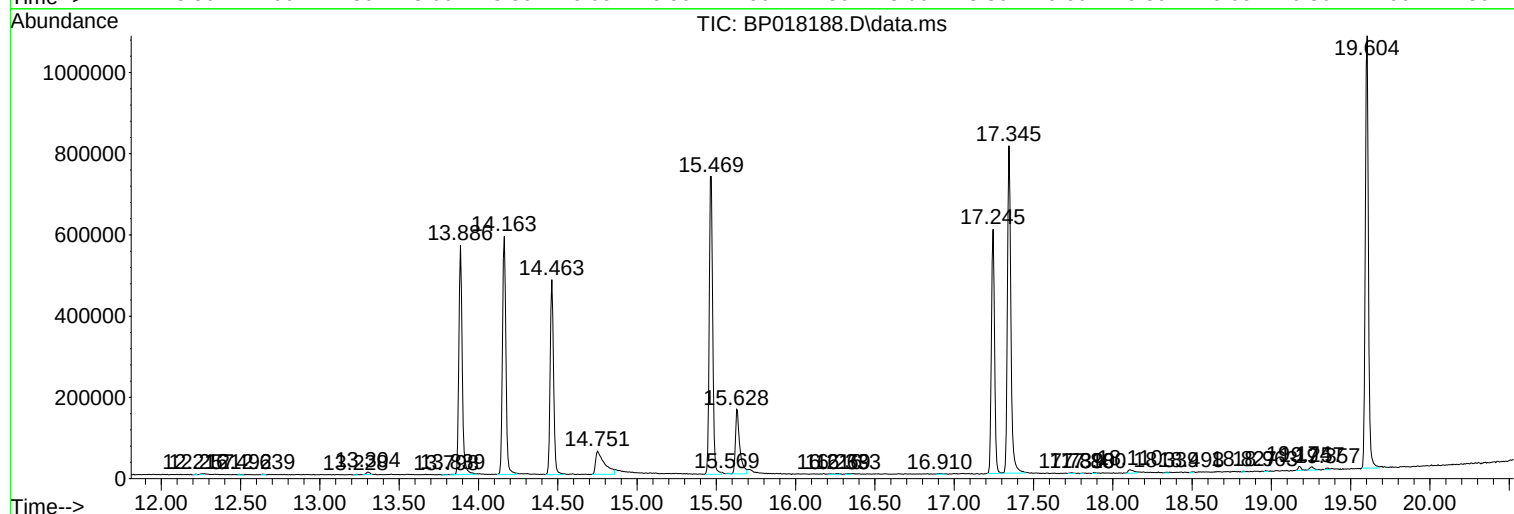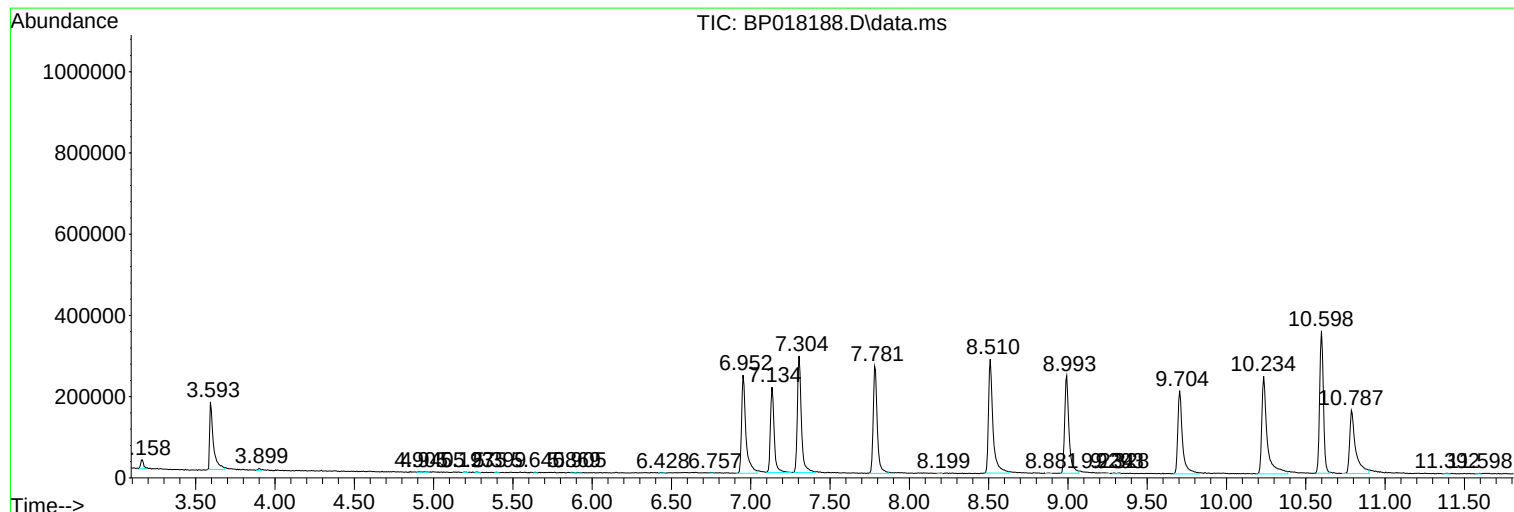

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
Data File : BP018188.D
Acq On : 15 Nov 2023 23:54
Operator : MA/JU
Sample : PB157169BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK169

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
Data File : BP018188.D
Acq On : 15 Nov 2023 23:54
Operator : MA/JU
Sample : PB157169BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK169

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------