

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
 Data File : BP018189.D
 Acq On : 16 Nov 2023 00:28
 Operator : MA/JU
 Sample : PB157121BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK121

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018189.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.158	9	12	17	rVB	20141	22536	1.55%	0.147%
2	3.593	83	86	99	rBV	152490	254917	17.58%	1.666%
3	3.823	123	125	126	rVB2	2251	1497	0.10%	0.010%
4	3.899	135	138	142	rVB6	4464	5867	0.40%	0.038%
5	4.846	297	299	301	rBV3	1619	1573	0.11%	0.010%
6	5.234	363	365	367	rBV3	1861	1915	0.13%	0.013%
7	5.322	376	380	382	rVB5	974	1531	0.11%	0.010%
8	5.399	390	393	395	rBV4	1685	2069	0.14%	0.014%
9	5.434	395	399	402	rVV5	1318	2361	0.16%	0.015%
10	6.869	640	643	647	rBV5	1866	2168	0.15%	0.014%
11	6.952	651	657	678	rBV	225198	436068	30.08%	2.850%
12	7.134	683	688	699	rVV	195728	309783	21.37%	2.025%
13	7.305	711	717	731	rBV	266023	464658	32.05%	3.037%
14	7.781	790	798	815	rBV	255039	448909	30.96%	2.934%
15	7.905	817	819	823	rVB5	2053	2536	0.17%	0.017%
16	8.511	916	922	940	rBV2	258080	511698	35.29%	3.344%
17	8.675	948	950	952	rVB2	1610	1450	0.10%	0.009%
18	8.993	996	1004	1016	rBV	227269	433104	29.87%	2.831%
19	9.340	1060	1063	1066	rBV5	1936	2002	0.14%	0.013%
20	9.605	1105	1108	1111	rVB5	1658	2192	0.15%	0.014%
21	9.634	1111	1113	1116	rBV4	1400	2005	0.14%	0.013%
22	9.705	1118	1125	1140	rBV	196713	386058	26.63%	2.523%
23	9.893	1154	1157	1160	rVB4	1394	1475	0.10%	0.010%
24	10.163	1199	1203	1208	rVB8	1501	2140	0.15%	0.014%
25	10.234	1208	1215	1241	rBV	219690	523169	36.09%	3.419%
26	10.528	1261	1265	1266	rBV4	1197	1576	0.11%	0.010%
27	10.599	1270	1277	1290	rVB	333658	555606	38.32%	3.631%
28	10.705	1294	1295	1299	rVB4	1480	1532	0.11%	0.010%
29	10.787	1303	1309	1330	rBV	136630	366824	25.30%	2.397%
30	11.416	1413	1416	1420	rVB6	984	1491	0.10%	0.010%
31	11.510	1428	1432	1434	rBV4	1294	1555	0.11%	0.010%
32	11.640	1453	1454	1458	rVV4	1507	1969	0.14%	0.013%
33	11.693	1460	1463	1467	rVB6	1433	1837	0.13%	0.012%
34	11.775	1474	1477	1478	rVB2	1616	1488	0.10%	0.010%
35	12.263	1556	1560	1562	rBV5	2213	3487	0.24%	0.023%
36	12.293	1564	1565	1570	rVV5	1350	1858	0.13%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
 Data File : BP018189.D
 Acq On : 16 Nov 2023 00:28
 Operator : MA/JU
 Sample : PB157121BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK121

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

37	12.781	1644	1648	1651	rVB6	1317	1671	0.12%	0.011%
38	13.157	1710	1712	1715	rVB4	1402	1494	0.10%	0.010%
39	13.199	1715	1719	1720	rBV3	1366	1791	0.12%	0.012%
40	13.310	1734	1738	1744	rVB9	3004	4897	0.34%	0.032%

41	13.404	1751	1754	1755	rBV2	1284	1462	0.10%	0.010%
42	13.451	1758	1762	1765	rVV6	1339	1896	0.13%	0.012%
43	13.516	1768	1773	1776	rVV7	1109	1657	0.11%	0.011%
44	13.581	1783	1784	1789	rVB4	1202	1666	0.11%	0.011%
45	13.728	1806	1809	1813	rBV5	2258	3303	0.23%	0.022%

46	13.887	1830	1836	1848	rBV	523320	786134	54.22%	5.138%
47	14.010	1855	1857	1860	rVB4	1638	1659	0.11%	0.011%
48	14.034	1860	1861	1866	rBV5	1648	1784	0.12%	0.012%
49	14.163	1876	1883	1894	rBV2	561069	820018	56.56%	5.359%
50	14.293	1903	1905	1910	rVB6	2790	3950	0.27%	0.026%

51	14.463	1927	1934	1945	rBV	465460	672636	46.39%	4.396%
52	14.751	1977	1983	1998	rBV4	50345	194661	13.43%	1.272%
53	15.093	2039	2041	2045	rVB4	1748	2167	0.15%	0.014%
54	15.240	2063	2066	2069	rBV5	1366	1751	0.12%	0.011%
55	15.469	2098	2105	2122	rBV	680072	1047936	72.28%	6.849%

56	15.634	2127	2133	2144	rBV	143588	280908	19.38%	1.836%
57	16.445	2268	2271	2275	rVB5	984	1621	0.11%	0.011%
58	16.481	2275	2277	2280	rBV4	1339	1567	0.11%	0.010%
59	16.516	2280	2283	2286	rVB5	1603	1896	0.13%	0.012%
60	16.663	2305	2308	2310	rBV4	1330	1504	0.10%	0.010%

61	16.710	2312	2316	2319	rVB6	1347	1905	0.13%	0.012%
62	17.057	2373	2375	2381	rVB6	1624	2246	0.15%	0.015%
63	17.245	2400	2407	2418	rBV	561188	799717	55.16%	5.226%
64	17.345	2418	2424	2441	rVV2	758547	1152359	79.48%	7.531%
65	17.651	2472	2476	2478	rBV5	1163	1601	0.11%	0.010%

66	17.904	2517	2519	2522	rVV4	1579	1585	0.11%	0.010%
67	17.945	2524	2526	2533	rVB7	1548	3085	0.21%	0.020%
68	17.998	2533	2535	2538	rBV4	1141	1592	0.11%	0.010%
69	18.110	2549	2554	2562	rBV7	7991	19213	1.33%	0.126%
70	18.404	2602	2604	2606	rBV2	1429	1546	0.11%	0.010%

71	18.598	2634	2637	2638	rBV3	1523	1562	0.11%	0.010%
72	18.945	2694	2696	2699	rBV3	1835	1924	0.13%	0.013%
73	19.181	2730	2736	2740	rVB6	11192	16290	1.12%	0.106%
74	19.257	2745	2749	2753	rVV6	7910	11171	0.77%	0.073%
75	19.604	2802	2808	2822	rBV	996458	1368662	94.40%	8.945%

76	21.375	3104	3109	3120	rBV	615290	897229	61.89%	5.864%
----	--------	------	------	------	-----	--------	--------	--------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
Data File : BP018189.D
Acq On : 16 Nov 2023 00:28
Operator : MA/JU
Sample : PB157121BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK121

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Title : SVOA CALIBRATION

77	23.680	3494	3501	3512	rBV2	718655	1449822	100.00%	9.475%
78	23.845	3522	3529	3541	rBV	456753	966816	66.69%	6.319%




Sum of corrected areas: 15301258

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
Data File : BP018189.D
Acq On : 16 Nov 2023 00:28
Operator : MA/JU
Sample : PB157121BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK121

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

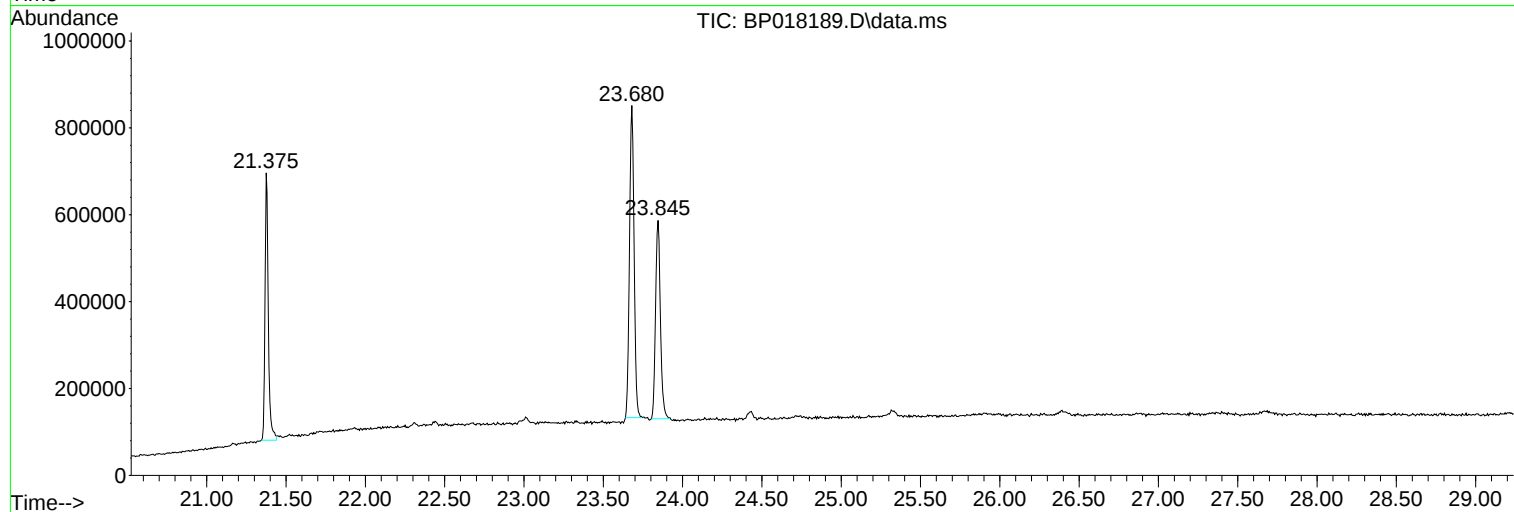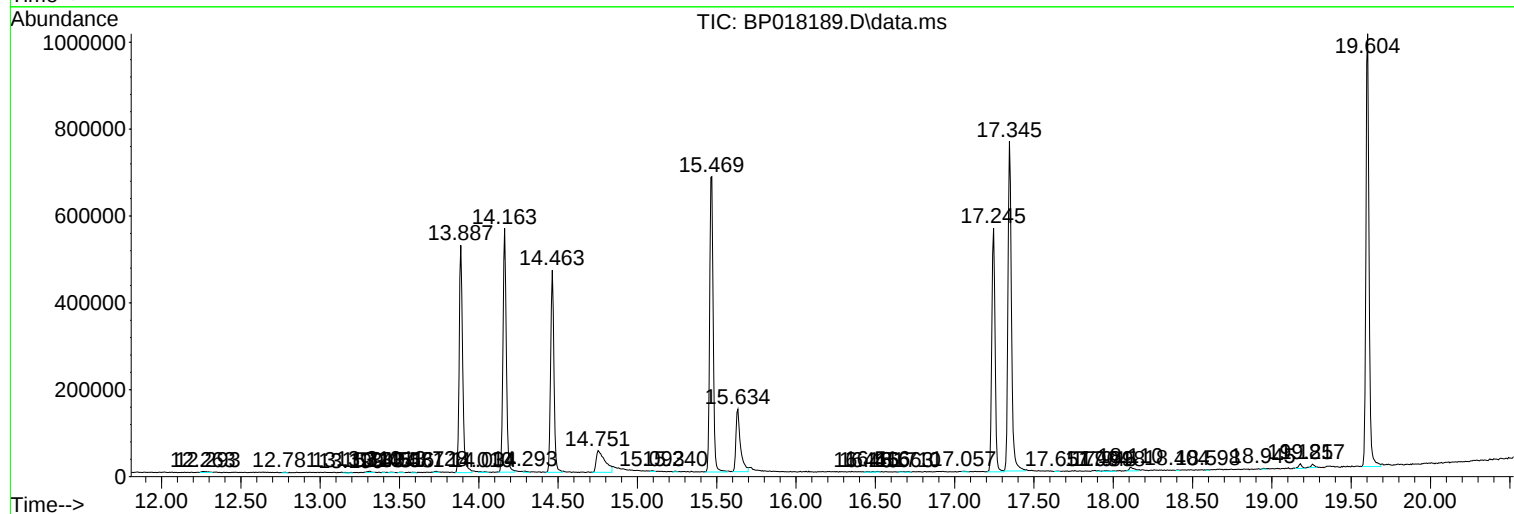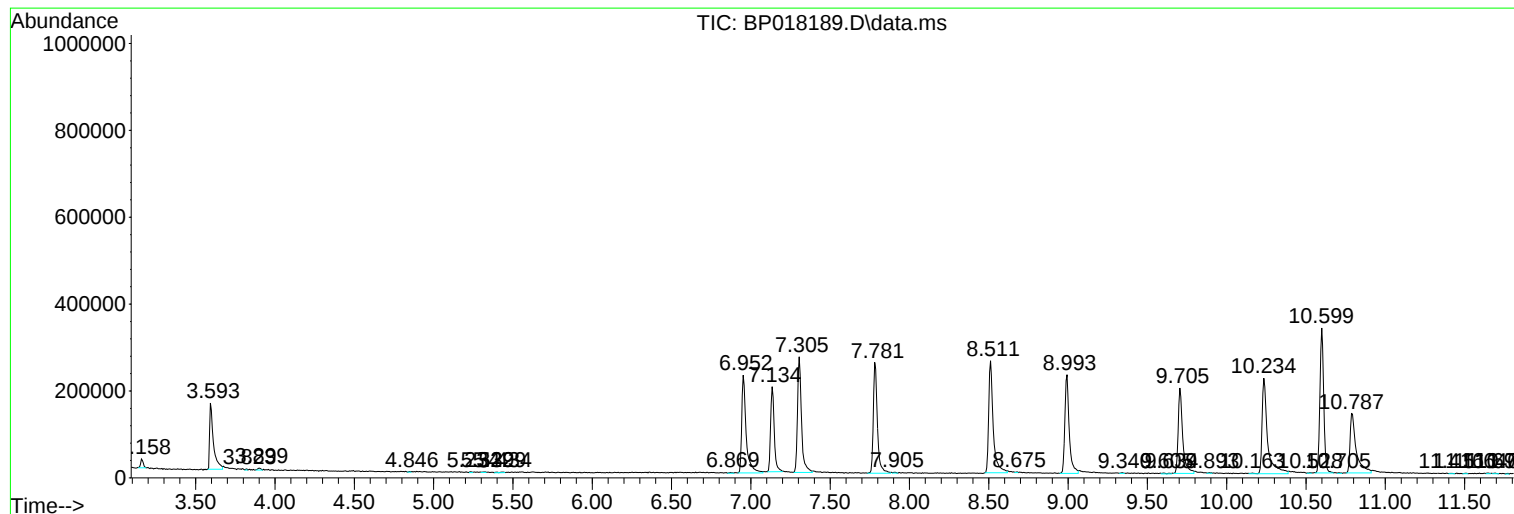

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
Data File : BP018189.D
Acq On : 16 Nov 2023 00:28
Operator : MA/JU
Sample : PB157121BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK121

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
Data File : BP018189.D
Acq On : 16 Nov 2023 00:28
Operator : MA/JU
Sample : PB157121BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK121

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------