

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
 Data File : BP018206.D
 Acq On : 16 Nov 2023 10:36
 Operator : MA/JU
 Sample : PB157171BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK171

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018206.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.158	9	12	21	rVB	23262	34026	1.85%	0.174%
2	3.593	83	86	105	rBV	190974	316429	17.22%	1.622%
3	3.829	124	126	130	rBV5	1766	2843	0.15%	0.015%
4	3.899	136	138	141	rBV4	3174	3553	0.19%	0.018%
5	4.358	215	216	220	rVB4	2465	2118	0.12%	0.011%
6	4.952	315	317	320	rVB4	2343	2368	0.13%	0.012%
7	5.276	370	372	377	rBV6	1904	2577	0.14%	0.013%
8	5.558	418	420	425	rVB5	2608	3200	0.17%	0.016%
9	6.234	532	535	538	rVV5	1918	2487	0.14%	0.013%
10	6.293	540	545	546	rBV5	1926	2938	0.16%	0.015%
11	6.317	546	549	552	rBV5	2042	2345	0.13%	0.012%
12	6.417	563	566	569	rVB5	2206	1919	0.10%	0.010%
13	6.728	617	619	625	rBV7	2143	2707	0.15%	0.014%
14	6.775	625	627	631	rVB5	1834	2590	0.14%	0.013%
15	6.952	651	657	672	rBV	270621	512470	27.89%	2.626%
16	7.134	682	688	704	rVB	241141	383617	20.87%	1.966%
17	7.305	711	717	731	rBV	320229	546469	29.74%	2.801%
18	7.781	792	798	818	rBV	284216	506612	27.57%	2.596%
19	8.511	915	922	940	rBV	314537	628739	34.21%	3.222%
20	8.993	996	1004	1019	rBV	264374	524682	28.55%	2.689%
21	9.705	1118	1125	1143	rBV	239640	470535	25.60%	2.411%
22	10.005	1173	1176	1180	rVB6	1449	2238	0.12%	0.011%
23	10.052	1180	1184	1186	rBV4	1717	2638	0.14%	0.014%
24	10.234	1208	1215	1236	rBV	270836	613771	33.40%	3.146%
25	10.599	1268	1277	1288	rBV	386391	662142	36.03%	3.393%
26	10.787	1303	1309	1336	rBV	186437	496899	27.04%	2.547%
27	11.352	1401	1405	1406	rBV4	1719	2125	0.12%	0.011%
28	12.257	1554	1559	1566	rBV10	3907	10856	0.59%	0.056%
29	12.663	1623	1628	1632	rBV8	1784	3364	0.18%	0.017%
30	13.252	1723	1728	1731	rVB7	1261	1952	0.11%	0.010%
31	13.304	1731	1737	1741	rBV6	7373	14260	0.78%	0.073%
32	13.887	1830	1836	1851	rBV	695015	1012364	55.09%	5.188%
33	13.993	1851	1854	1862	rVB10	3218	7722	0.42%	0.040%
34	14.163	1876	1883	1900	rBV	700475	1070452	58.25%	5.486%
35	14.463	1928	1934	1946	rBV	584425	855013	46.53%	4.382%
36	14.563	1950	1951	1956	rVV5	1528	1923	0.10%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
 Data File : BP018206.D
 Acq On : 16 Nov 2023 10:36
 Operator : MA/JU
 Sample : PB157171BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK171

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

37	14.622	1959	1961	1965	rBV5	1513	2004	0.11%	0.010%
38	14.746	1977	1982	2004	rBV4	81662	334008	18.18%	1.712%
39	15.075	2036	2038	2042	rVB5	1438	1963	0.11%	0.010%
40	15.463	2098	2104	2122	rBV	918666	1378386	75.01%	7.064%
41	15.628	2127	2132	2143	rBV	233352	428445	23.31%	2.196%
42	15.928	2181	2183	2186	rVB4	2031	2053	0.11%	0.011%
43	15.987	2189	2193	2196	rBV6	1674	2274	0.12%	0.012%
44	16.034	2199	2201	2205	rBV4	1529	2405	0.13%	0.012%
45	16.257	2238	2239	2243	rVB3	1801	2087	0.11%	0.011%
46	16.298	2243	2246	2251	rBV7	1863	3349	0.18%	0.017%
47	16.922	2348	2352	2354	rVB5	2066	2171	0.12%	0.011%
48	17.245	2401	2407	2417	rBV	801762	1074573	58.47%	5.507%
49	17.345	2419	2424	2443	rVB2	1058019	1552399	84.48%	7.956%
50	17.945	2525	2526	2529	rBV3	1906	2403	0.13%	0.012%
51	18.110	2550	2554	2556	rBV5	6288	8273	0.45%	0.042%
52	18.269	2580	2581	2586	rBV5	1784	2613	0.14%	0.013%
53	18.322	2586	2590	2592	rBV5	1371	1940	0.11%	0.010%
54	18.451	2610	2612	2617	rVB6	1990	2488	0.14%	0.013%
55	19.181	2731	2736	2741	rBV4	14107	21122	1.15%	0.108%
56	19.257	2745	2749	2754	rBV2	12458	18938	1.03%	0.097%
57	19.345	2762	2764	2765	rBV2	3577	2347	0.13%	0.012%
58	19.604	2802	2808	2819	rBV	1327728	1837695	100.00%	9.418%
59	21.381	3105	3110	3122	rBV	780541	1150234	62.59%	5.895%
60	23.686	3495	3502	3513	rVB2	925043	1826212	99.38%	9.359%
61	23.851	3523	3530	3541	rVB	529584	1139222	61.99%	5.838%




Sum of corrected areas: 19512547

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
Data File : BP018206.D
Acq On : 16 Nov 2023 10:36
Operator : MA/JU
Sample : PB157171BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK171

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

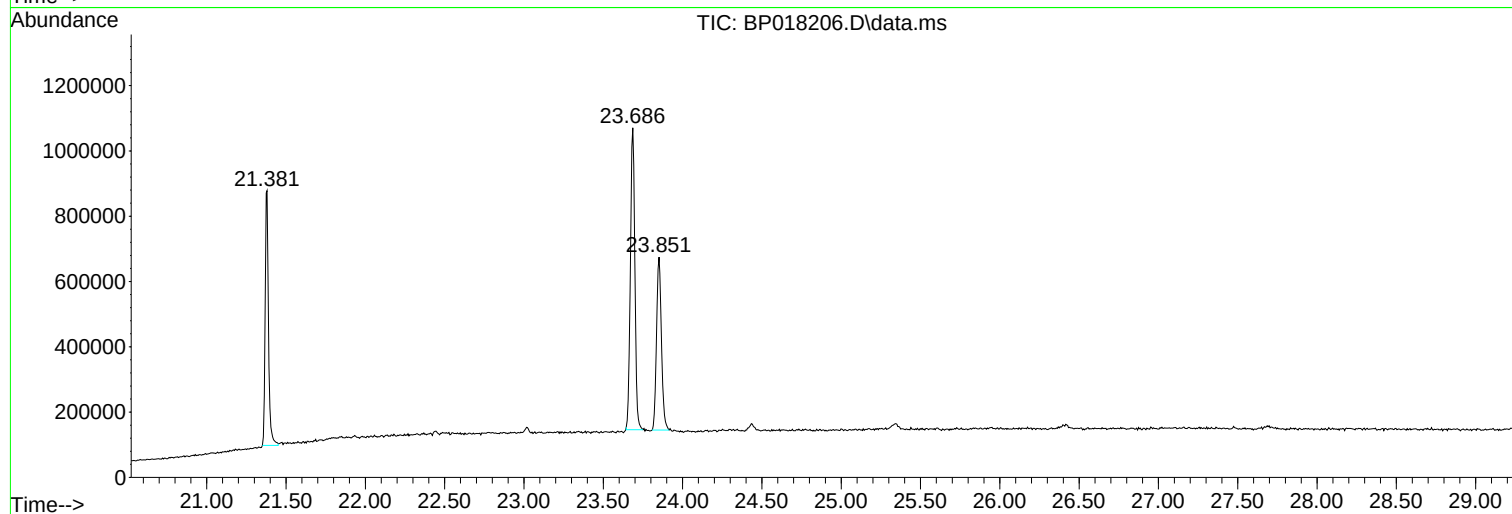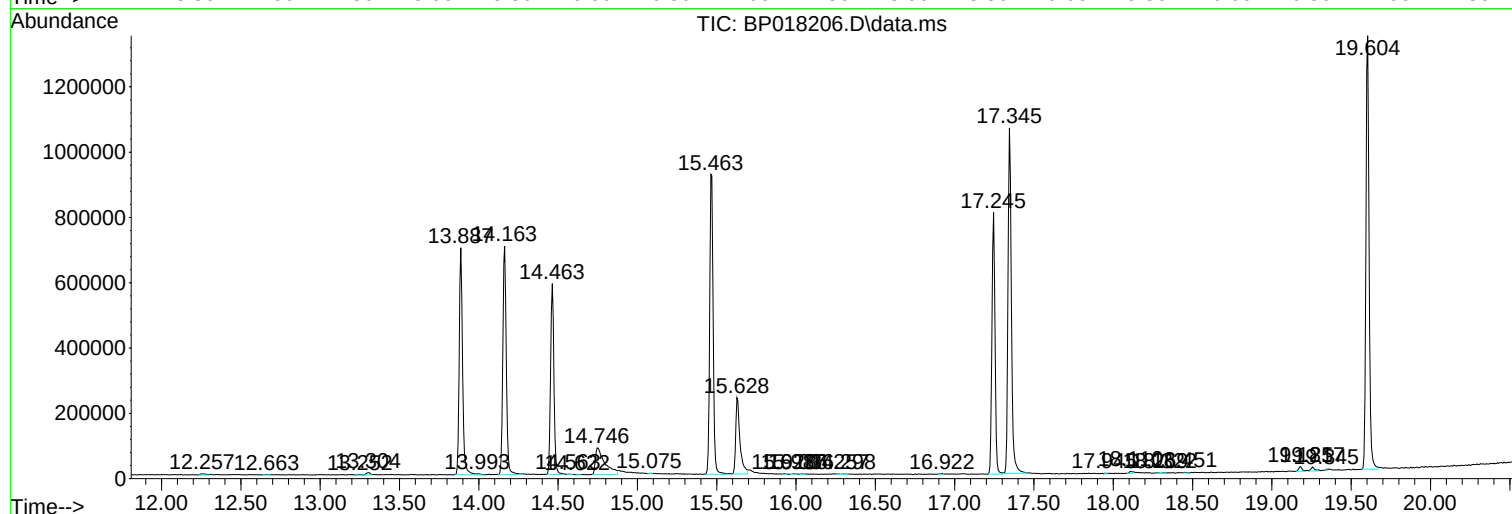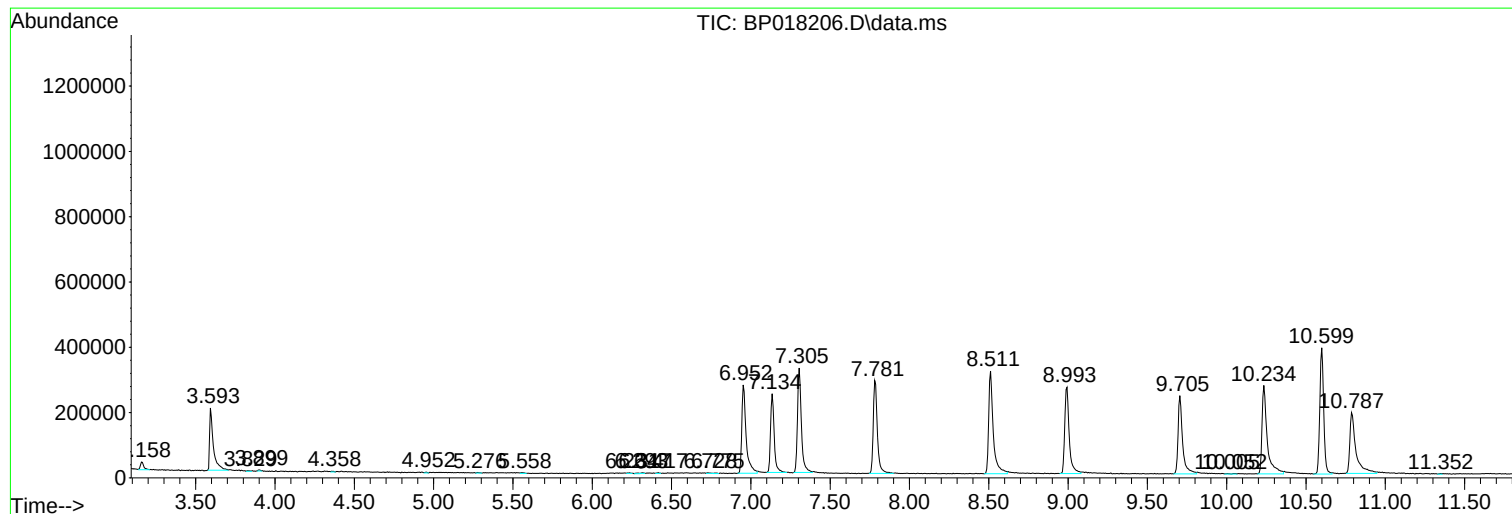

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
Data File : BP018206.D
Acq On : 16 Nov 2023 10:36
Operator : MA/JU
Sample : PB157171BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK171

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
Data File : BP018206.D
Acq On : 16 Nov 2023 10:36
Operator : MA/JU
Sample : PB157171BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK171

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc