

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
 Data File : BP018207.D
 Acq On : 16 Nov 2023 11:10
 Operator : MA/JU
 Sample : 05338-23
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCDM6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018207.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.158	9	12	16	rBV	24991	29524	1.46%	0.151%
2	3.199	16	19	24	rVB	14214	17845	0.88%	0.091%
3	3.593	83	86	100	rBV	234185	380706	18.80%	1.946%
4	3.905	136	139	143	rVB6	3660	4978	0.25%	0.025%
5	4.740	276	281	282	rVB5	1424	2123	0.10%	0.011%
6	5.946	482	486	490	rBV6	1380	2263	0.11%	0.012%
7	6.358	551	556	557	rBV5	1346	2250	0.11%	0.011%
8	6.952	651	657	675	rBV	347002	631507	31.19%	3.227%
9	7.134	682	688	705	rVB	291606	457002	22.57%	2.335%
10	7.305	710	717	737	rBV	384509	665246	32.85%	3.400%
11	7.781	792	798	812	rBV	229088	417424	20.62%	2.133%
12	8.510	914	922	942	rBV	415501	788396	38.94%	4.029%
13	8.787	967	969	974	rBV6	1346	2059	0.10%	0.011%
14	8.993	996	1004	1021	rBV	333989	636796	31.45%	3.254%
15	9.157	1031	1032	1037	rVB5	4123	3605	0.18%	0.018%
16	9.705	1118	1125	1148	rBV	297430	587437	29.01%	3.002%
17	9.922	1157	1162	1166	rVB8	1930	3497	0.17%	0.018%
18	10.234	1208	1215	1235	rBV	347698	761230	37.59%	3.890%
19	10.599	1268	1277	1285	rBV	290883	486319	24.02%	2.485%
20	10.787	1302	1309	1329	rBV	274637	673443	33.26%	3.442%
21	11.228	1379	1384	1386	rVB6	1788	2935	0.14%	0.015%
22	11.799	1477	1481	1484	rVB5	1807	2027	0.10%	0.010%
23	12.246	1552	1557	1562	rBV7	4022	7781	0.38%	0.040%
24	12.657	1621	1627	1630	rBV7	1648	2452	0.12%	0.013%
25	12.822	1652	1655	1658	rBV5	1467	2288	0.11%	0.012%
26	13.069	1693	1697	1701	rVV7	1282	2043	0.10%	0.010%
27	13.310	1734	1738	1741	rVB5	5173	6888	0.34%	0.035%
28	13.422	1753	1757	1758	rBV3	1495	2429	0.12%	0.012%
29	13.887	1828	1836	1851	rBV	763797	1112635	54.95%	5.686%
30	14.163	1876	1883	1898	rBV2	822088	1198835	59.21%	6.126%
31	14.463	1926	1934	1947	rBV	427101	614610	30.35%	3.141%
32	14.745	1974	1982	2003	rBV2	94915	362803	17.92%	1.854%
33	14.940	2013	2015	2022	rVB7	5092	7970	0.39%	0.041%
34	15.463	2098	2104	2115	rBV	996448	1483656	73.27%	7.582%
35	15.628	2126	2132	2144	rBV	240412	453261	22.39%	2.316%
36	16.087	2206	2210	2213	rVB6	1756	2552	0.13%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
 Data File : BP018207.D
 Acq On : 16 Nov 2023 11:10
 Operator : MA/JU
 Sample : 05338-23
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCDM6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

37	16.257	2238	2239	2243	rVB4	1874	2285	0.11%	0.012%
38	16.392	2258	2262	2264	rVB5	1573	2032	0.10%	0.010%
39	17.051	2372	2374	2378	rVB5	1912	2660	0.13%	0.014%
40	17.245	2398	2407	2418	rBV	502300	695457	34.35%	3.554%
41	17.345	2418	2424	2439	rVV	1051969	1574846	77.78%	8.048%
42	17.634	2471	2473	2476	rBV4	1629	2184	0.11%	0.011%
43	17.951	2524	2527	2531	rVB5	1799	2800	0.14%	0.014%
44	18.110	2552	2554	2556	rBV3	4990	5161	0.25%	0.026%
45	18.416	2602	2606	2607	rBV3	1608	2113	0.10%	0.011%
46	18.610	2636	2639	2641	rVV4	1927	2462	0.12%	0.013%
47	19.180	2732	2736	2742	rBV2	12504	16930	0.84%	0.087%
48	19.251	2744	2748	2758	rVB2	10219	21219	1.05%	0.108%
49	19.604	2802	2808	2819	rBV	1366998	1815287	89.65%	9.277%
50	21.380	3105	3110	3123	rBV	514628	758186	37.44%	3.875%
51	23.686	3494	3502	3514	rBV2	1031052	2024834	100.00%	10.348%
52	23.851	3523	3530	3543	rVB	355544	820835	40.54%	4.195%




Sum of corrected areas: 19568106

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
Data File : BP018207.D
Acq On : 16 Nov 2023 11:10
Operator : MA/JU
Sample : 05338-23
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCDM6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

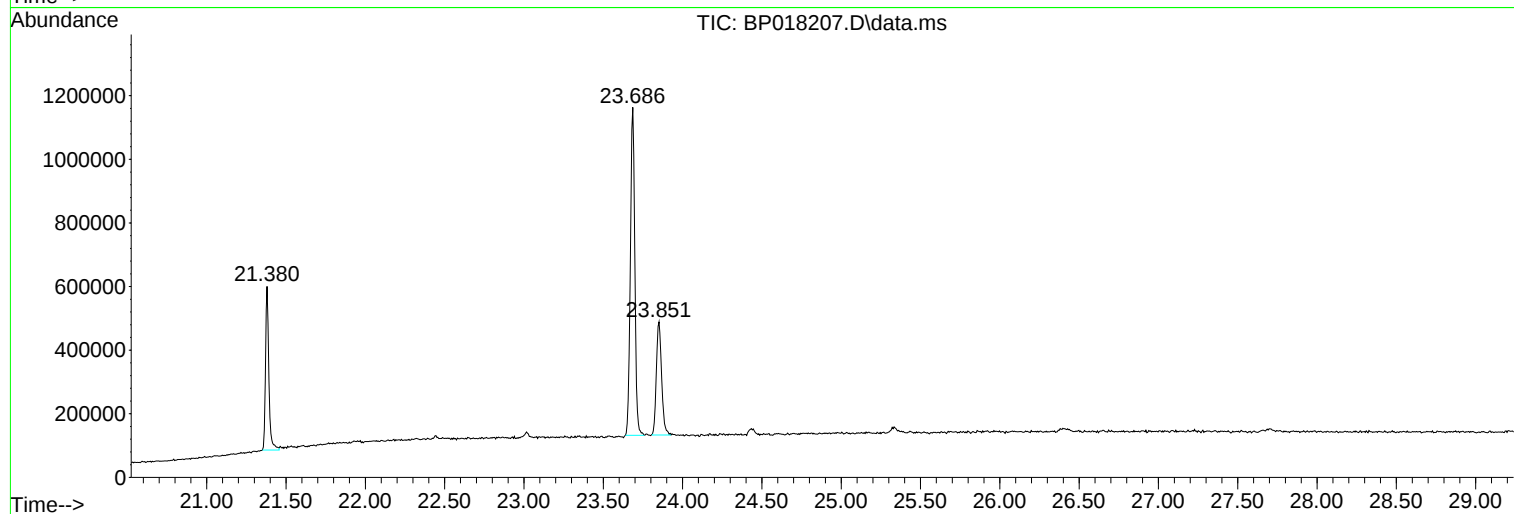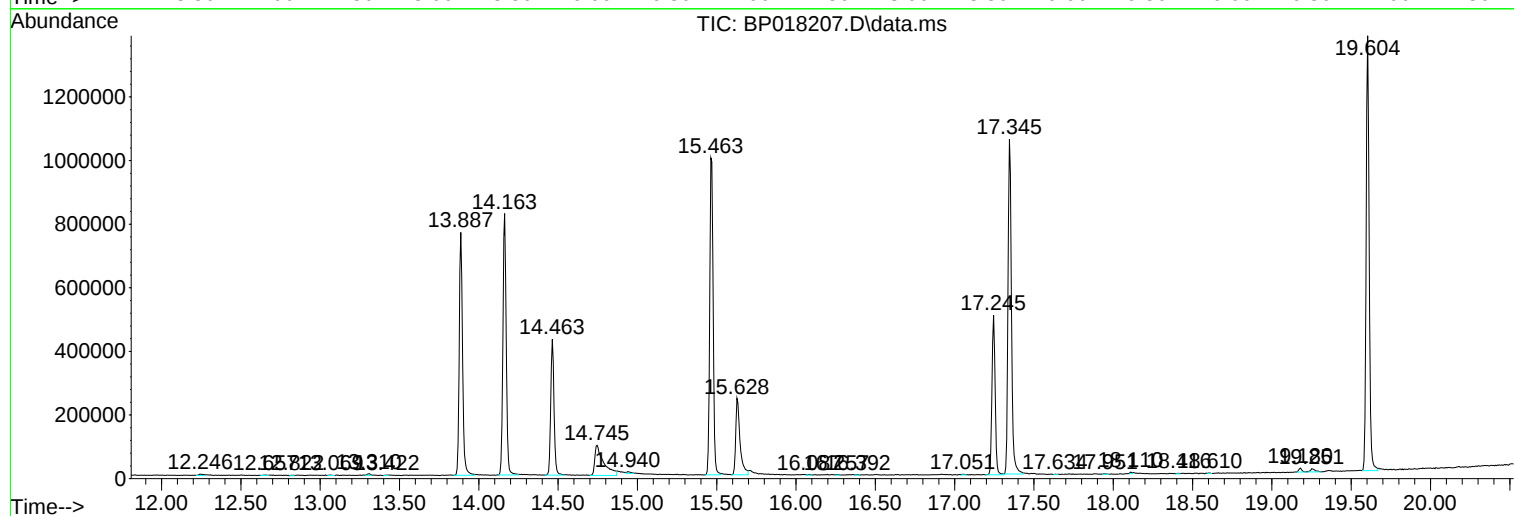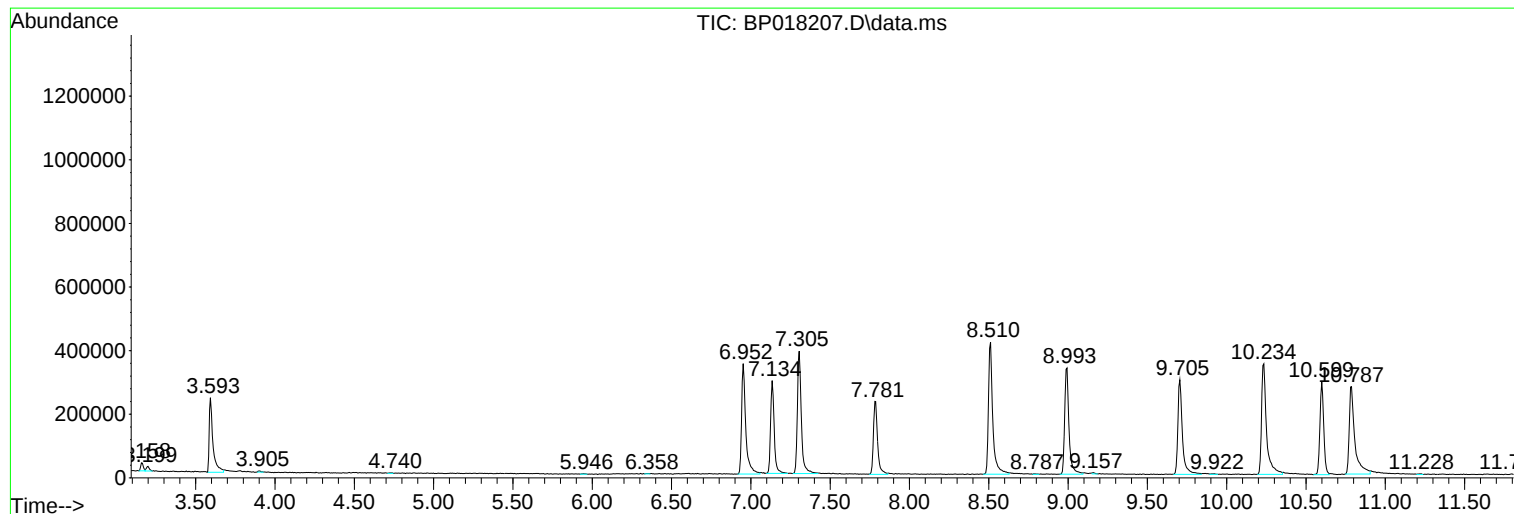

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
Data File : BP018207.D
Acq On : 16 Nov 2023 11:10
Operator : MA/JU
Sample : 05338-23
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCDM6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111523\
Data File : BP018207.D
Acq On : 16 Nov 2023 11:10
Operator : MA/JU
Sample : 05338-23
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCDM6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc