

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111621\
 Data File : BP007993.D
 Acq On : 16 Nov 2021 10:55
 Operator : CG/JU
 Sample : PB140389BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB140389BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP007993.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.428	357	364	379	rBV	2495836	3653885	36.15%	9.204%
2	7.017	627	634	656	rBV	2169470	3487341	34.50%	8.784%
3	7.840	767	774	784	rBV	425338	653452	6.47%	1.646%
4	8.999	963	971	988	rBV	1280888	2166082	21.43%	5.456%
5	10.640	1242	1250	1260	rBV	540064	926759	9.17%	2.334%
6	13.104	1661	1669	1684	rBV	3711176	5488944	54.31%	13.826%
7	14.481	1896	1903	1917	rBV	931673	1369892	13.55%	3.451%
8	15.975	2149	2157	2186	rBV	3485383	5003903	49.51%	12.604%
9	17.240	2363	2372	2386	rBV	1188243	1797621	17.79%	4.528%
10	19.804	2802	2808	2818	rBV	8360612	10107438	100.00%	25.459%
11	21.328	3063	3067	3076	rBV	1777175	2380528	23.55%	5.996%
12	23.739	3470	3477	3488	rVB2	1299086	2664425	26.36%	6.711%




Sum of corrected areas: 39700270

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111621\
Data File : BP007993.D
Acq On : 16 Nov 2021 10:55
Operator : CG/JU
Sample : PB140389BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140389BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

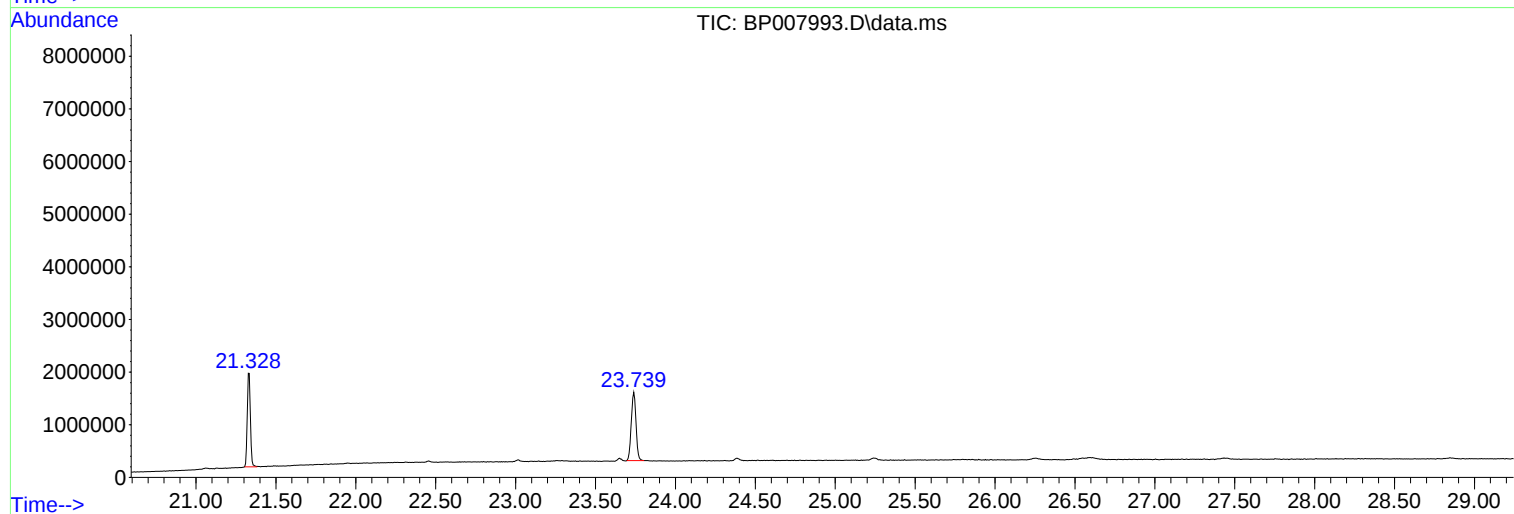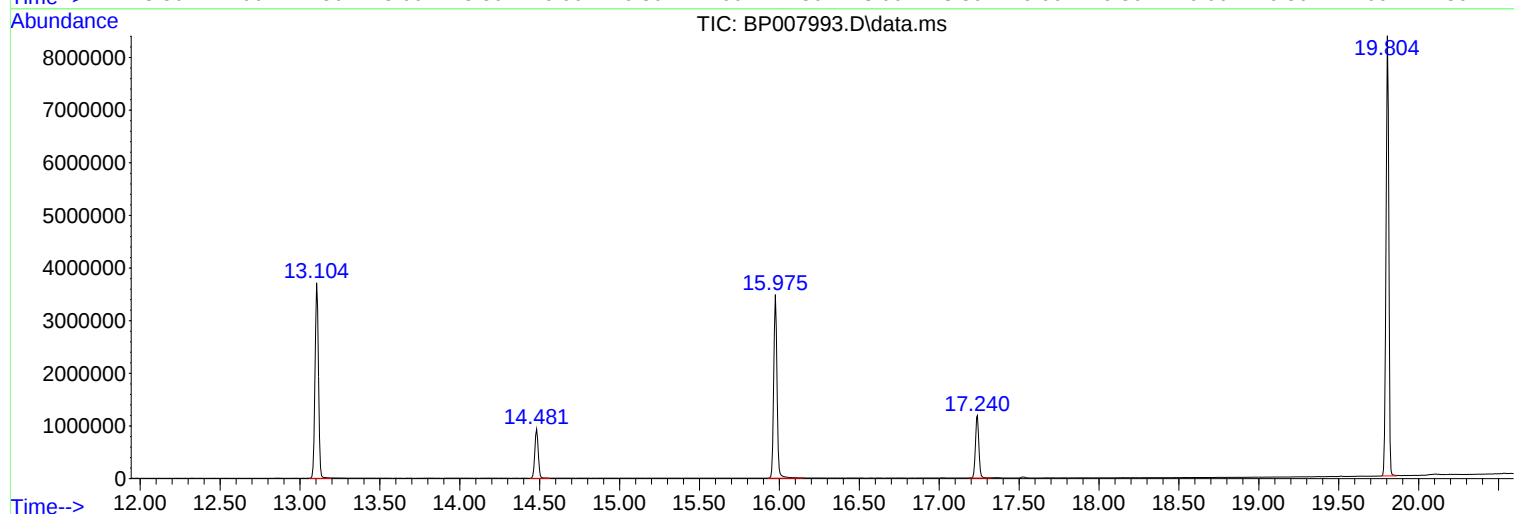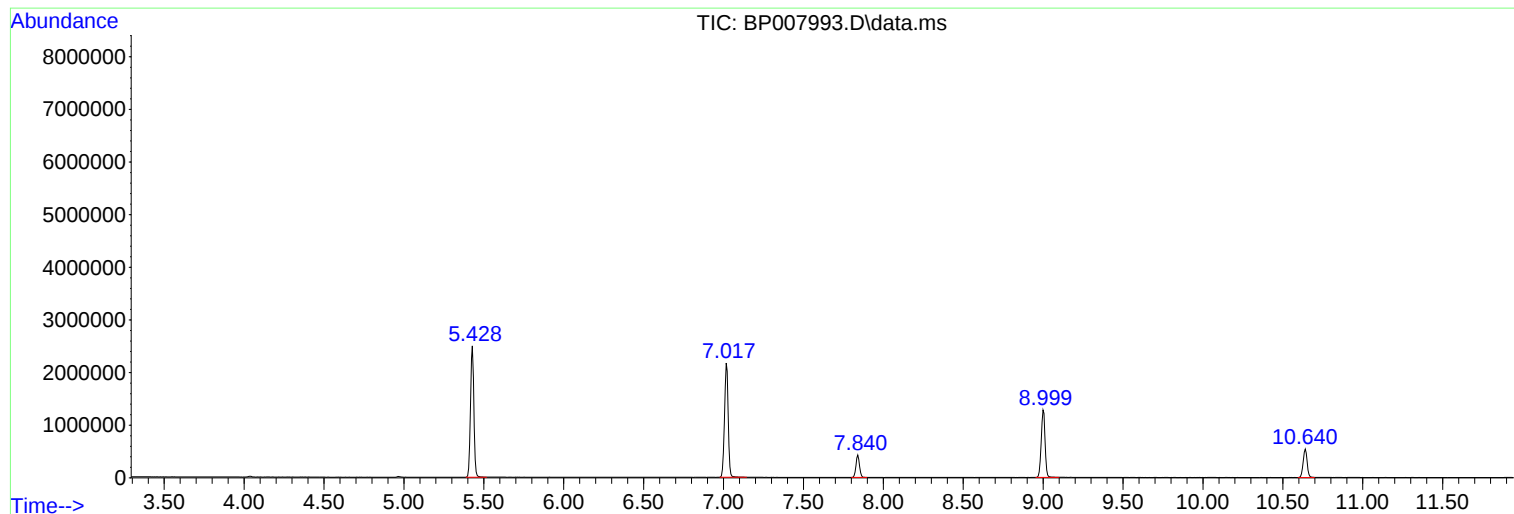

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111621\
Data File : BP007993.D
Acq On : 16 Nov 2021 10:55
Operator : CG/JU
Sample : PB140389BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140389BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111621\
Data File : BP007993.D
Acq On : 16 Nov 2021 10:55
Operator : CG/JU
Sample : PB140389BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140389BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------