
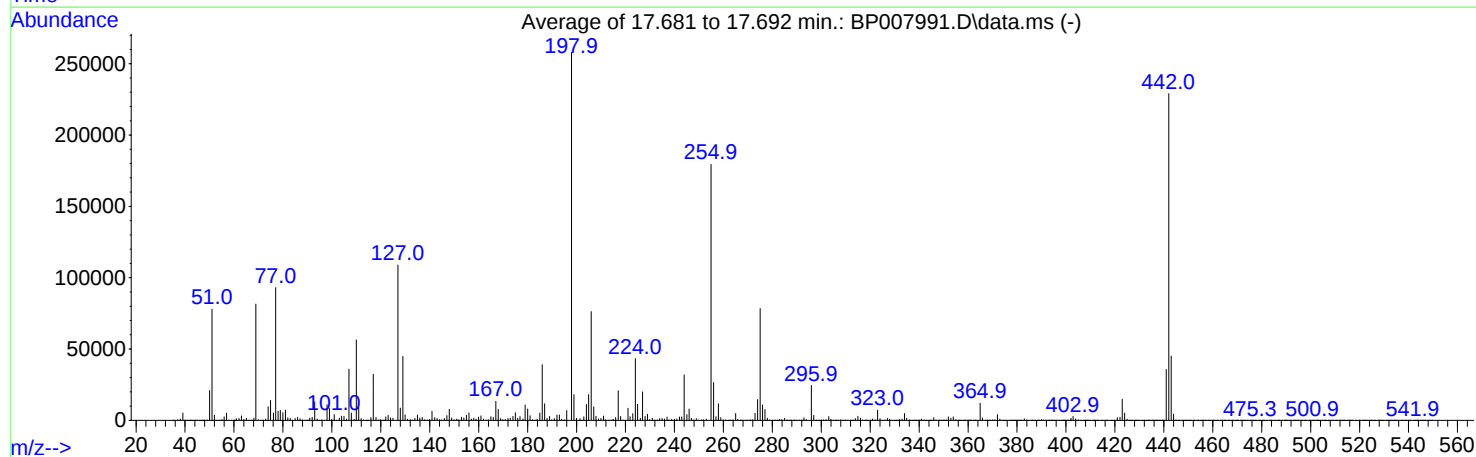


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111621\
 Data File : BP007991.D
 Acq On : 16 Nov 2021 09:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 15 05:36:49 2021

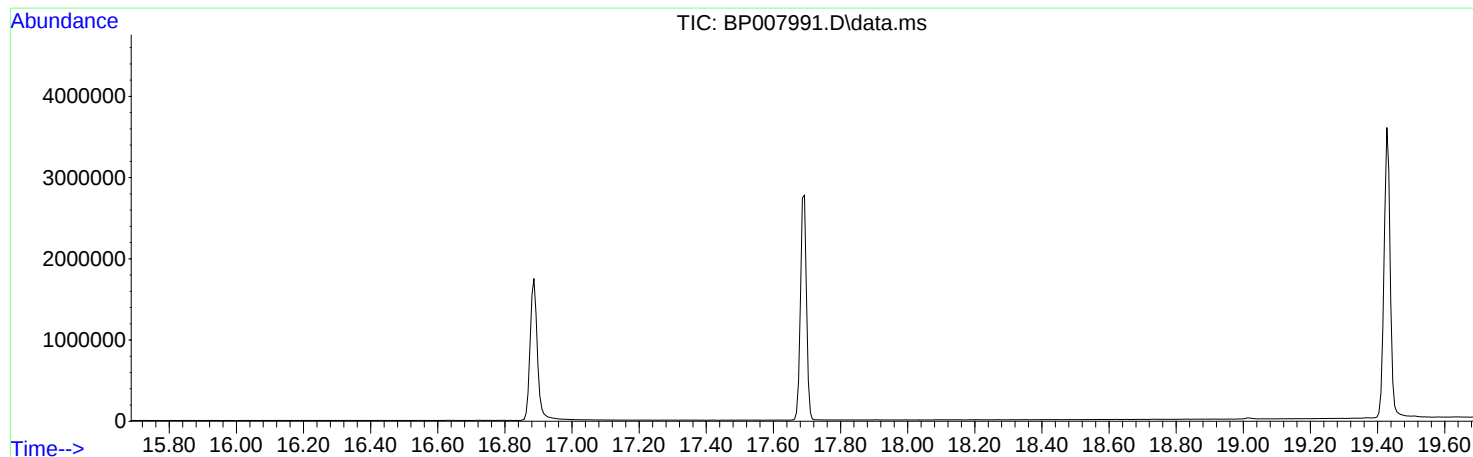




AutoFind: Scans 2447, 2448, 2449; Background Corrected with Scan 2440

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.2	77871	PASS
68	69	0.00	2	1.9	1585	PASS
69	198	0.00	100	31.6	81540	PASS
70	69	0.00	2	0.6	481	PASS
127	198	10	80	42.3	108955	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	257865	PASS
199	198	5	9	7.0	18036	PASS
275	198	10	60	30.4	78401	PASS
365	198	1	100	4.6	11961	PASS
441	198	0.01	100	13.8	35617	PASS
442	442	100	100	100.0	229022	PASS
443	442	15	24	19.7	45144	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111621\
Data File : BP007991.D
Acq On : 16 Nov 2021 09:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 16 12:18:58 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 15 05:36:49 2021
Response via : Initial Calibration

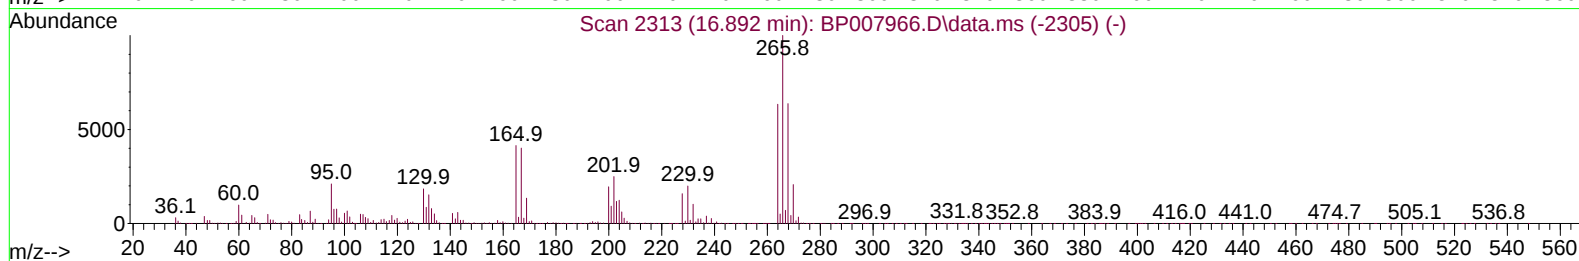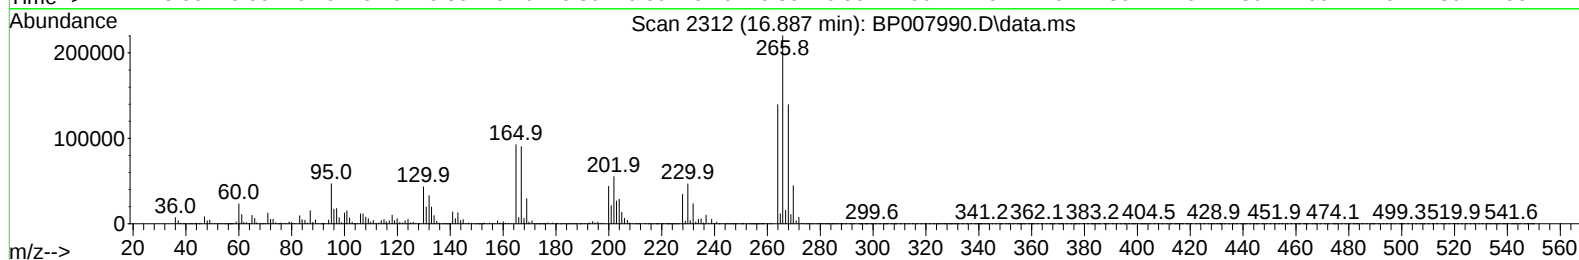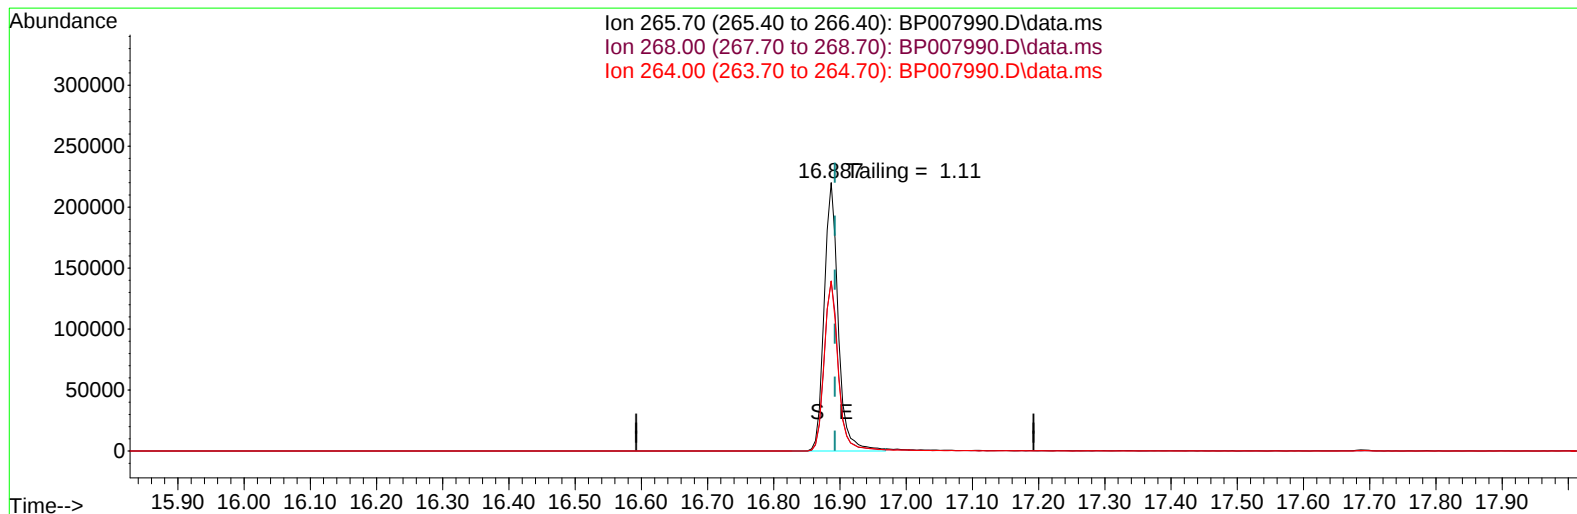

TIC: BP007990.D\data.ms

(70) Pentachlorophenol (C)

16.887min (-0.006) 6785106.45 ng




response 327004

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.60	63.30
264.00	60.90	63.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111621\
 Data File : BP007991.D
 Acq On : 16 Nov 2021 09:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Nov 16 12:18:58 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 15 05:36:49 2021
 Response via : Initial Calibration

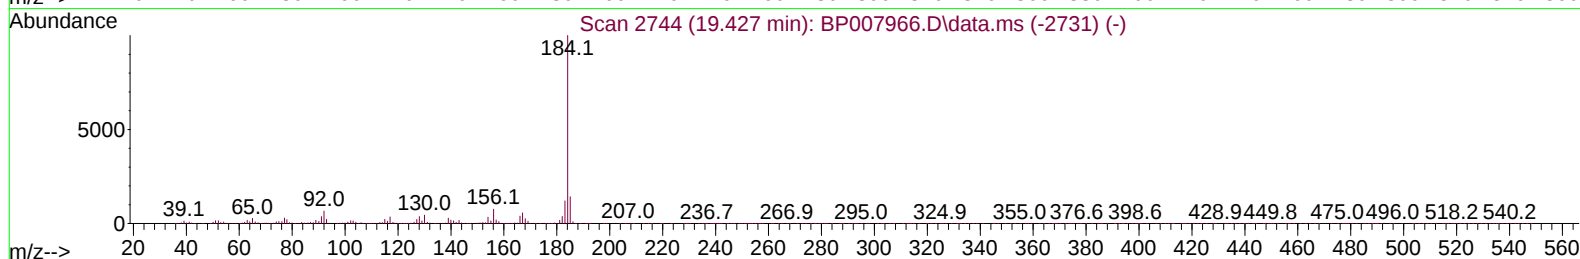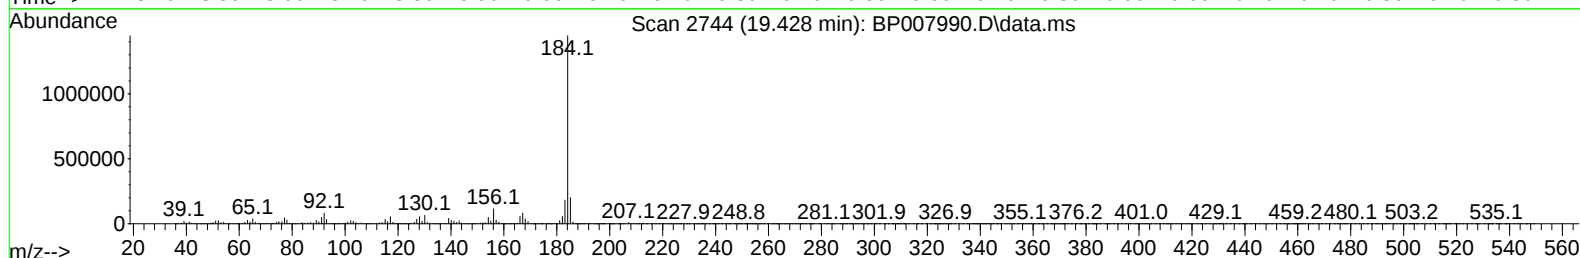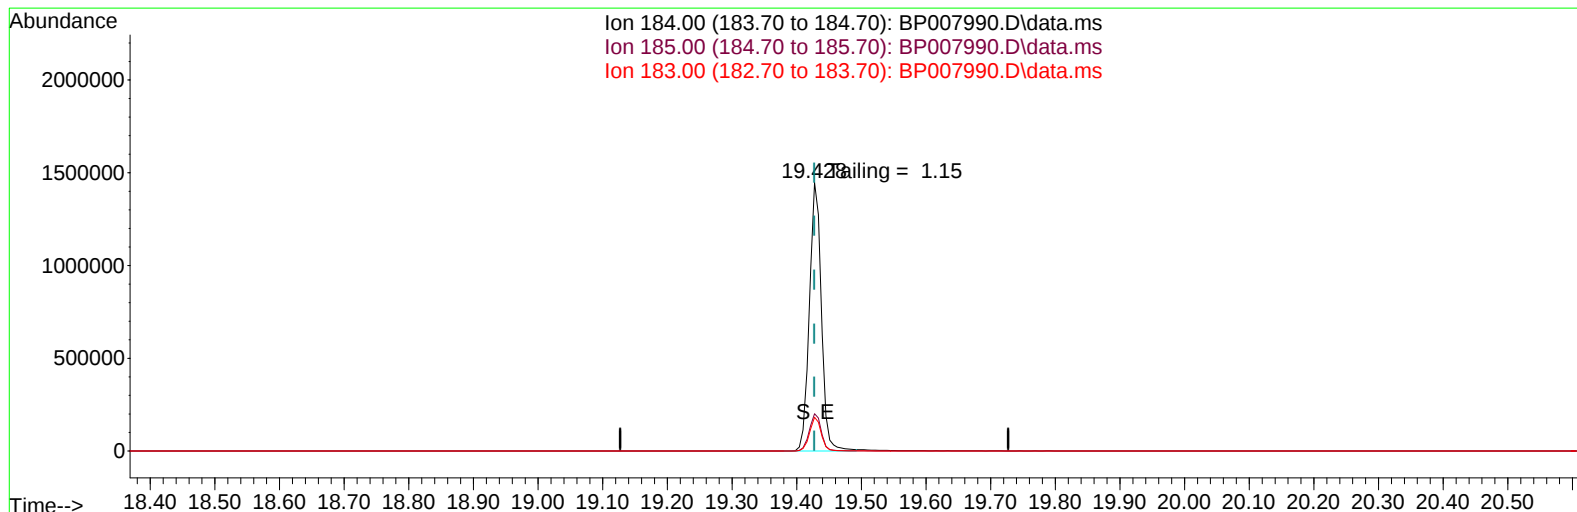

TIC: BP007990.D\data.ms

(77) Benzidine

19.428min (+ 0.001) 425638.96 ng

response 1880847

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.92
183.00	11.40	12.60
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/16/2021	BNA_P	BP007991.D
Compound Name	Response	Retention Time
DDT	1058324	20.63
DDD	11436	20.2
DDE	2214	19.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13650	1071974	1.27

Instrument :
BNA_P
ClientSampleId :
DFTPP