
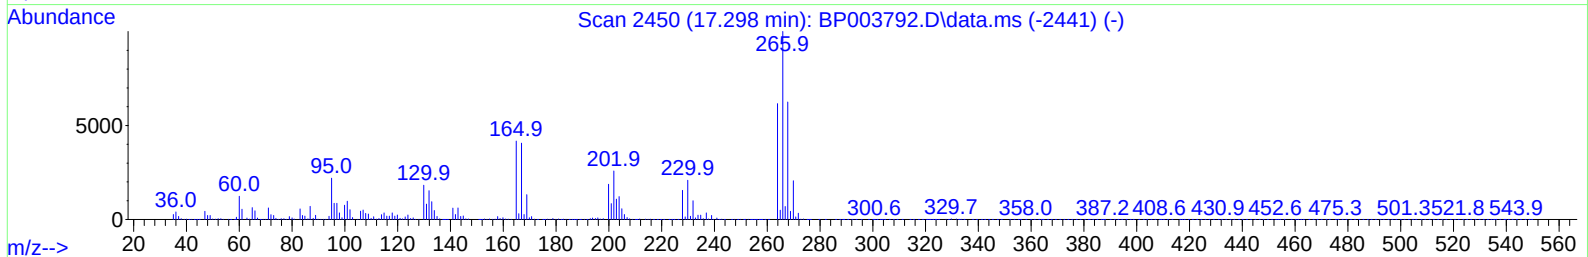
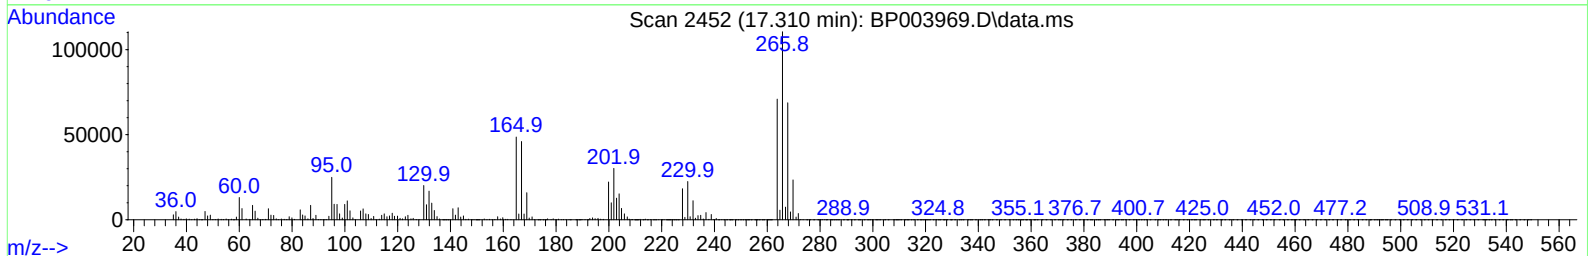


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP111720\  
Data File : BP003969.D  
Acq On : 17 Nov 2020 11:31  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 18 03:46:53 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\8270-BP110320.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Nov 12 15:22:47 2020  
Response via : Initial Calibration

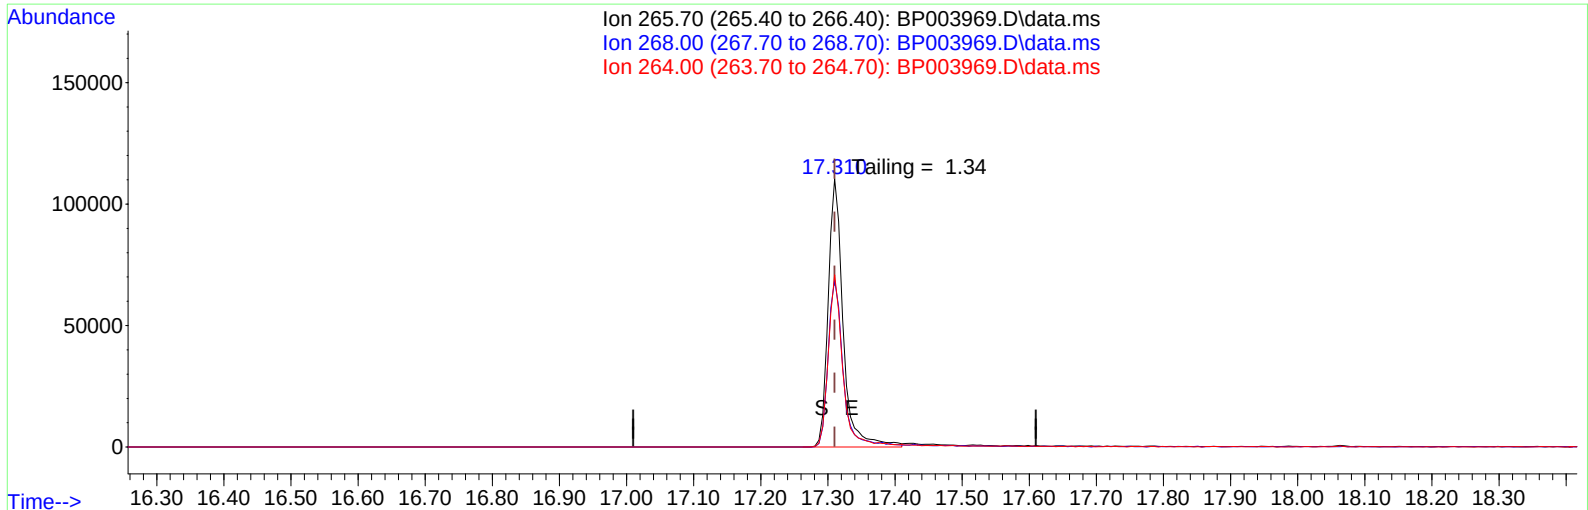

TIC: BP003969.D\data.ms

**(70) Pentachlorophenol (C)**




17.310min (+ 0.000) 727294.32 ng

response 171858

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.90  | 62.20  |
| 264.00 | 63.30  | 64.18  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP111720\  
Data File : BP003969.D  
Acq On : 17 Nov 2020 11:31  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 18 03:46:53 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\8270-BP110320.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Nov 12 15:22:47 2020  
Response via : Initial Calibration

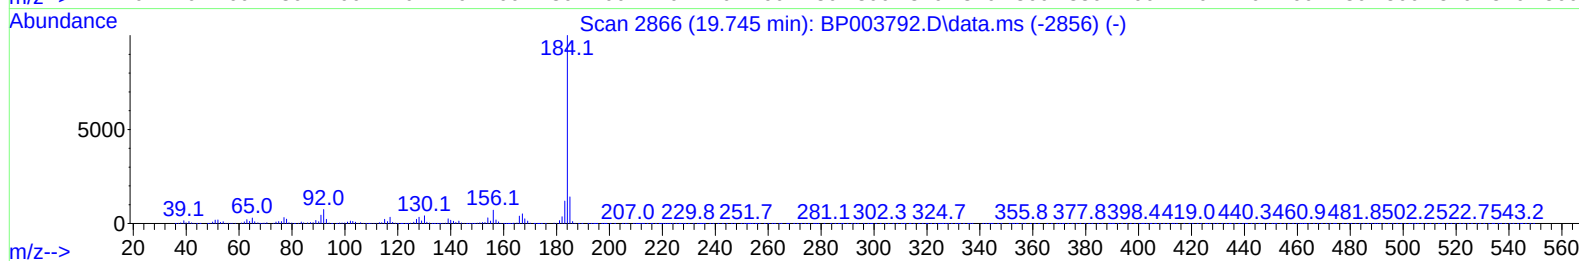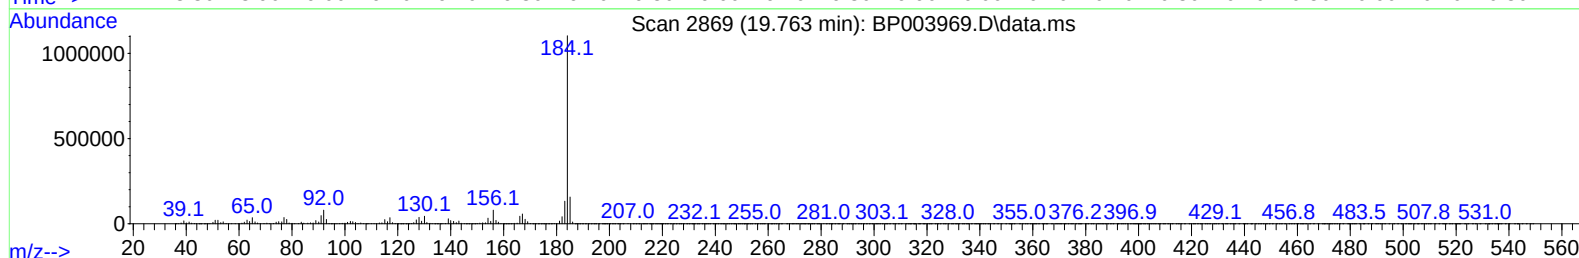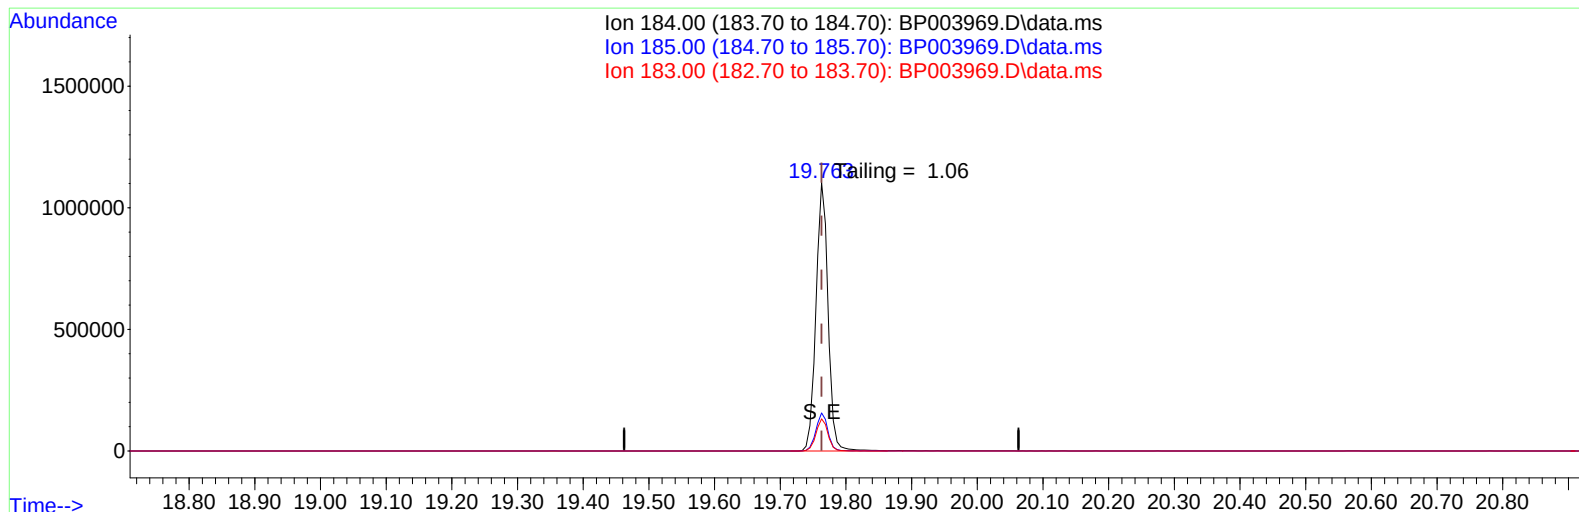

TIC: BP003969.D\data.ms

**(77) Benzidine****19.763min (+ 0.000) 252881.02 ng****response 1413670**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.40  | 14.20  |
| 183.00 | 12.00  | 12.00  |
| 0.00   | 0.00   | 0.00   |