




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
 Data File : BP018226.D
 Acq On : 17 Nov 2023 17:54
 Operator : MA/JU
 Sample : 05369-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCDN6

Manual IntegrationsAPPROVED

Quant Time: Nov 17 21:52:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 15 18:13:37 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
 Supervised By :mohammad ahmed 11/19/2023

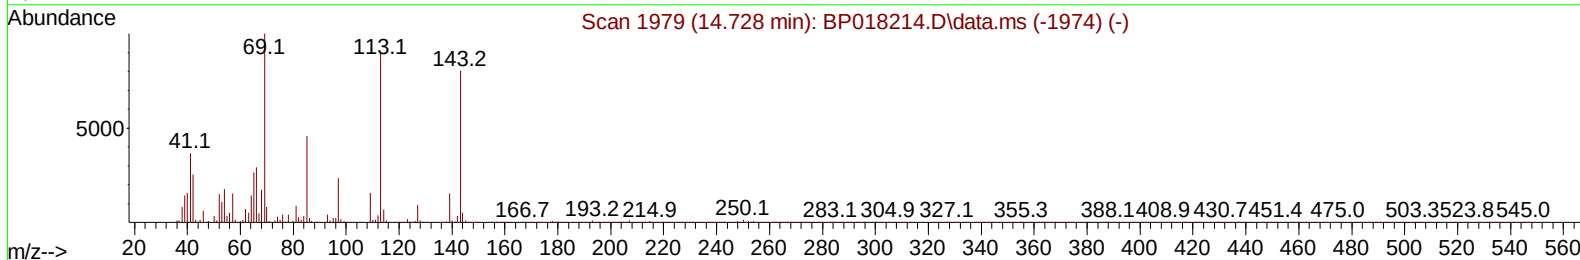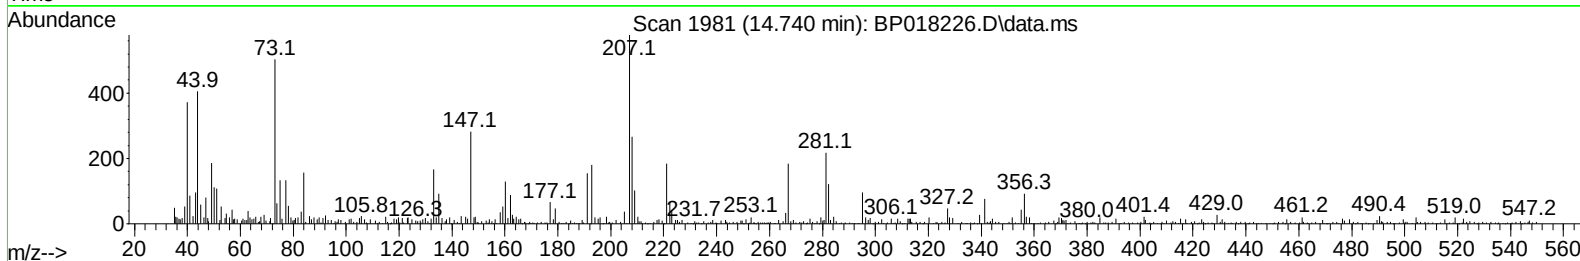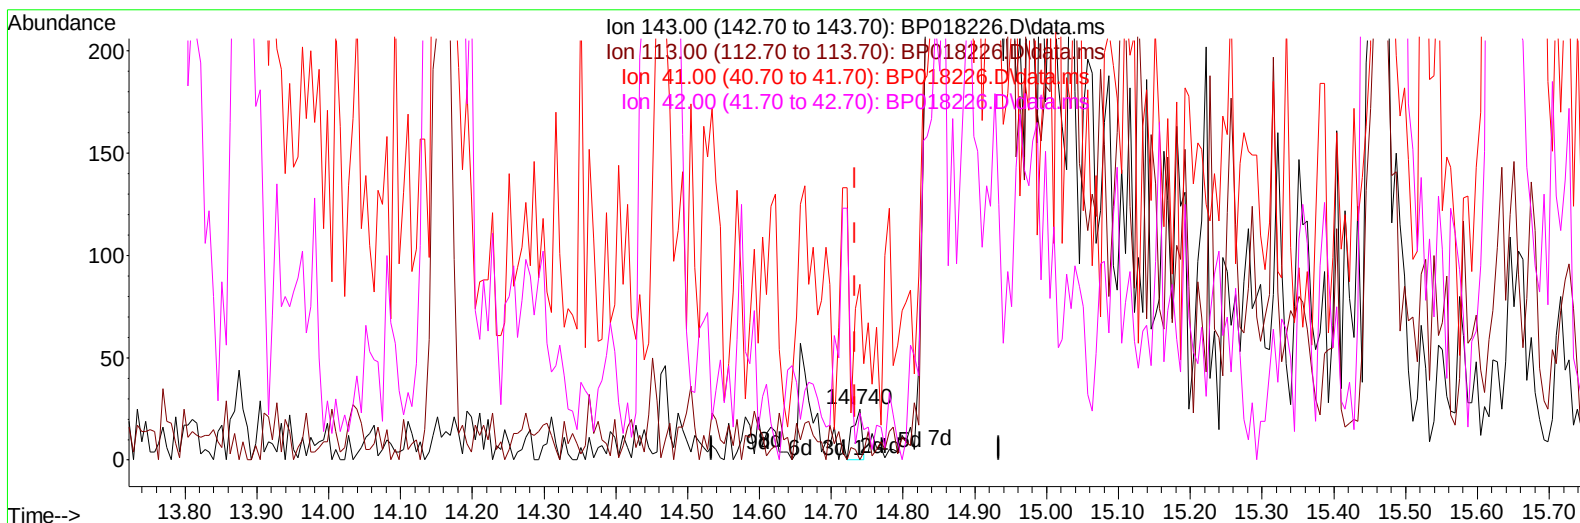

TIC: BP018226.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.740min (+ 0.006) 0.02 ng/ul

response 22

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.00	0.00#
41.00	47.70	344.00#
42.00	30.10	92.00#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
Data File : BP018226.D
Acq On : 17 Nov 2023 17:54
Operator : MA/JU
Sample : 05369-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCDN6

Manual IntegrationsAPPROVED

Quant Time: Nov 17 21:52:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 15 18:13:37 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
Supervised By :mohammad ahmed 11/19/2023

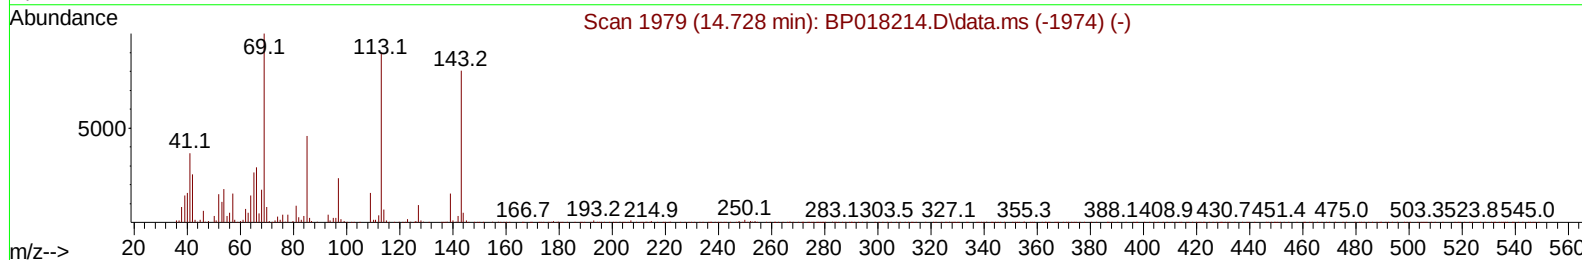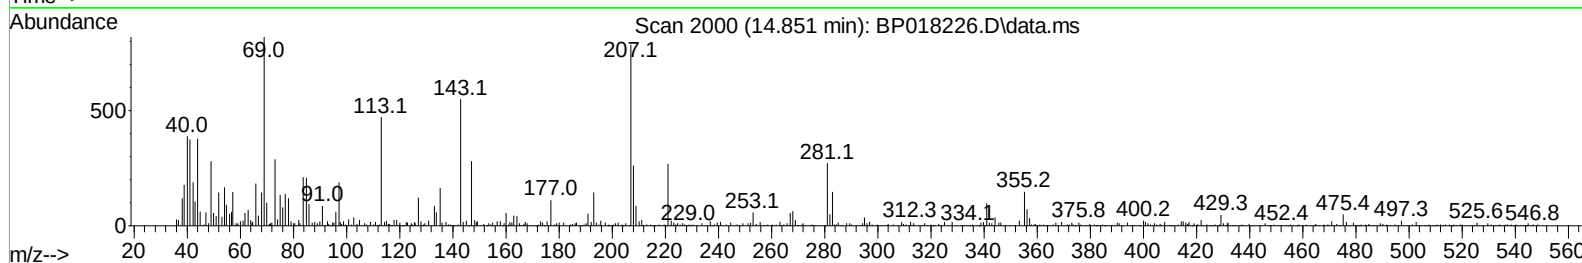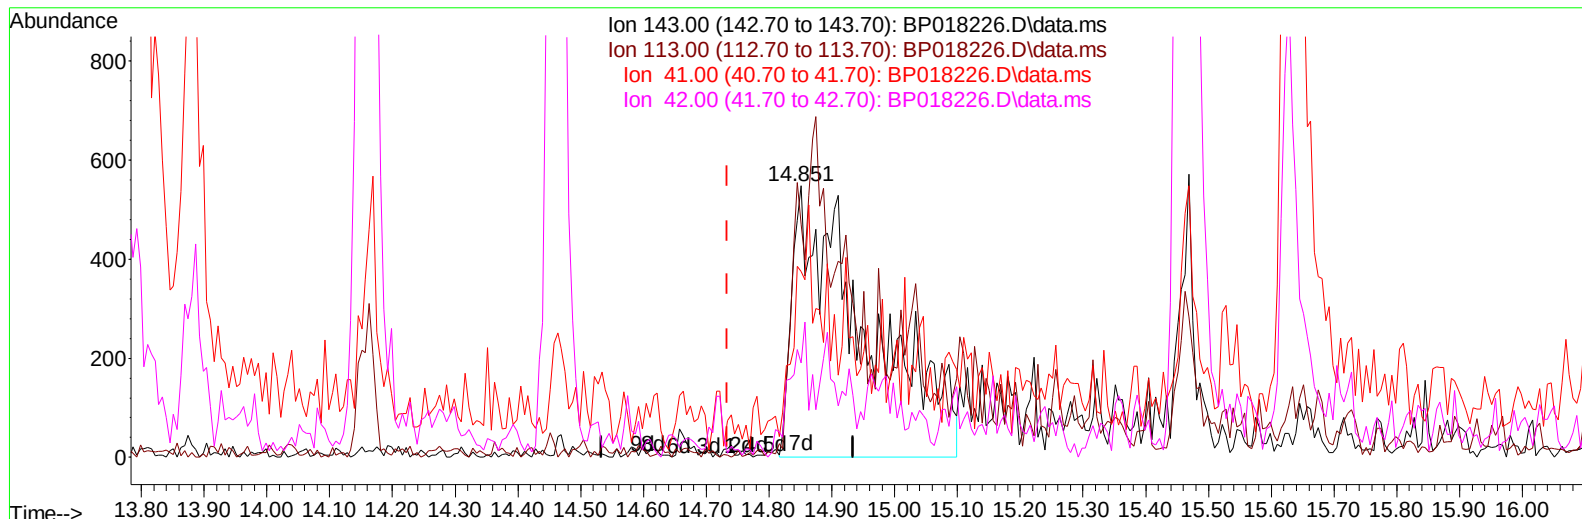

TIC: BP018226.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.851min (+ 0.118) 3.62 ng/ul m

response 4479

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.00	85.95
41.00	47.70	68.43#
42.00	30.10	34.67

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
 Data File : BP018226.D
 Acq On : 17 Nov 2023 17:54
 Operator : MA/JU
 Sample : 05369-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCDN6

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/19/2023
 Supervised By :mohammad ahmed 11/19/2023

Quant Time: Nov 17 22:24:04 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 15 18:13:37 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.781	152	35357	20.000	ng/ul	0.00
20) Naphthalene-d8	10.599	136	128574	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.463	164	89696	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.245	188	196771	20.000	ng/ul	0.00
79) Chrysene-d12	21.380	240	193563	20.000	ng/ul	0.00
88) Perylene-d12	23.851	264	224166	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.158	96	5050	5.038	ng/uL	0.00
4) Pyridine-d5	3.605	84	23404	8.956	ng/ul	0.01
7) Phenol-d5	6.969	99	20192	5.915	ng/ul	0.02
9) Bis-(2-Chloroethyl)eth...	7.134	67	95532	47.623	ng/ul	0.00
11) 2-Chlorophenol-d4	7.305	132	86756	32.095	ng/ul	0.00
15) 4-Methylphenol-d8	8.516	113	48048	17.178	ng/ul	0.00
21) Nitrobenzene-d5	8.993	128	56232	48.544	ng/ul	0.00
24) 2-Nitrophenol-d4	9.705	143	49014	37.349	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.234	165	73531	31.437	ng/ul	0.00
31) 4-Chloroaniline-d4	10.787	131	96930	30.219	ng/ul	0.00
46) Dimethylphthalate-d6	13.887	166	381459	46.092	ng/ul	0.00
49) Acenaphthylene-d8	14.157	160	394698	43.787	ng/ul	0.00
54) 4-Nitrophenol-d4	14.851	143	4479m	3.622	ng/ul	0.12
60) Fluorene-d10	15.463	176	314941	46.092	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.628	200	48452	34.061	ng/ul	0.00
73) Anthracene-d10	17.345	188	540206	50.761	ng/ul	0.00
81) Pyrene-d10	19.598	212	667159	51.601	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.686	264	673673	51.683	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
Data File : BP018226.D
Acq On : 17 Nov 2023 17:54
Operator : MA/JU
Sample : 05369-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCDN6

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/19/2023
Supervised By :mohammad ahmed 11/19/2023

Quant Time: Nov 17 22:24:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 15 18:13:37 2023
Response via : Initial Calibration

