




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
 Data File : BP018232.D
 Acq On : 17 Nov 2023 21:57
 Operator : MA/JU
 Sample : 05369-16
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCDP3

Manual IntegrationsAPPROVED

Quant Time: Nov 17 22:40:20 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 15 18:13:37 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
 Supervised By :mohammad ahmed 11/19/2023

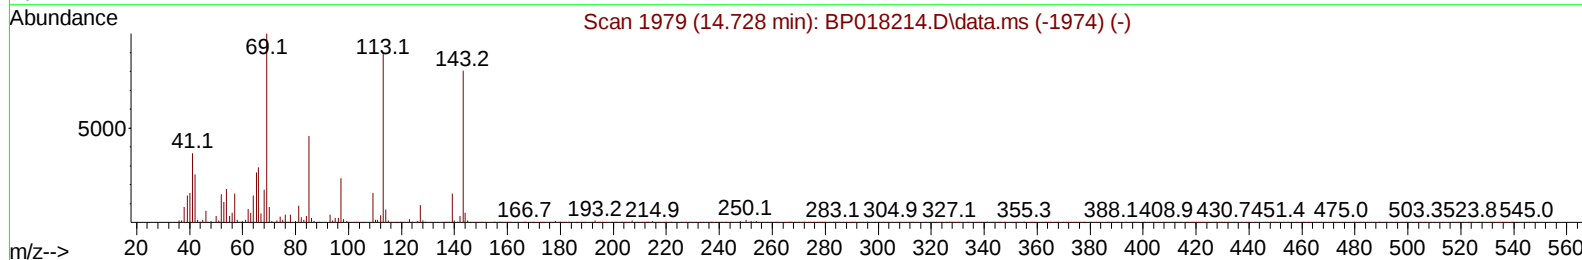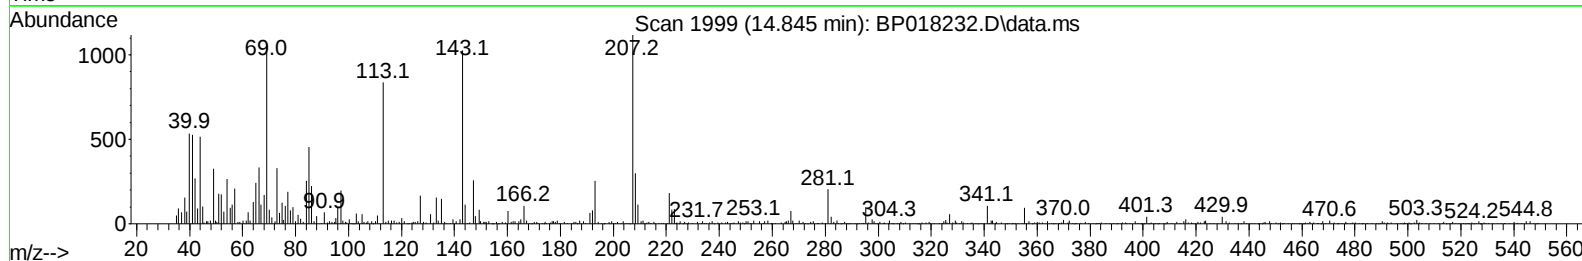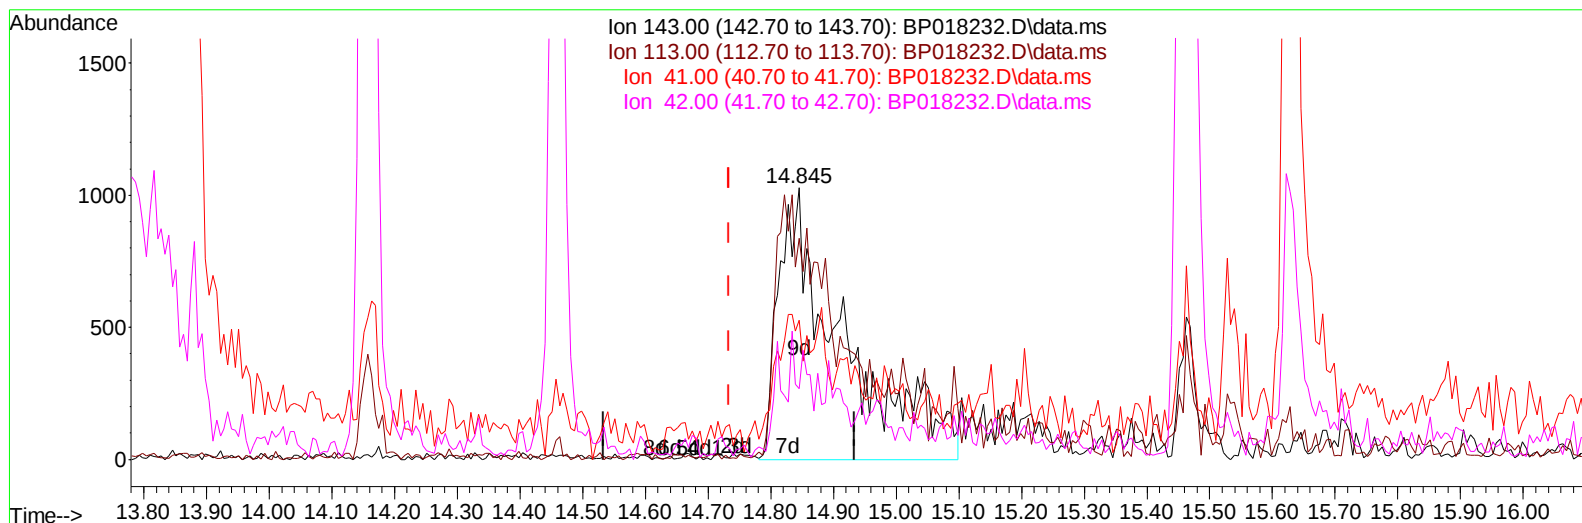

TIC: BP018232.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.845min (+ 0.112) 4.63 ng/ul m

response 7256

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.00	81.32#
41.00	47.70	51.26
42.00	30.10	26.07

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
 Data File : BP018232.D
 Acq On : 17 Nov 2023 21:57
 Operator : MA/JU
 Sample : 05369-16
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCDP3

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/19/2023
 Supervised By :mohammad ahmed 11/19/2023

Quant Time: Nov 17 22:40:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 15 18:13:37 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.781	152	43552	20.000	ng/ul	0.00
20) Naphthalene-d8	10.599	136	162089	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.457	164	113780	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.245	188	264069	20.000	ng/ul	0.00
79) Chrysene-d12	21.375	240	262799	20.000	ng/ul	0.00
88) Perylene-d12	23.851	264	294650	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.158	96	7155	5.795	ng/uL	0.00
4) Pyridine-d5	3.605	84	43490	13.510	ng/ul	0.01
7) Phenol-d5	6.964	99	24392	5.801	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	7.134	67	101974	41.269	ng/ul	0.00
11) 2-Chlorophenol-d4	7.305	132	95332	28.631	ng/ul	0.00
15) 4-Methylphenol-d8	8.511	113	57537	16.700	ng/ul	0.00
21) Nitrobenzene-d5	8.987	128	63709	43.626	ng/ul	0.00
24) 2-Nitrophenol-d4	9.699	143	62536	37.799	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.234	165	98149	33.286	ng/ul	0.00
31) 4-Chloroaniline-d4	10.781	131	137970	34.120	ng/ul	0.00
46) Dimethylphthalate-d6	13.881	166	460325	43.848	ng/ul	0.00
49) Acenaphthylene-d8	14.157	160	466341	40.784	ng/ul	0.00
54) 4-Nitrophenol-d4	14.845	143	7256m	4.625	ng/ul	0.11
60) Fluorene-d10	15.463	176	377665	43.573	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.628	200	63270	33.143	ng/ul	0.00
73) Anthracene-d10	17.339	188	637053	44.606	ng/ul	0.00
81) Pyrene-d10	19.598	212	808826	46.077	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.686	264	807593	47.137	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
Data File : BP018232.D
Acq On : 17 Nov 2023 21:57
Operator : MA/JU
Sample : 05369-16
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCDP3

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/19/2023
Supervised By :mohammad ahmed 11/19/2023

Quant Time: Nov 17 22:40:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 15 18:13:37 2023
Response via : Initial Calibration

