




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
 Data File : BP018234.D
 Acq On : 17 Nov 2023 23:05
 Operator : MA/JU
 Sample : 05369-18MSD
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCDP3MSD

Manual IntegrationsAPPROVED

Quant Time: Nov 17 23:41:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 15 18:13:37 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
 Supervised By :mohammad ahmed 11/19/2023

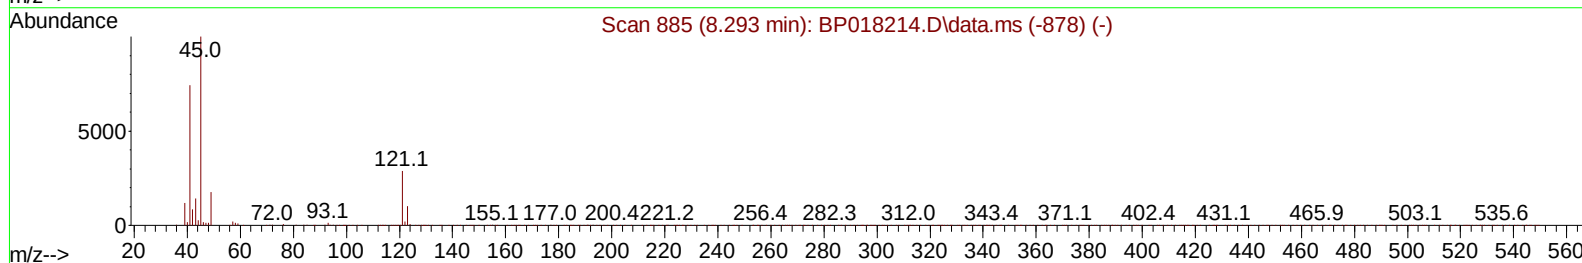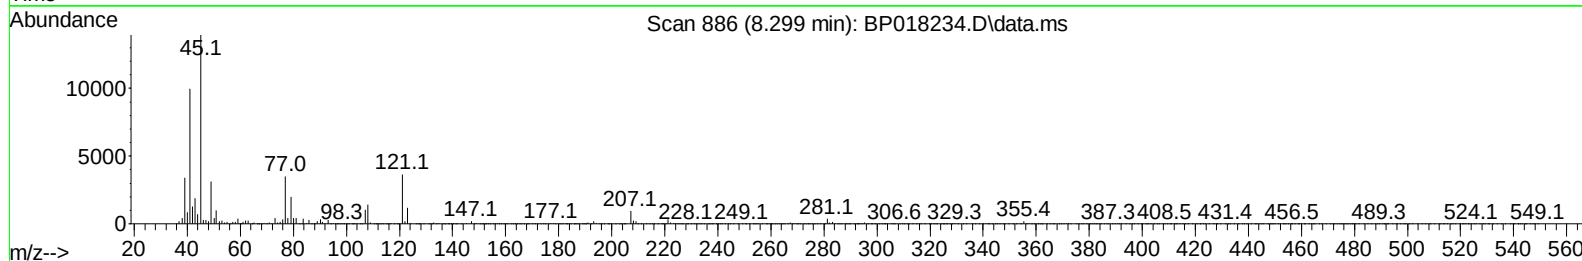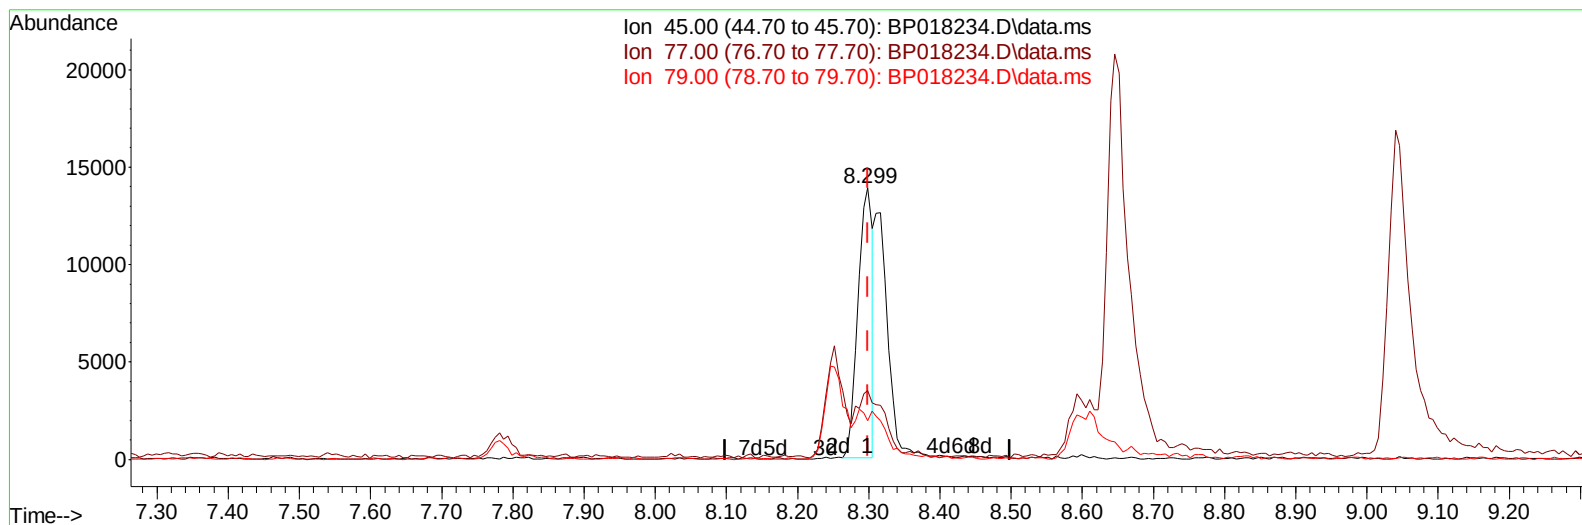

TIC: BP018234.D\data.ms

(14) 2,2'-oxybis(1-Chloropropane)

8.299min (+ 0.000) 4.83 ng/ul

response 19671

Ion	Exp%	Act%
45.00	100.00	100.00
77.00	20.10	25.25#
79.00	13.90	14.33
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
 Data File : BP018234.D
 Acq On : 17 Nov 2023 23:05
 Operator : MA/JU
 Sample : 05369-18MSD
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCDP3MSD

Manual IntegrationsAPPROVED

Quant Time: Nov 17 23:41:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 15 18:13:37 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
 Supervised By :mohammad ahmed 11/19/2023

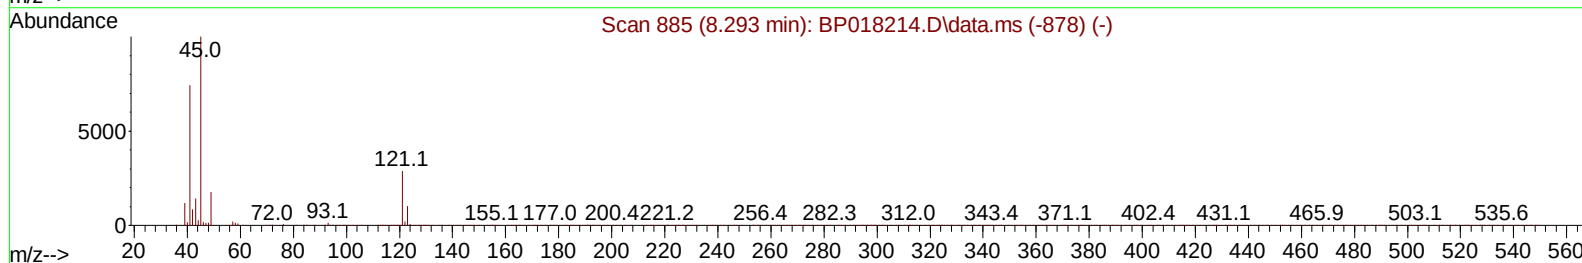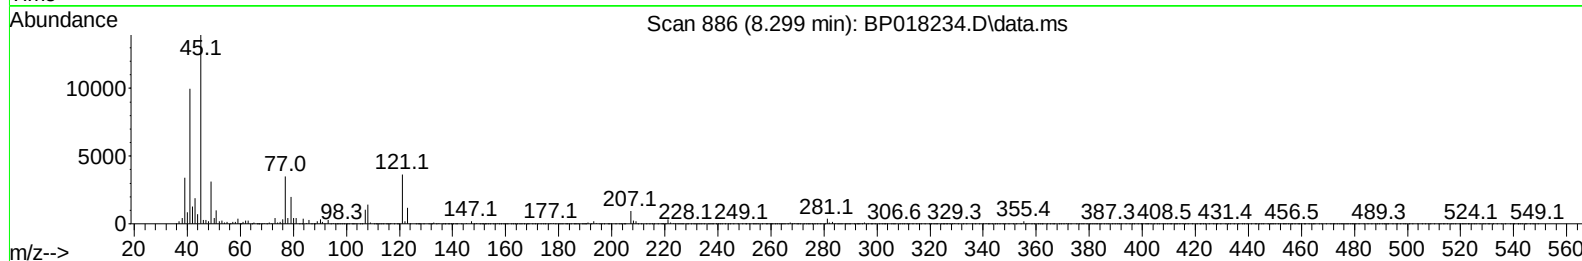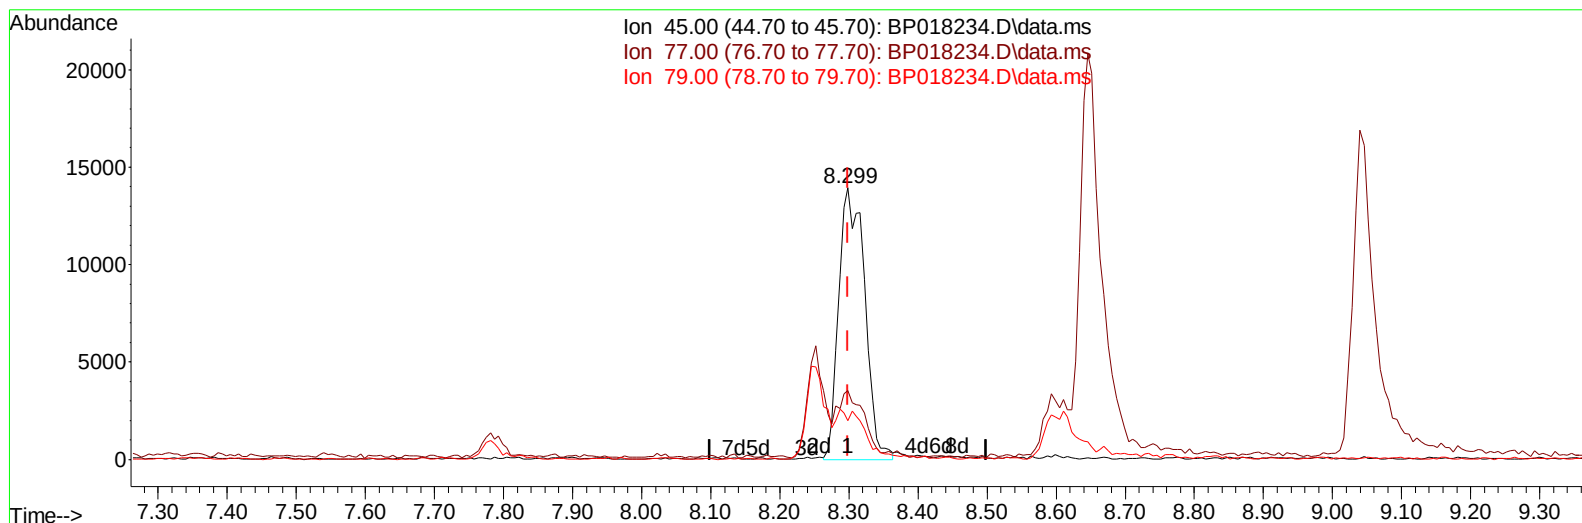

TIC: BP018234.D\data.ms

(14) 2,2'-oxybis(1-Chloropropane)

8.299min (+ 0.000) 8.88 ng/ul m

response 36175

Ion	Exp%	Act%
45.00	100.00	100.00
77.00	20.10	25.25#
79.00	13.90	14.33
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
Data File : BP018234.D
Acq On : 17 Nov 2023 23:05
Operator : MA/JU
Sample : 05369-18MSD
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCDP3MSD

Manual IntegrationsAPPROVED

Quant Time: Nov 17 23:41:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 15 18:13:37 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
Supervised By :mohammad ahmed 11/19/2023

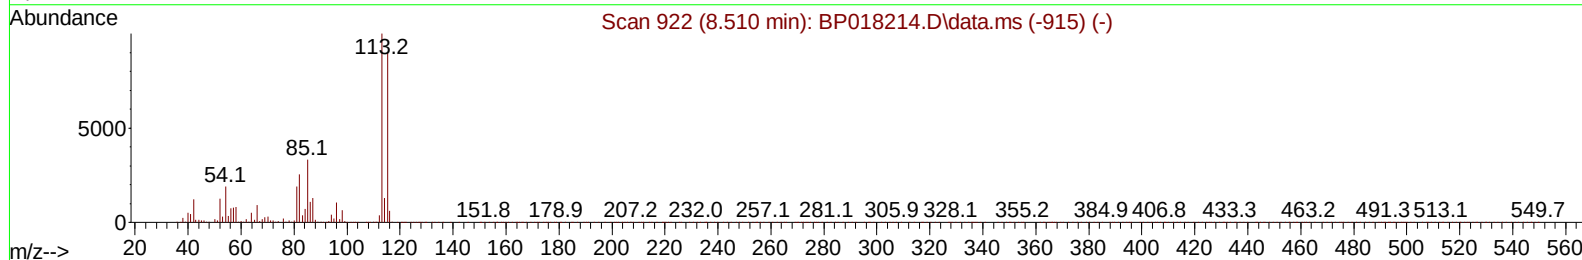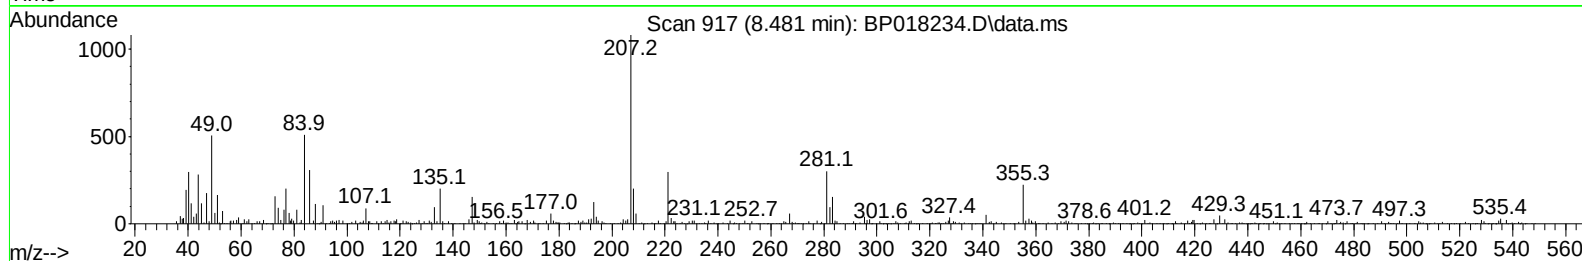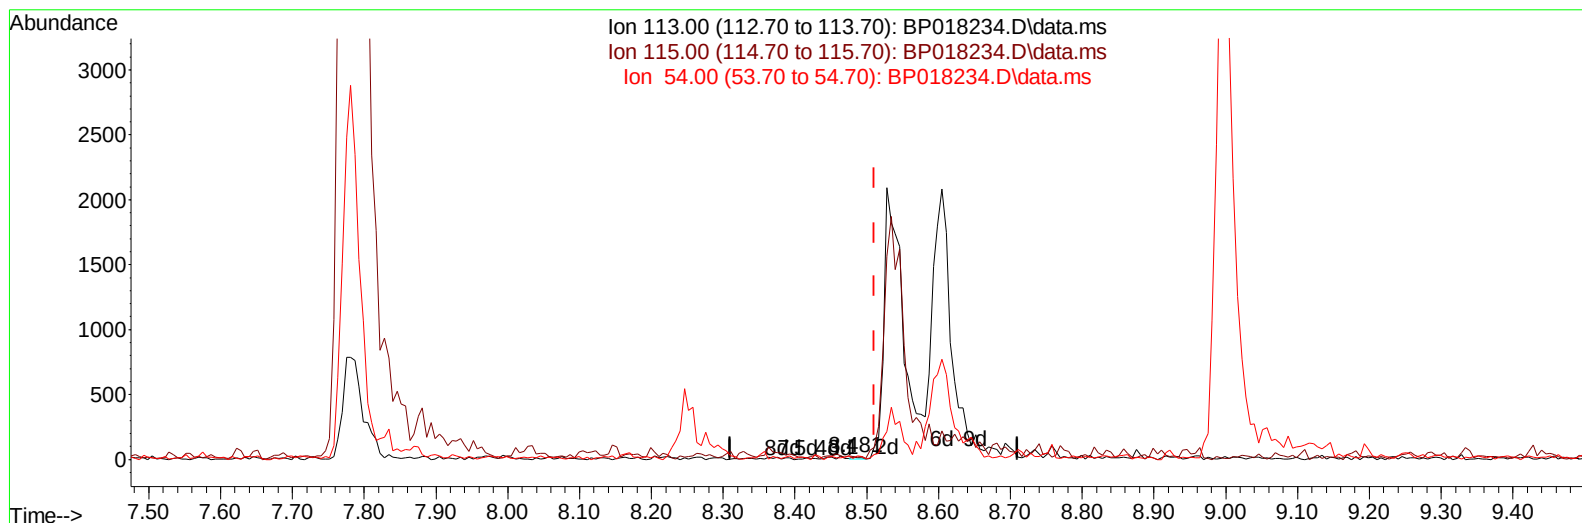

TIC: BP018234.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.481min (-0.029) 0.00 ng/u1

response 12

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	90.80	127.78#
54.00	17.00	33.33#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
Data File : BP018234.D
Acq On : 17 Nov 2023 23:05
Operator : MA/JU
Sample : 05369-18MSD
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCDP3MSD

Manual IntegrationsAPPROVED

Quant Time: Nov 17 23:41:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 15 18:13:37 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
Supervised By :mohammad ahmed 11/19/2023

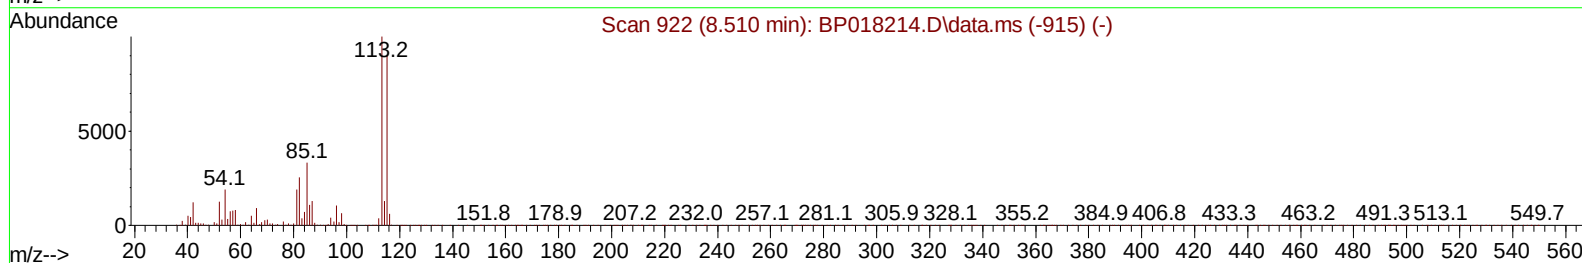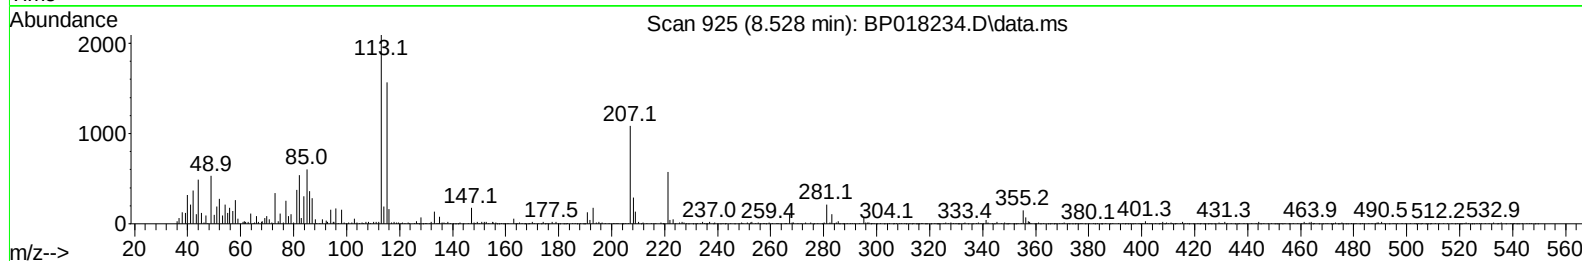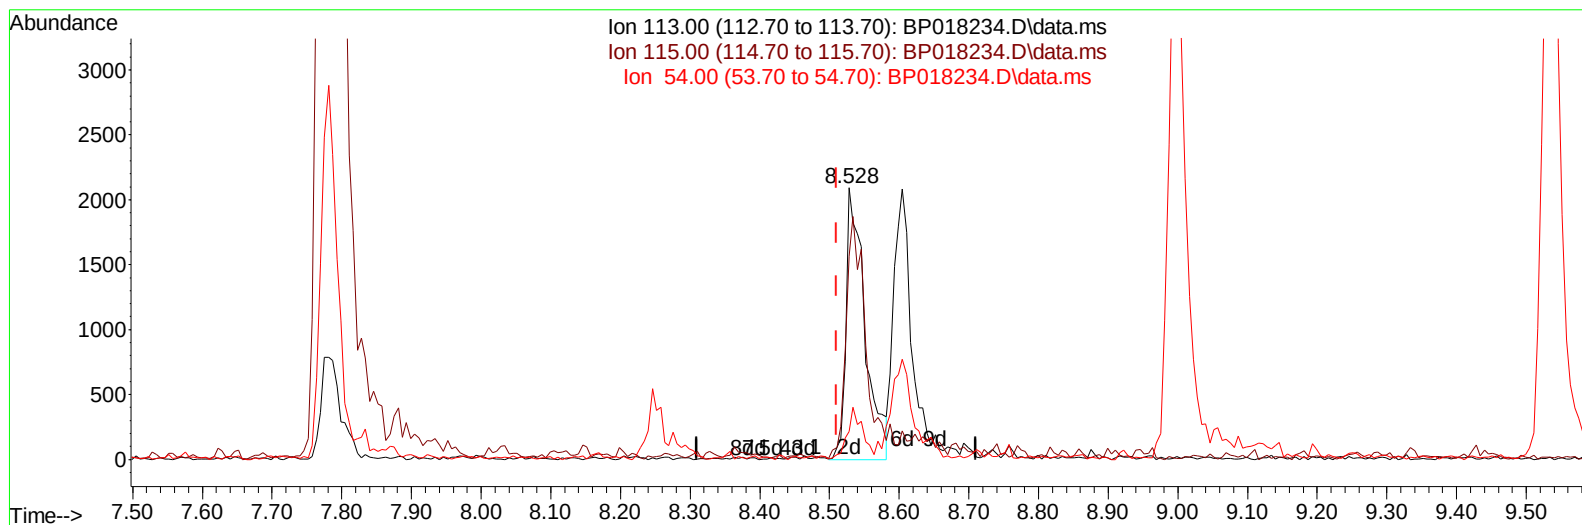

TIC: BP018234.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.528min (+ 0.018) 1.03 ng/ul m

response 3943

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	90.80	74.80
54.00	17.00	10.28#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
Data File : BP018234.D
Acq On : 17 Nov 2023 23:05
Operator : MA/JU
Sample : 05369-18MSD
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCDP3MSD

Manual IntegrationsAPPROVED

Quant Time: Nov 17 23:41:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 15 18:13:37 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
Supervised By :mohammad ahmed 11/19/2023

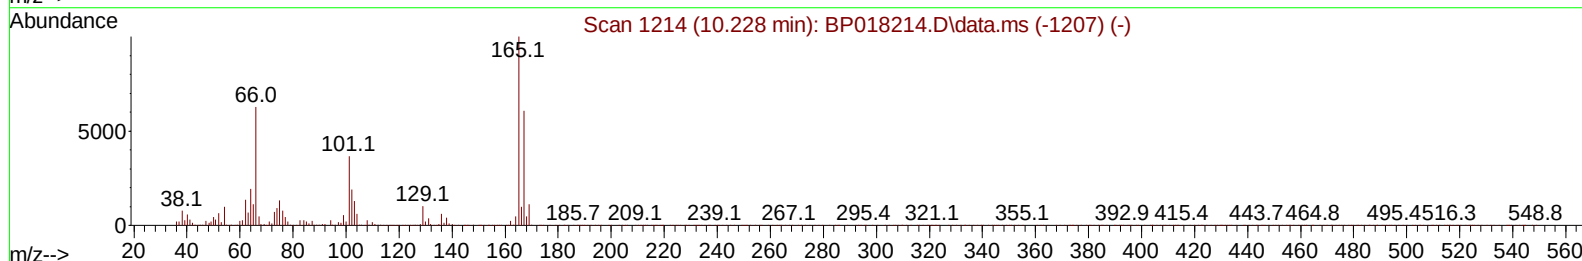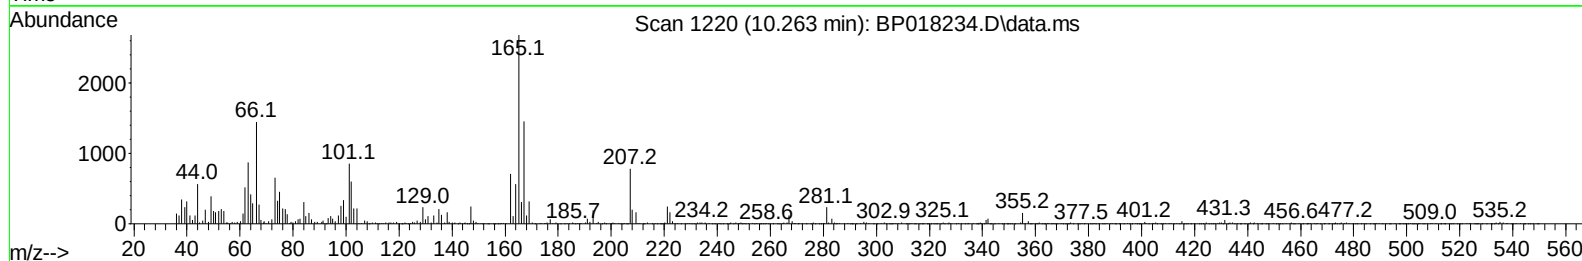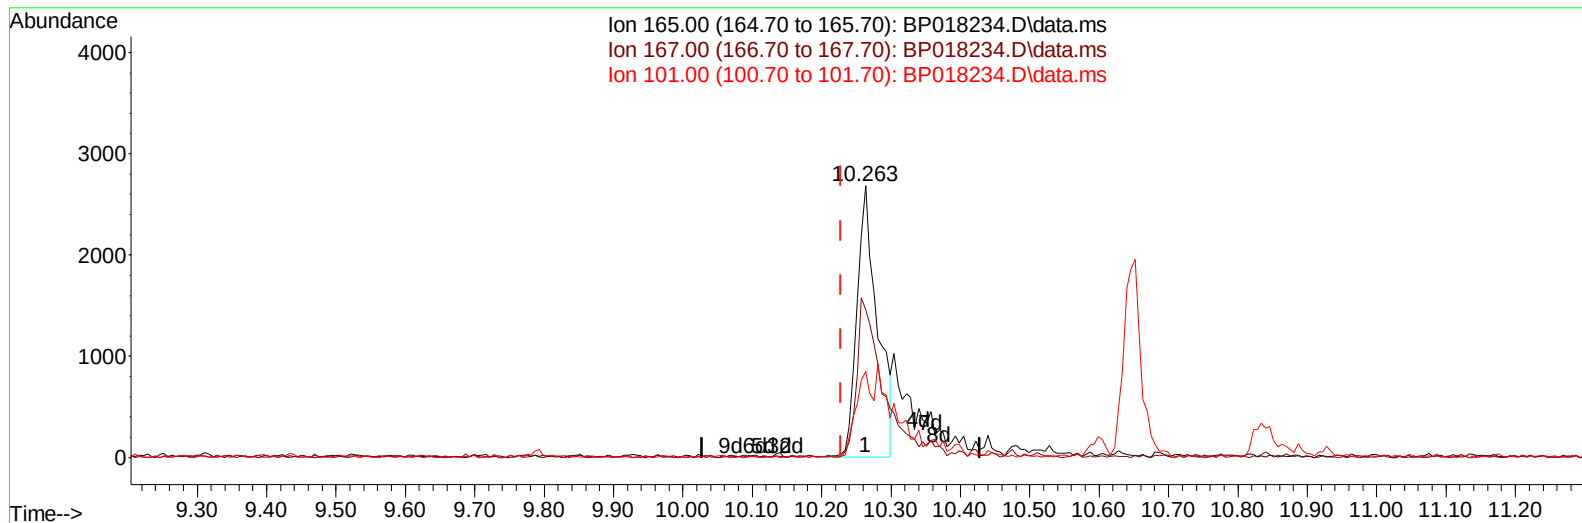

TIC: BP018234.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.263min (+ 0.035) 1.60 ng/ul

response 5456

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	61.40	54.25
101.00	35.50	31.80
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
 Data File : BP018234.D
 Acq On : 17 Nov 2023 23:05
 Operator : MA/JU
 Sample : 05369-18MSD
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCDP3MSD

Manual IntegrationsAPPROVED

Quant Time: Nov 17 23:41:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 15 18:13:37 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
 Supervised By :mohammad ahmed 11/19/2023

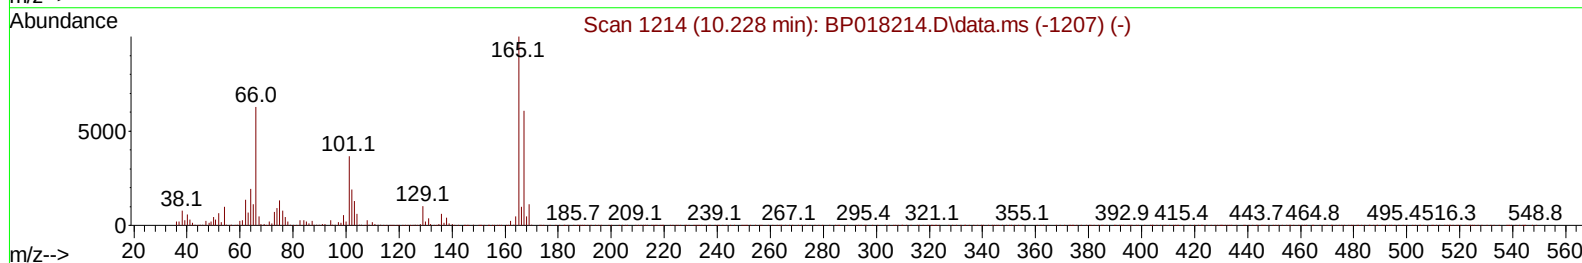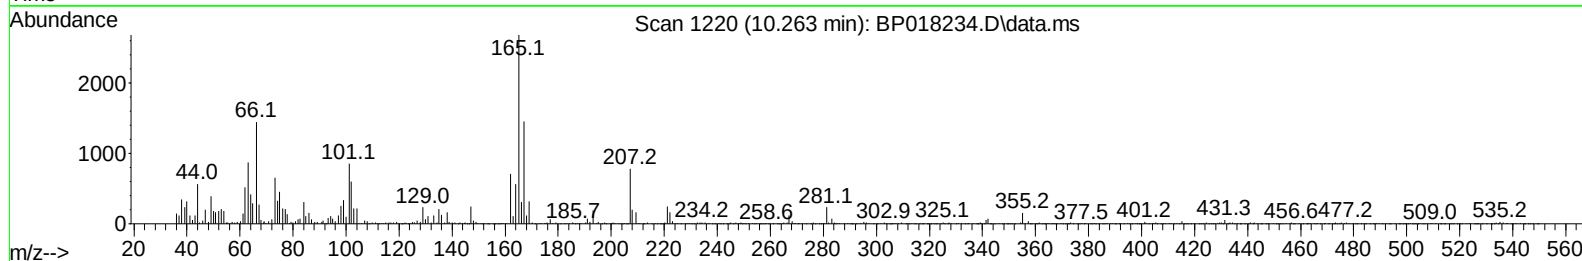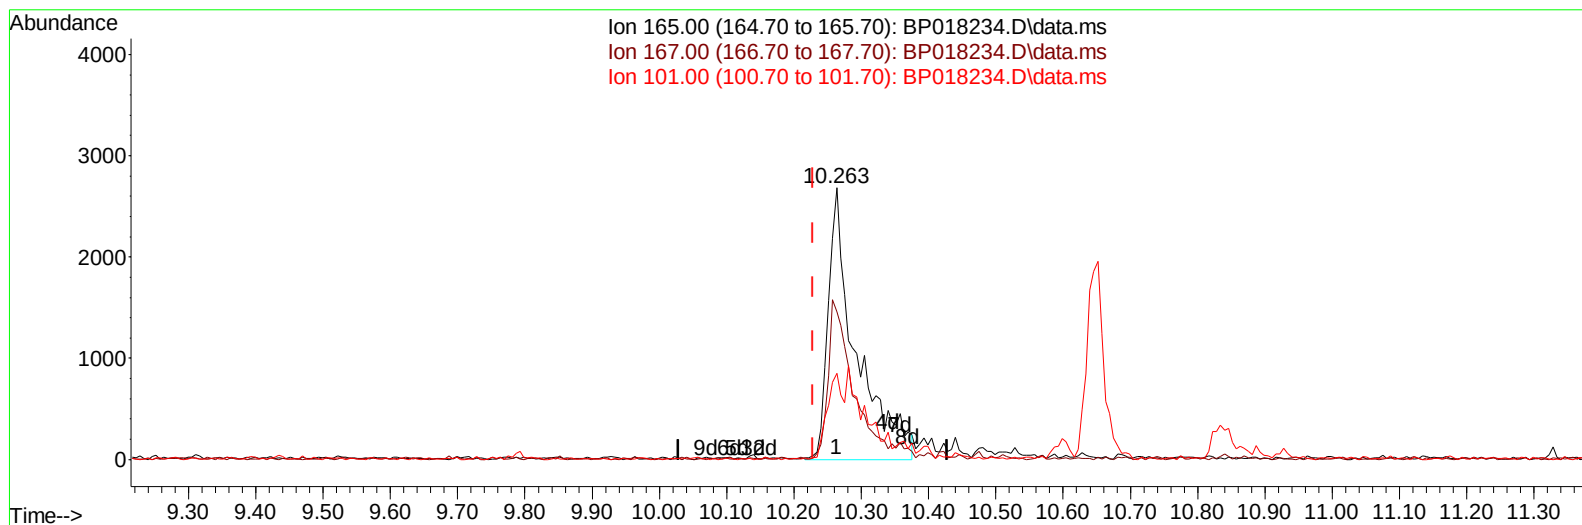

TIC: BP018234.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.263min (+ 0.035) 2.26 ng/ul m

response 7667

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	61.40	54.25
101.00	35.50	31.80
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
Data File : BP018234.D
Acq On : 17 Nov 2023 23:05
Operator : MA/JU
Sample : 05369-18MSD
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCDP3MSD

Manual IntegrationsAPPROVED

Quant Time: Nov 17 23:41:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 15 18:13:37 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
Supervised By :mohammad ahmed 11/19/2023

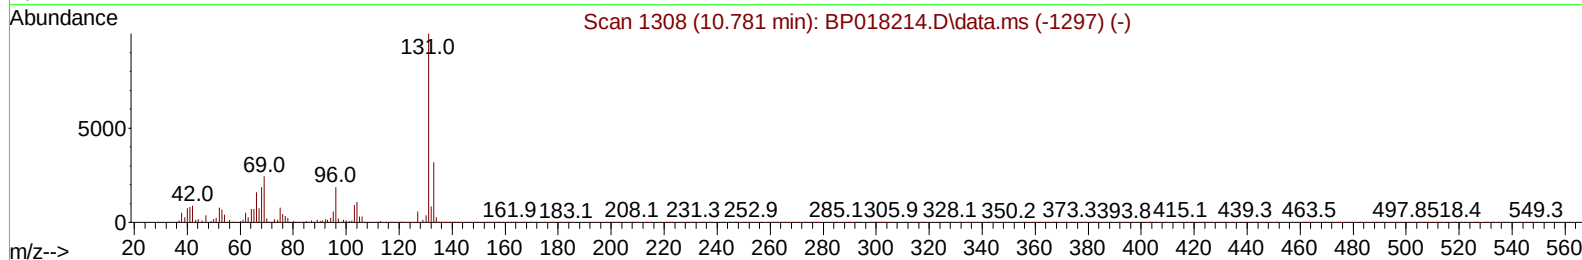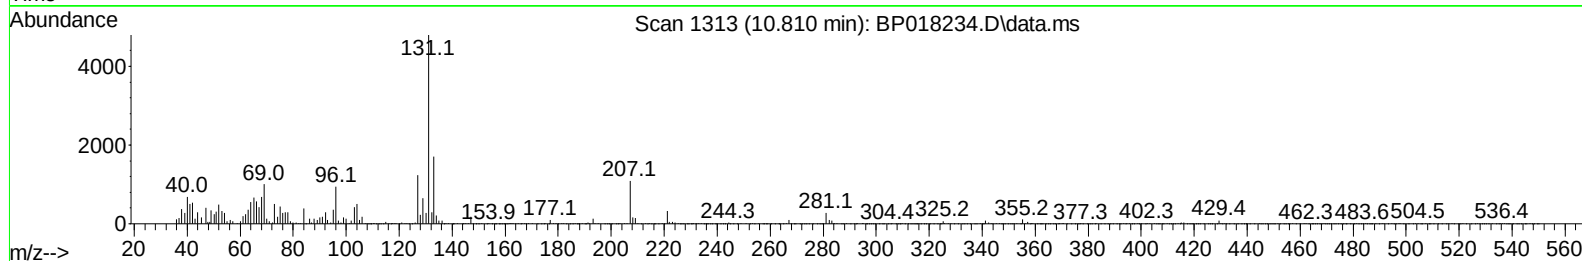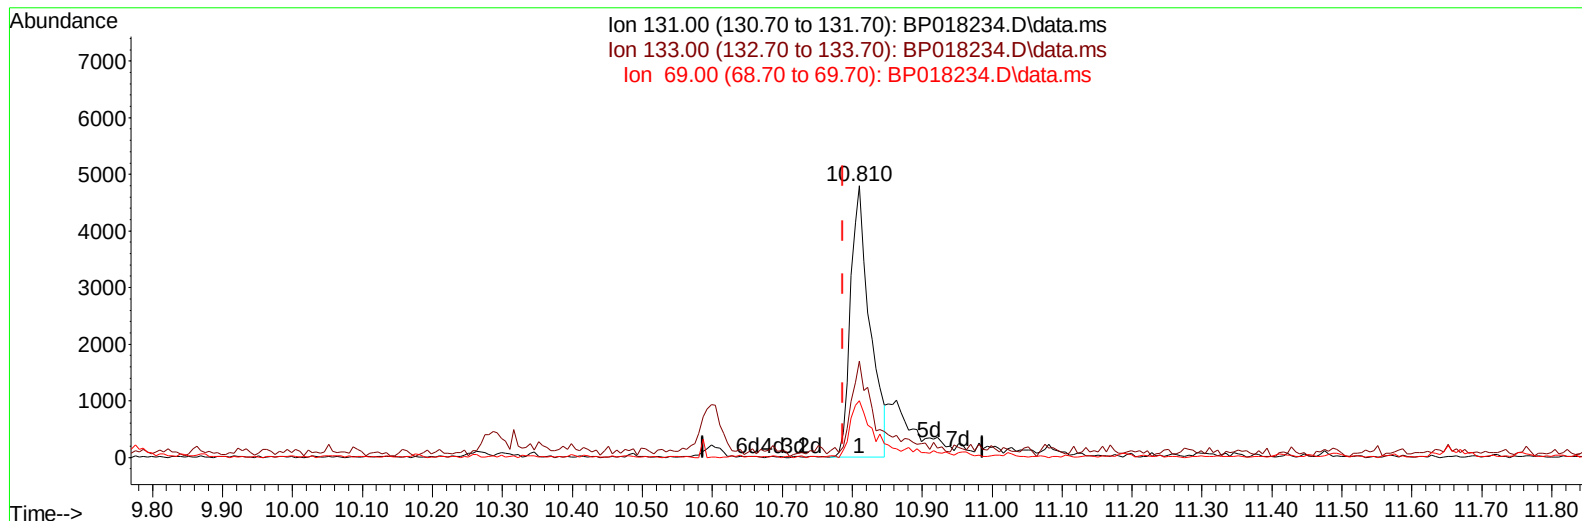

TIC: BP018234.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.810min (+ 0.024) 1.95 ng/u1

response 9102

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.20	35.45
69.00	20.00	20.92
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
 Data File : BP018234.D
 Acq On : 17 Nov 2023 23:05
 Operator : MA/JU
 Sample : 05369-18MSD
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCDP3MSD

Manual IntegrationsAPPROVED

Quant Time: Nov 17 23:41:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 15 18:13:37 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
 Supervised By :mohammad ahmed 11/19/2023

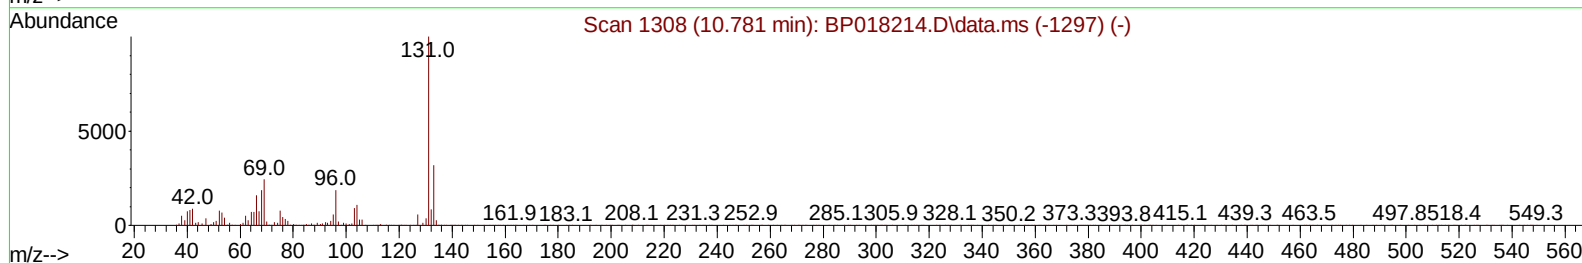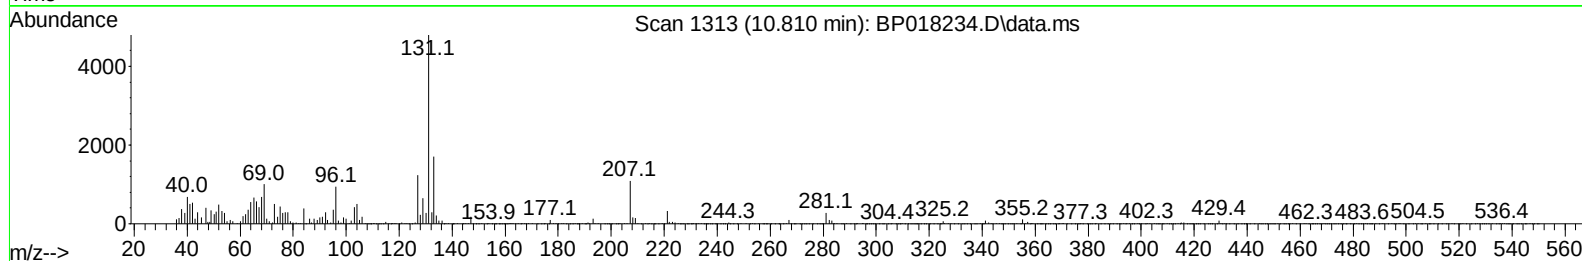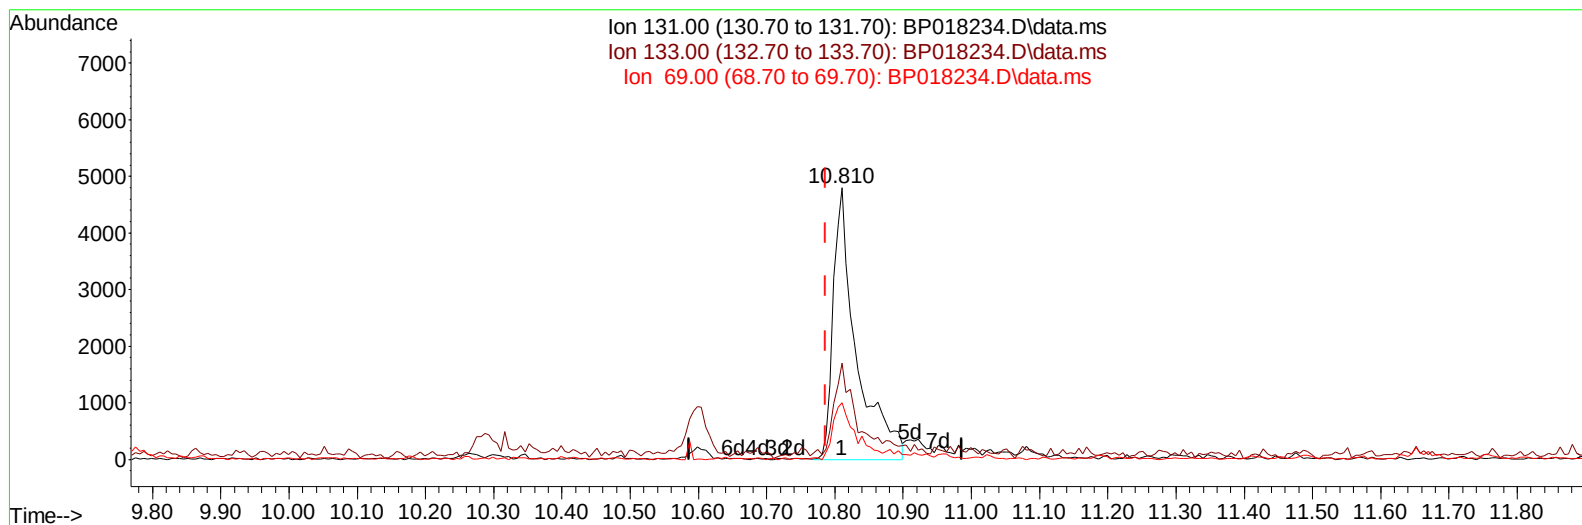

TIC: BP018234.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.810min (+ 0.024) 2.42 ng/ul m

response 11267

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.20	35.45
69.00	20.00	20.92
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
 Data File : BP018234.D
 Acq On : 17 Nov 2023 23:05
 Operator : MA/JU
 Sample : 05369-18MSD
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCDP3MSD

Manual IntegrationsAPPROVED

Quant Time: Nov 17 23:41:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 15 18:13:37 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
 Supervised By :mohammad ahmed 11/19/2023

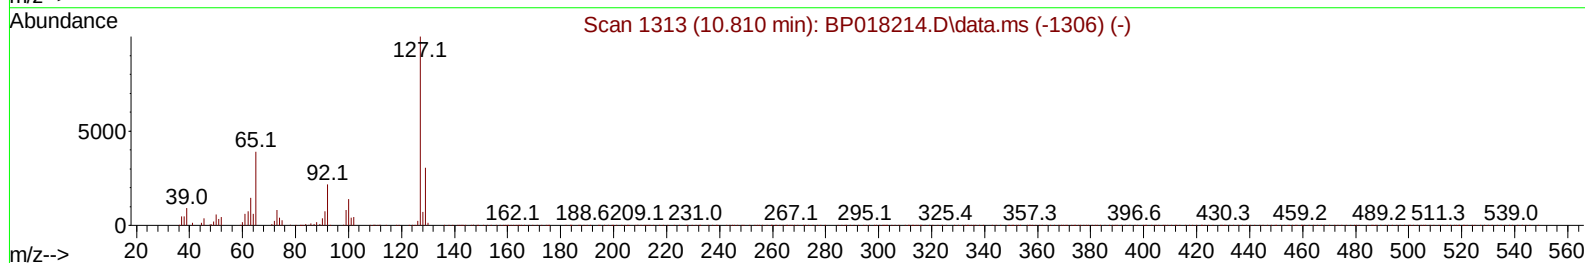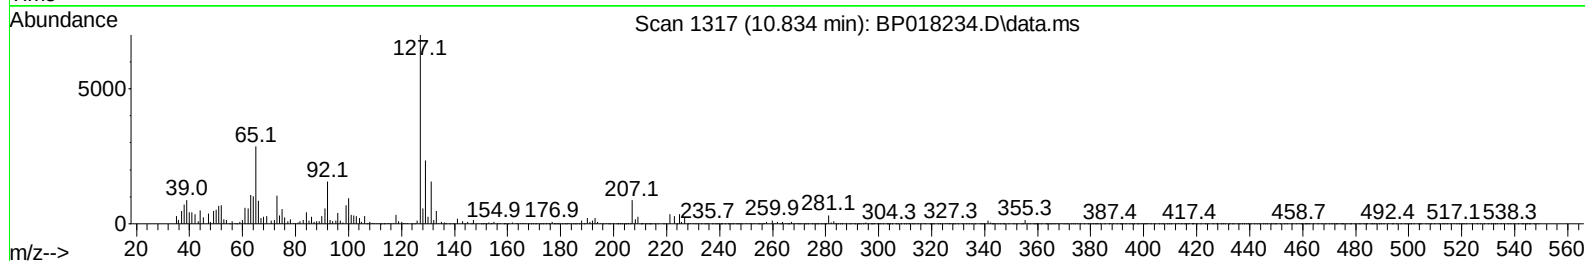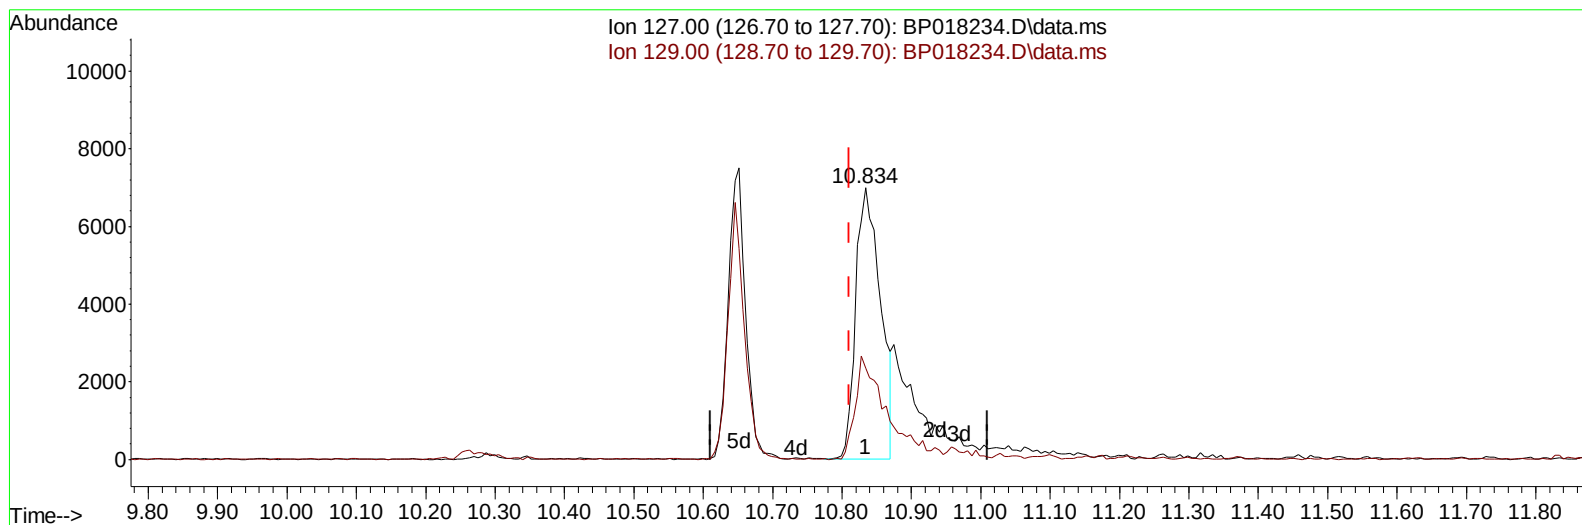

TIC: BP018234.D\data.ms

(32) 4-Chloroaniline

10.834min (+ 0.024) 3.88 ng/ul

response 17349

Ion	Exp%	Act%
127.00	100.00	100.00
129.00	32.60	33.64
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
 Data File : BP018234.D
 Acq On : 17 Nov 2023 23:05
 Operator : MA/JU
 Sample : 05369-18MSD
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCDP3MSD

Manual IntegrationsAPPROVED

Quant Time: Nov 17 23:41:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 15 18:13:37 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
 Supervised By :mohammad ahmed 11/19/2023

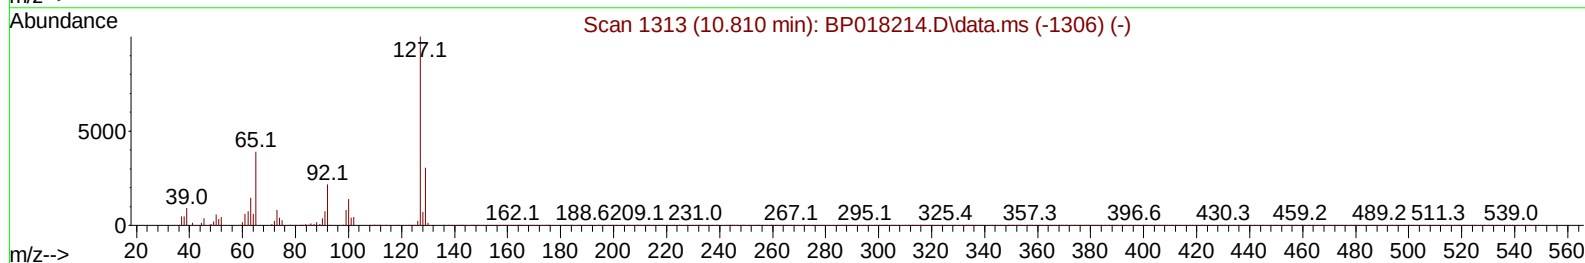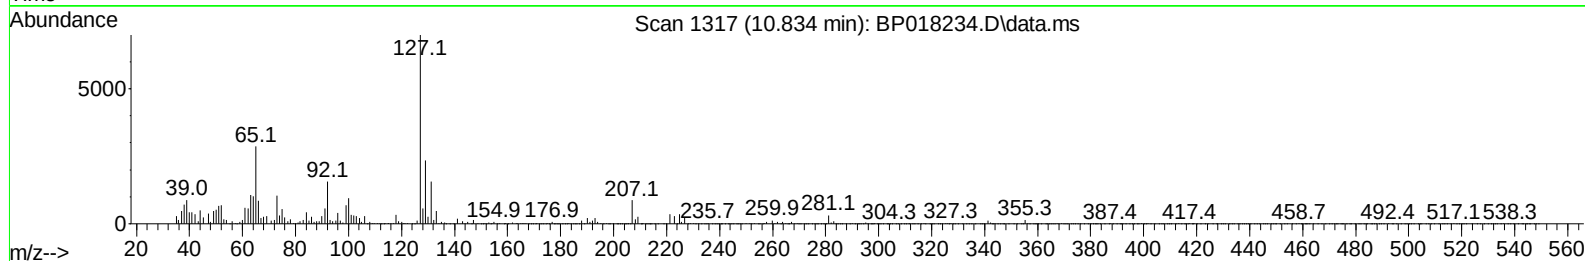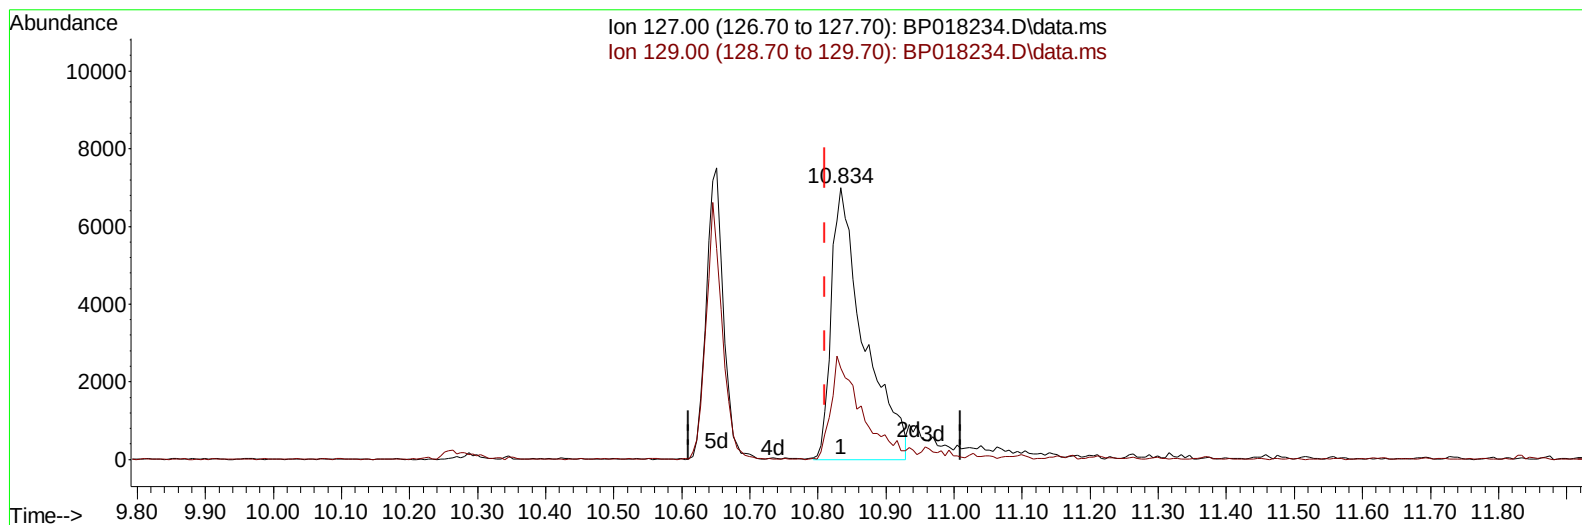

TIC: BP018234.D\data.ms

(32) 4-Chloroaniline

10.834min (+ 0.024) 5.21 ng/ul m

response 23251

Ion	Exp%	Act%
127.00	100.00	100.00
129.00	32.60	33.64
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
 Data File : BP018234.D
 Acq On : 17 Nov 2023 23:05
 Operator : MA/JU
 Sample : 05369-18MSD
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCDP3MSD

Manual IntegrationsAPPROVED

Quant Time: Nov 17 23:41:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 15 18:13:37 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
 Supervised By :mohammad ahmed 11/19/2023

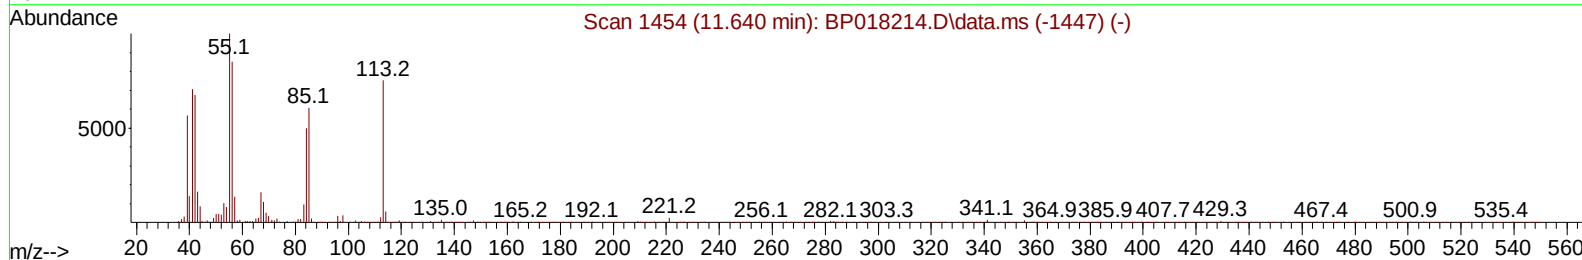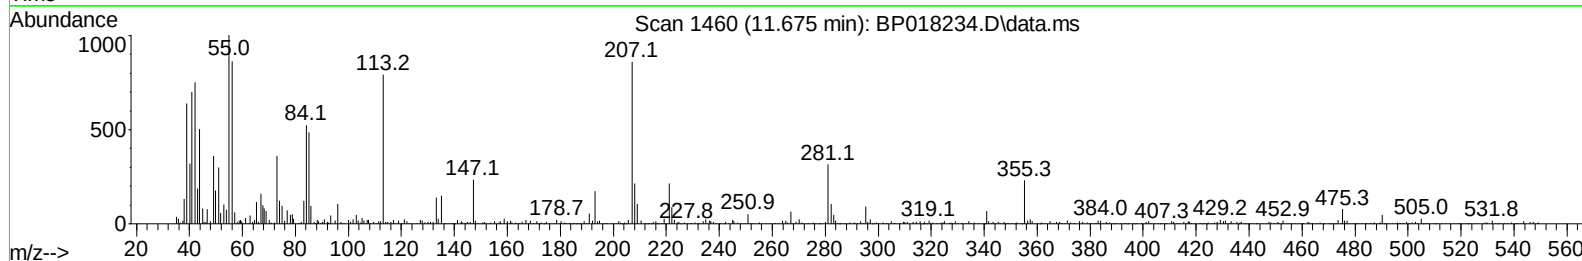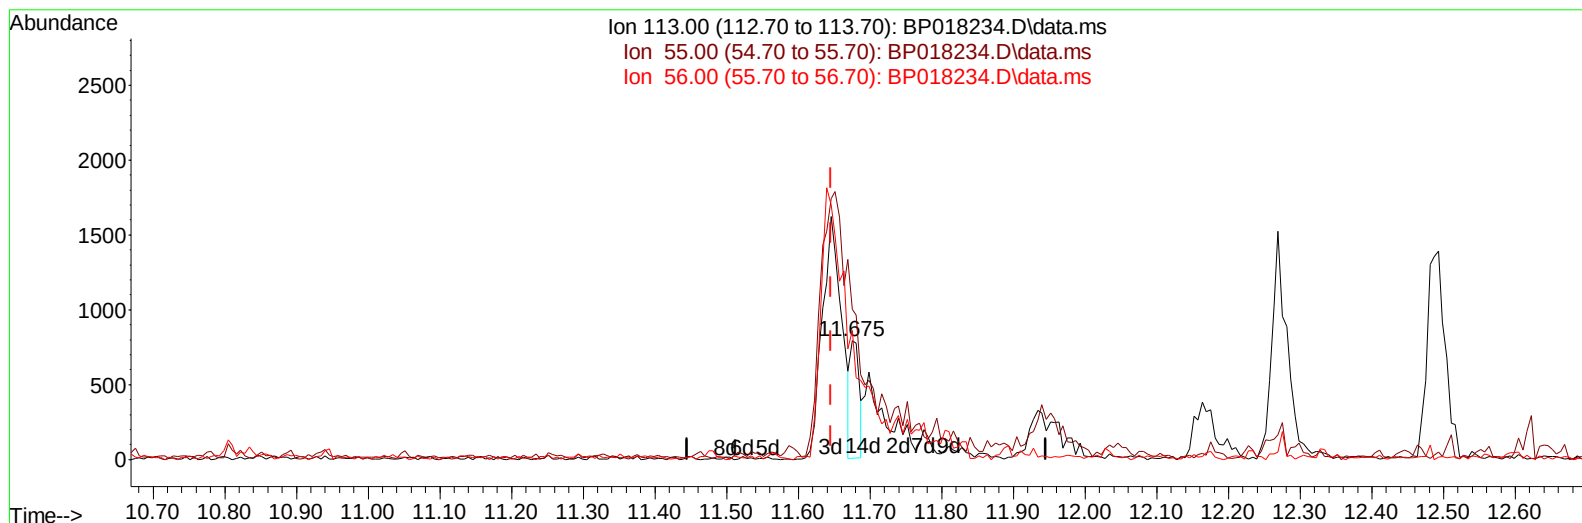

TIC: BP018234.D\data.ms

(34) Caprolactam

11.675min (+ 0.030) 0.63 ng/ul

response 682

Ion	Exp%	Act%
113.00	100.00	100.00
55.00	147.90	126.32
56.00	119.50	108.82
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
 Data File : BP018234.D
 Acq On : 17 Nov 2023 23:05
 Operator : MA/JU
 Sample : 05369-18MSD
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCDP3MSD

Manual IntegrationsAPPROVED

Quant Time: Nov 17 23:41:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 15 18:13:37 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
 Supervised By :mohammad ahmed 11/19/2023

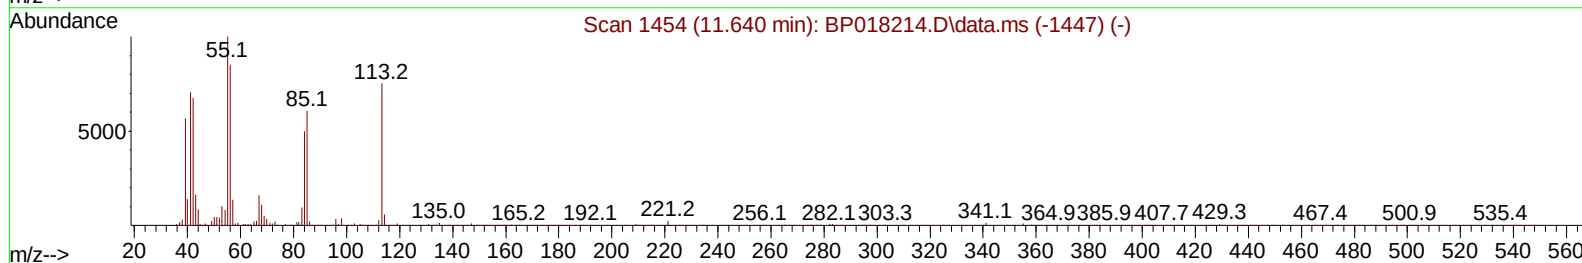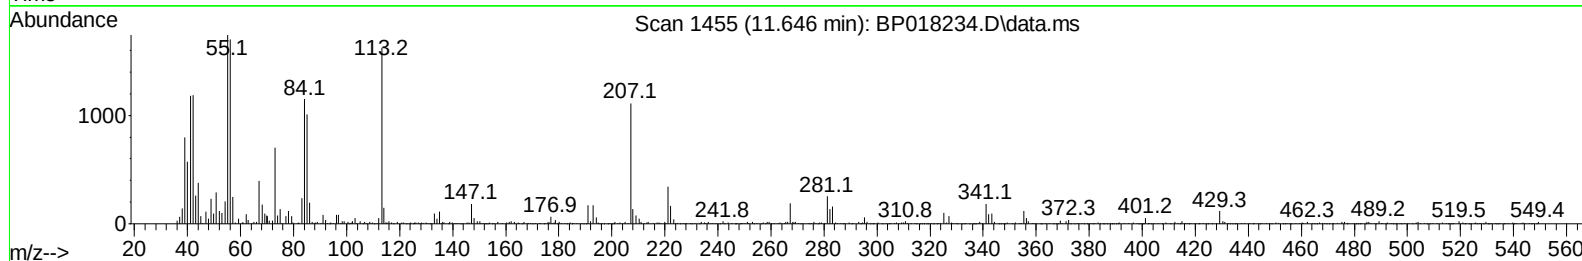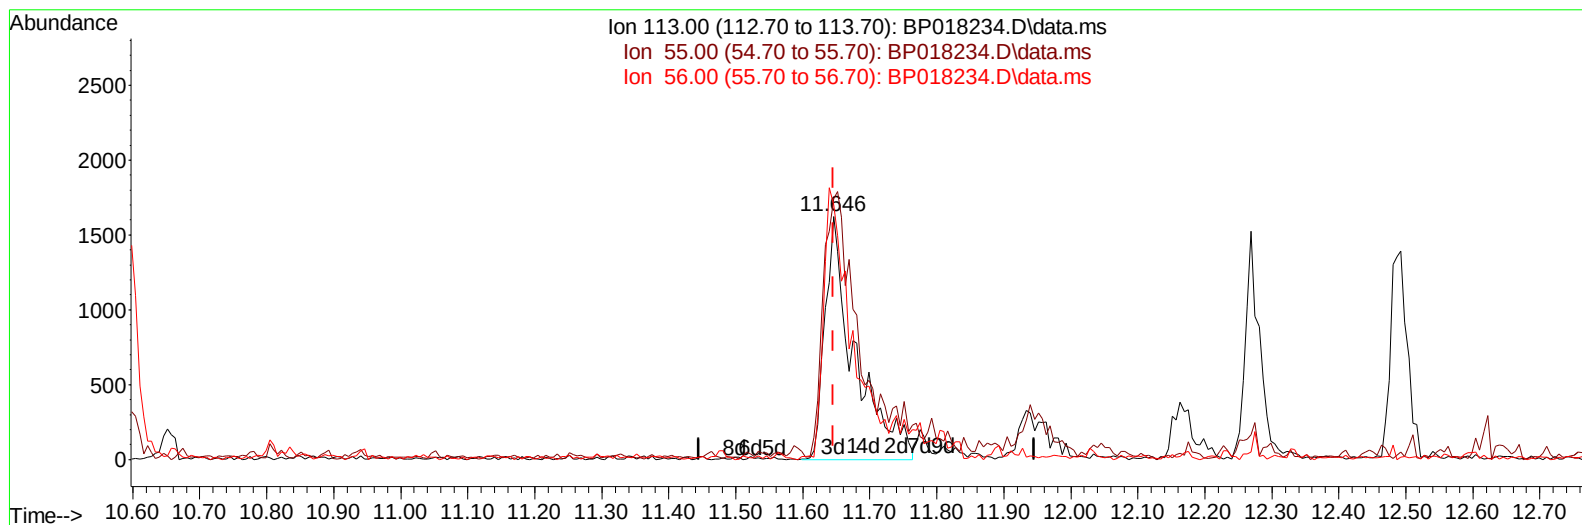

TIC: BP018234.D\data.ms

(34) Caprolactam

11.646min (+ 0.000) 4.63 ng/ul m

response 4989

Ion	Exp%	Act%
113.00	100.00	100.00
55.00	147.90	107.26#
56.00	119.50	104.68
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
Data File : BP018234.D
Acq On : 17 Nov 2023 23:05
Operator : MA/JU
Sample : 05369-18MSD
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCDP3MSD

Manual IntegrationsAPPROVED

Quant Time: Nov 17 23:41:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 15 18:13:37 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
Supervised By :mohammad ahmed 11/19/2023

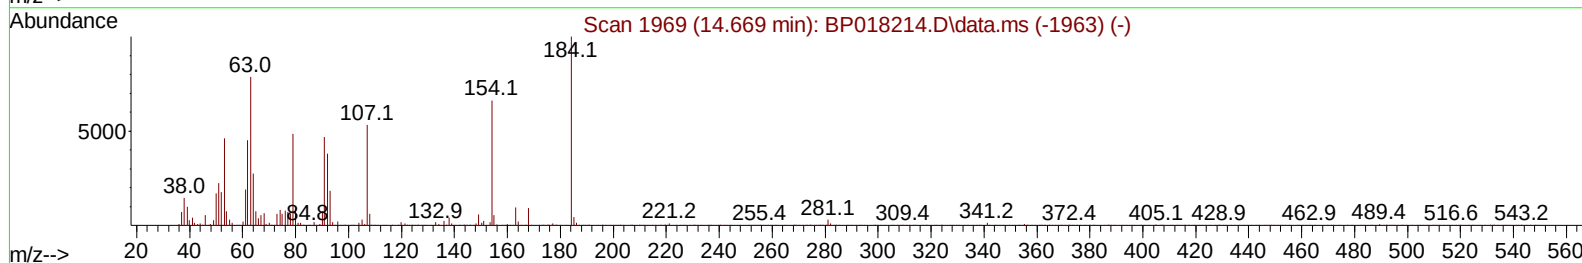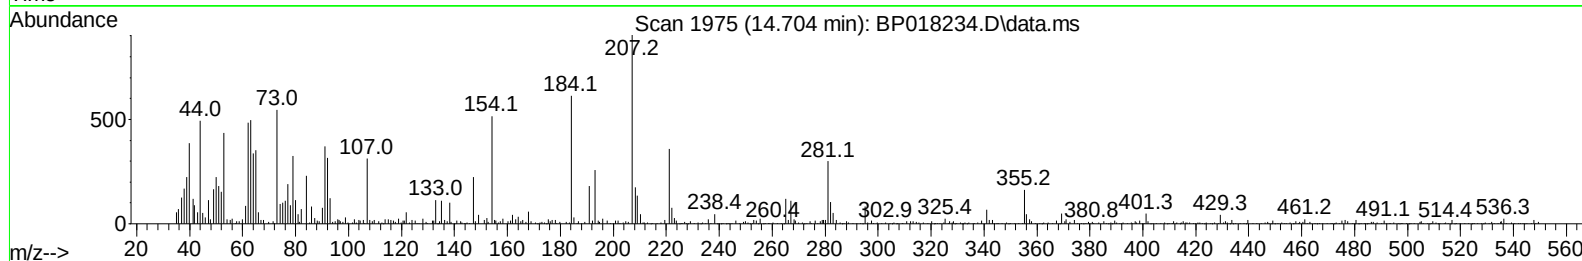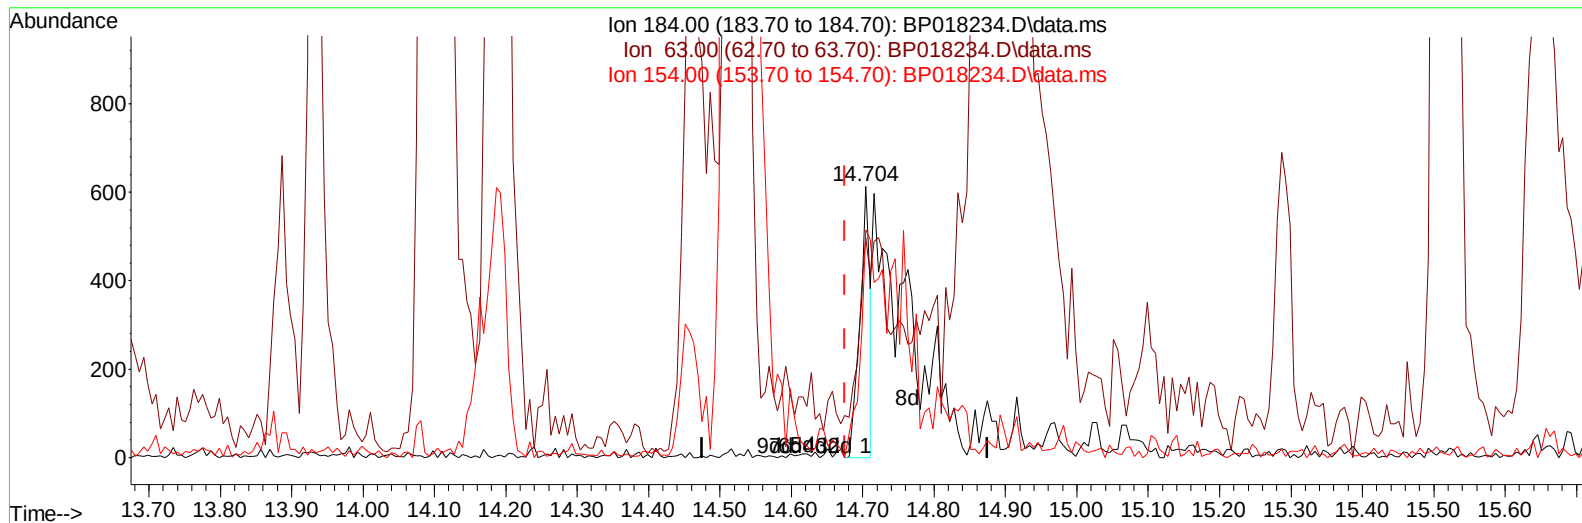

TIC: BP018234.D\data.ms

(53) 2,4-Dinitrophenol

14.704min (+ 0.030) 0.54 ng/ul

response 595

Ion	Exp%	Act%
184.00	100.00	100.00
63.00	84.60	80.94
154.00	75.30	83.88
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
Data File : BP018234.D
Acq On : 17 Nov 2023 23:05
Operator : MA/JU
Sample : 05369-18MSD
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCDP3MSD

Manual IntegrationsAPPROVED

Quant Time: Nov 17 23:41:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 15 18:13:37 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
Supervised By :mohammad ahmed 11/19/2023

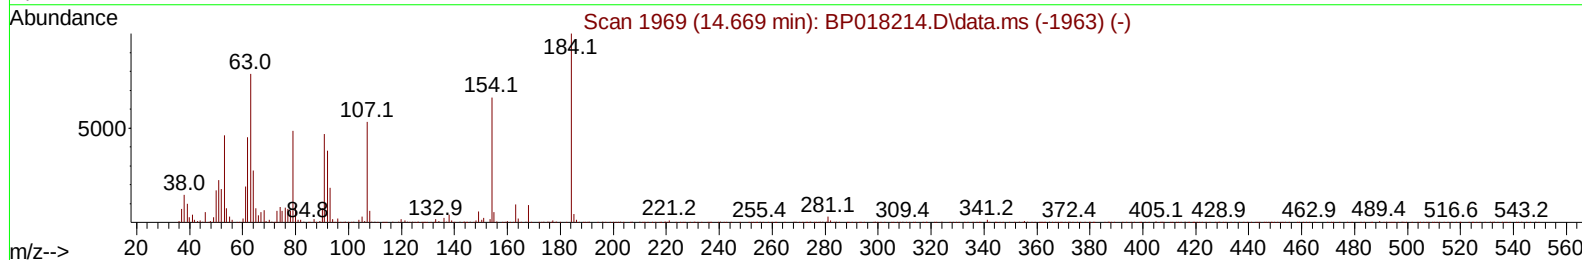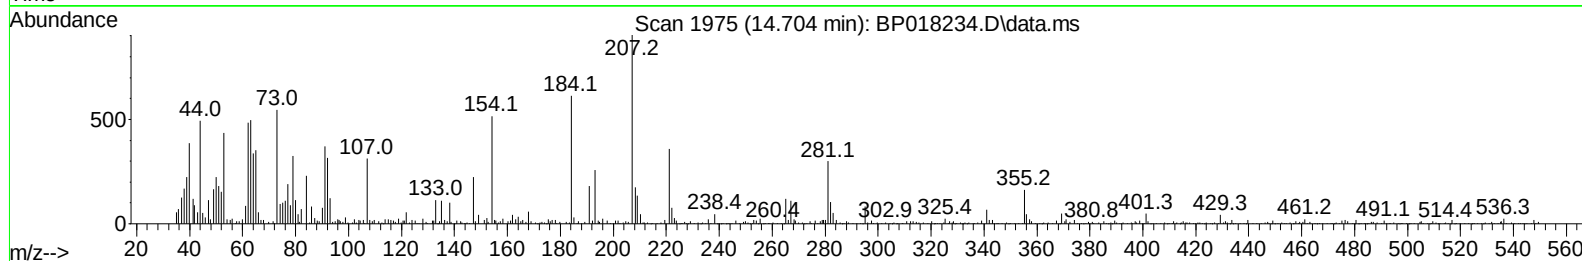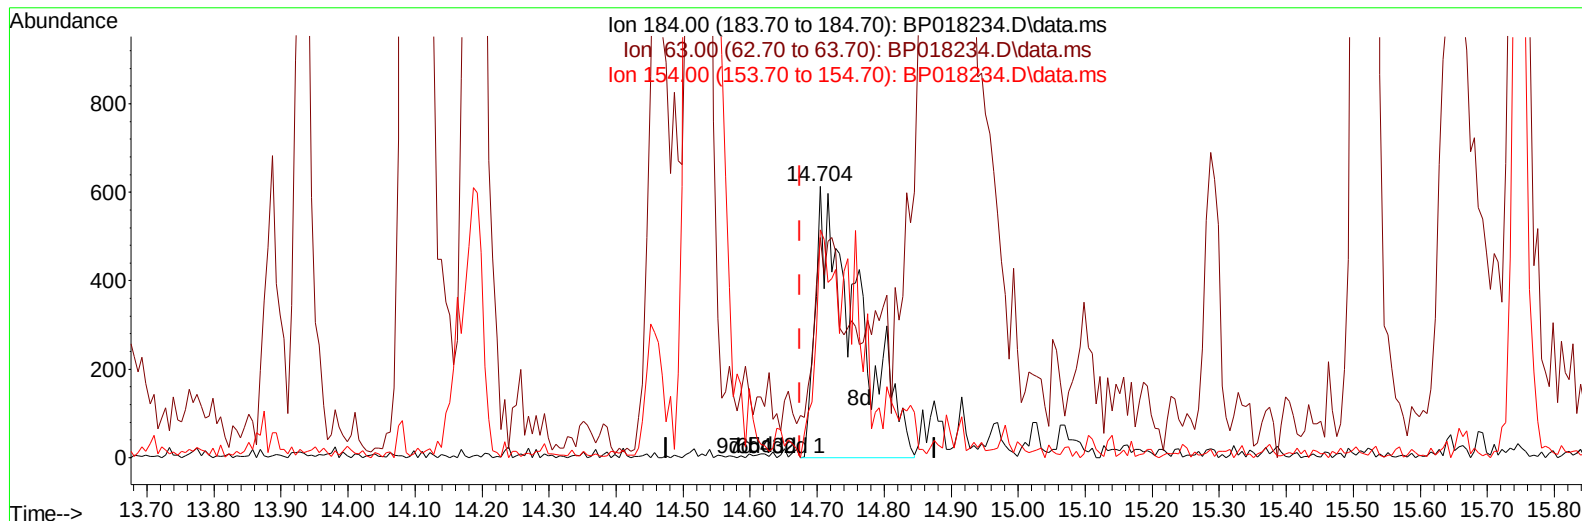

TIC: BP018234.D\data.ms

(53) 2,4-Dinitrophenol

14.704min (+ 0.030) 2.42 ng/ul m

response 2681

Ion	Exp%	Act%
184.00	100.00	100.00
63.00	84.60	80.94
154.00	75.30	83.88
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
 Data File : BP018234.D
 Acq On : 17 Nov 2023 23:05
 Operator : MA/JU
 Sample : 05369-18MSD
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCDP3MSD

Manual IntegrationsAPPROVED

Quant Time: Nov 17 23:41:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 15 18:13:37 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
 Supervised By :mohammad ahmed 11/19/2023

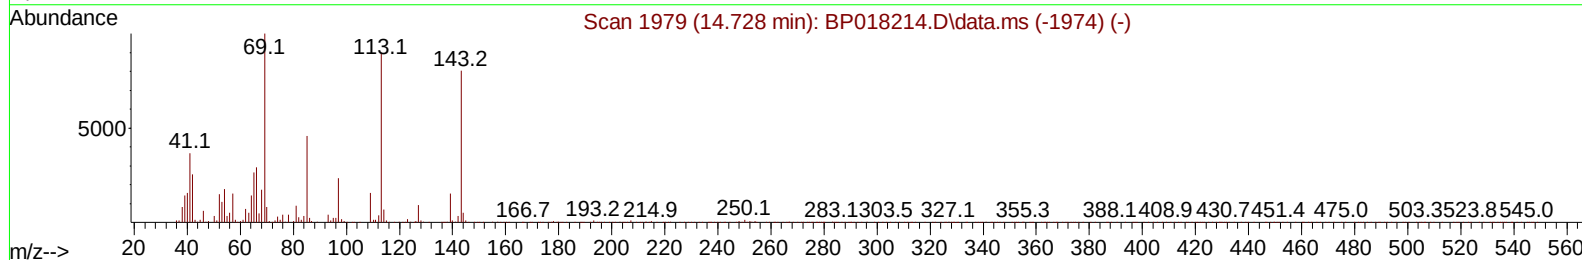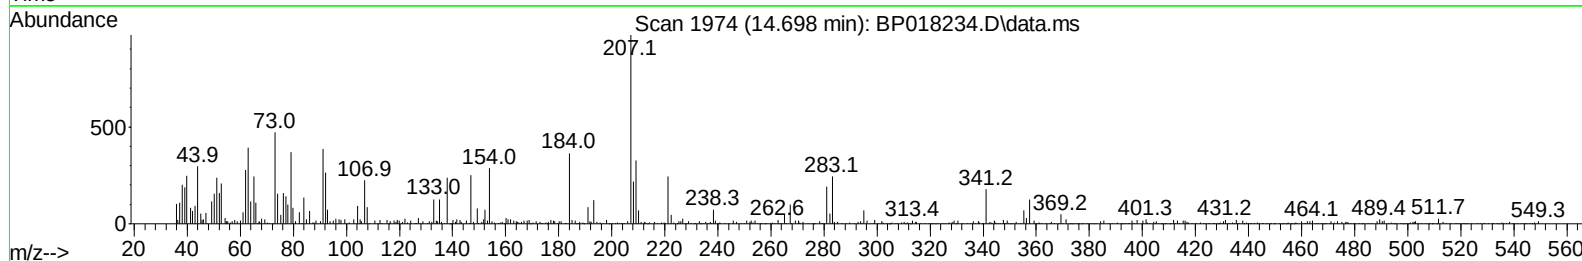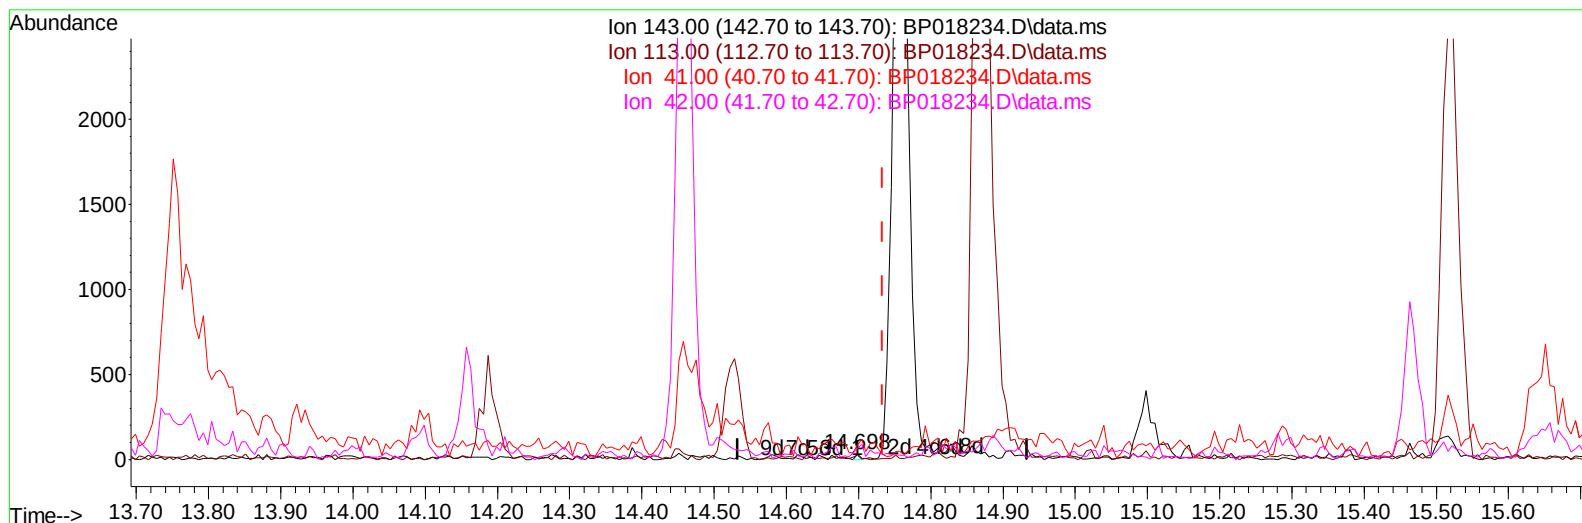

TIC: BP018234.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.698min (-0.035) 0.01 ng/ul

response 13

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.00	81.25#
41.00	47.70	262.50#
42.00	30.10	206.25#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
 Data File : BP018234.D
 Acq On : 17 Nov 2023 23:05
 Operator : MA/JU
 Sample : 05369-18MSD
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCDP3MSD

Manual IntegrationsAPPROVED

Quant Time: Nov 17 23:41:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 15 18:13:37 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
 Supervised By :mohammad ahmed 11/19/2023

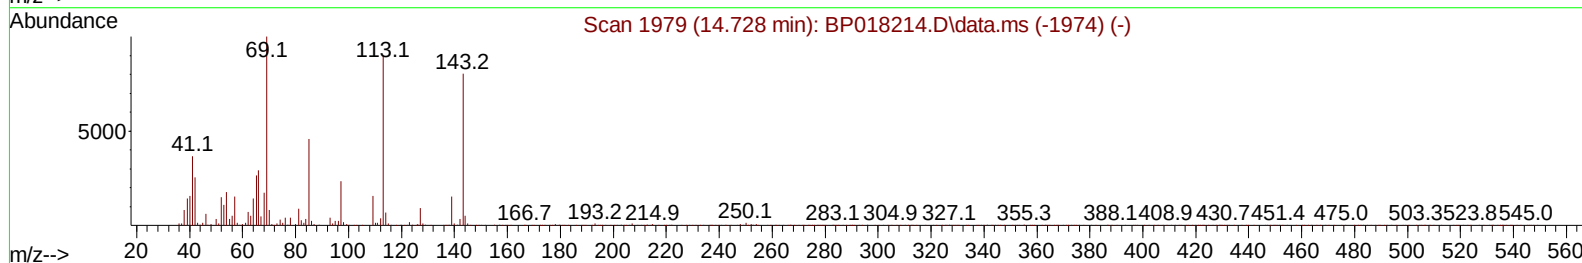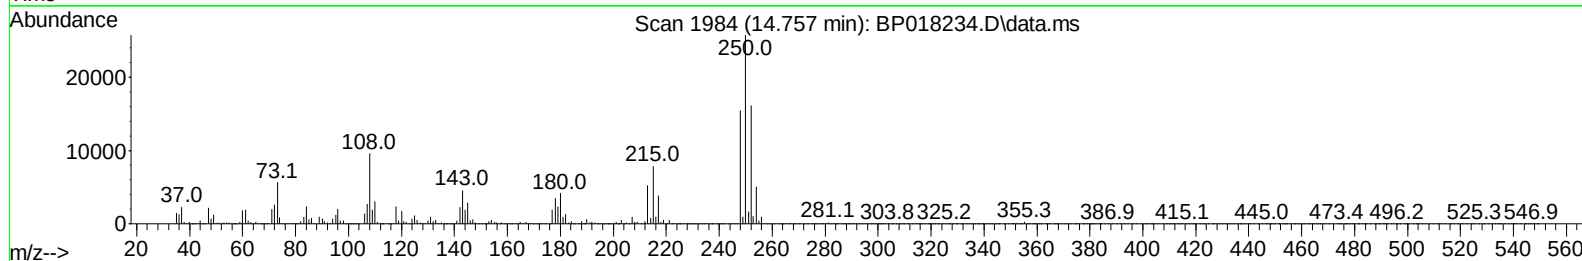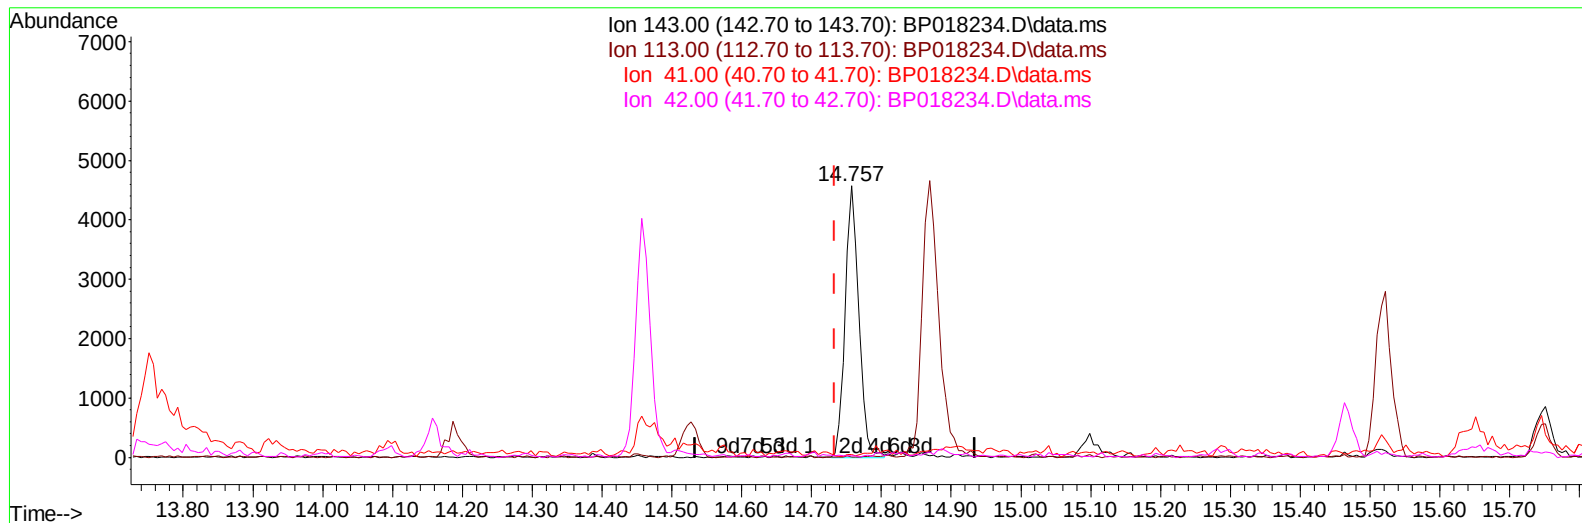

TIC: BP018234.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.757min (+ 0.024) 3.97 ng/ul m

response 6186

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.00	0.09#
41.00	47.70	1.01#
42.00	30.10	0.57#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
 Data File : BP018234.D
 Acq On : 17 Nov 2023 23:05
 Operator : MA/JU
 Sample : 05369-18MSD
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCDP3MSD

Manual IntegrationsAPPROVED

Quant Time: Nov 17 23:41:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 15 18:13:37 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
 Supervised By :mohammad ahmed 11/19/2023

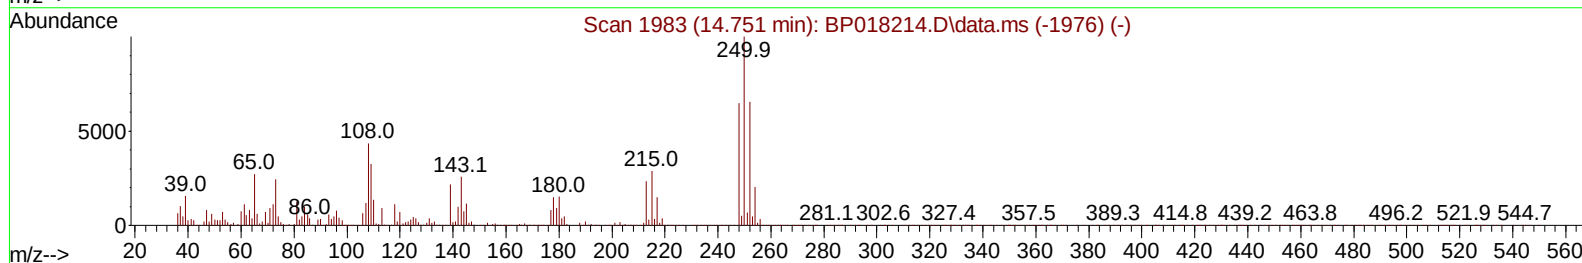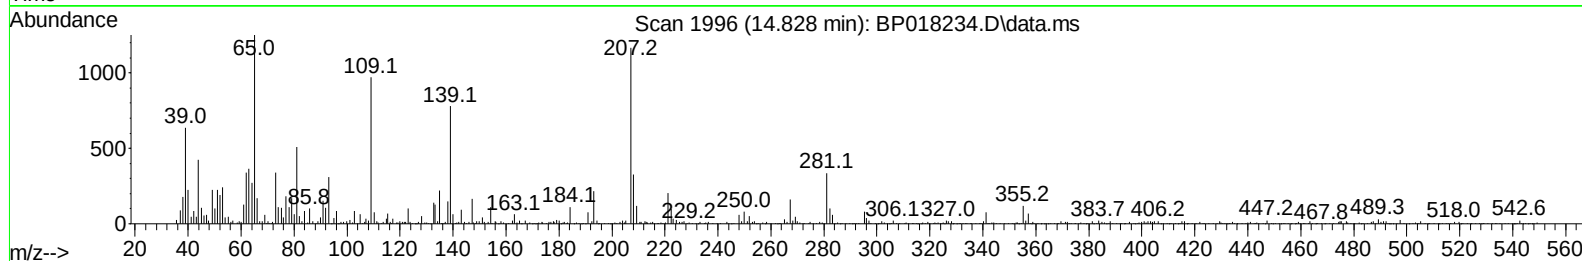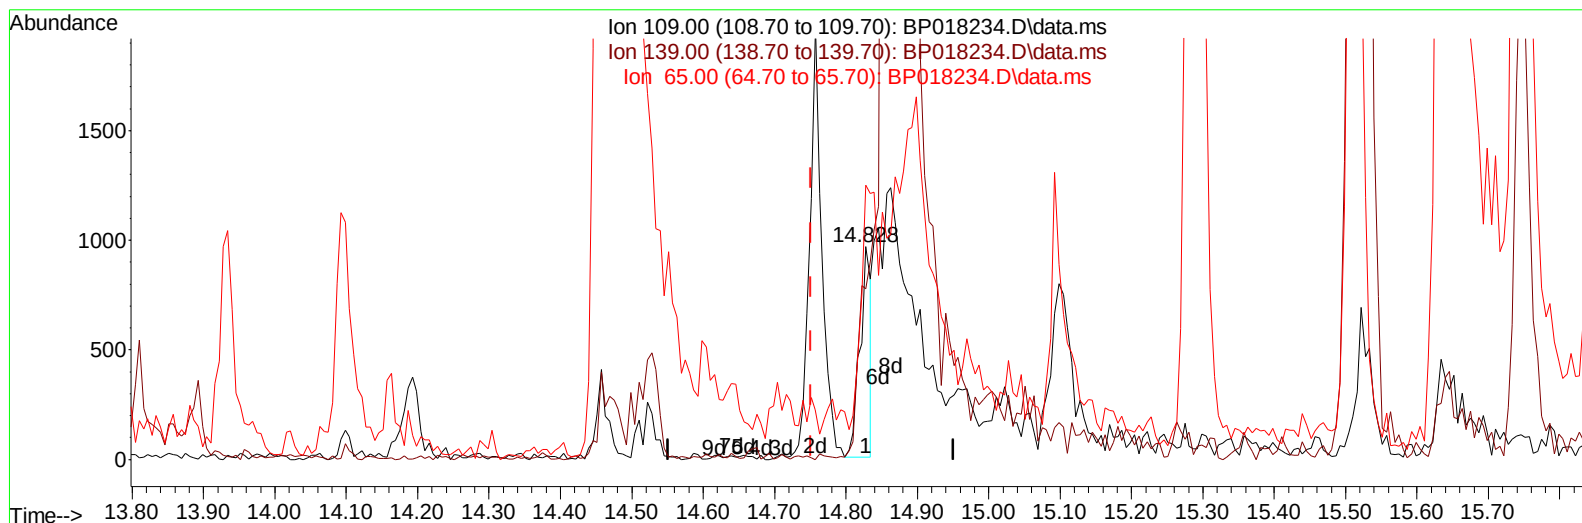

TIC: BP018234.D\data.ms

(55) 4-Nitrophenol

14.828min (+ 0.077) 0.49 ng/ul

response 1020

Ion	Exp%	Act%
109.00	100.00	100.00
139.00	93.60	80.31
65.00	117.20	128.97
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
Data File : BP018234.D
Acq On : 17 Nov 2023 23:05
Operator : MA/JU
Sample : 05369-18MSD
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCDP3MSD

Manual IntegrationsAPPROVED

Quant Time: Nov 17 23:49:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 15 18:13:37 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
Supervised By :mohammad ahmed 11/19/2023

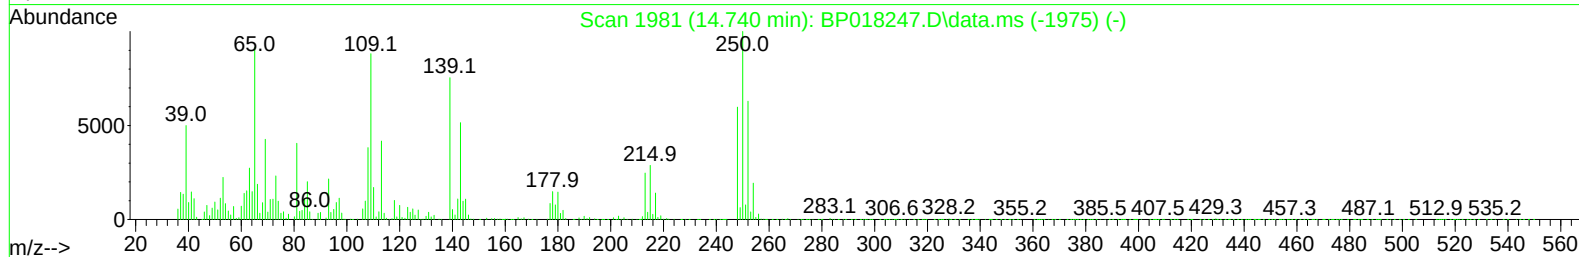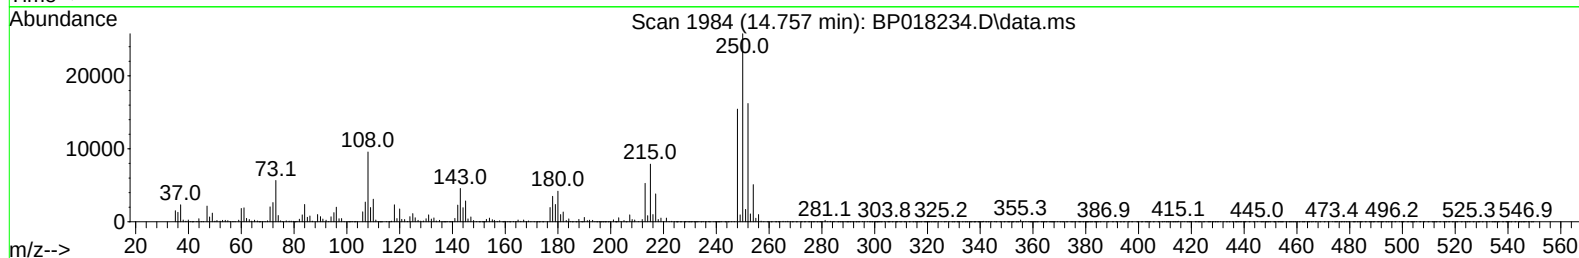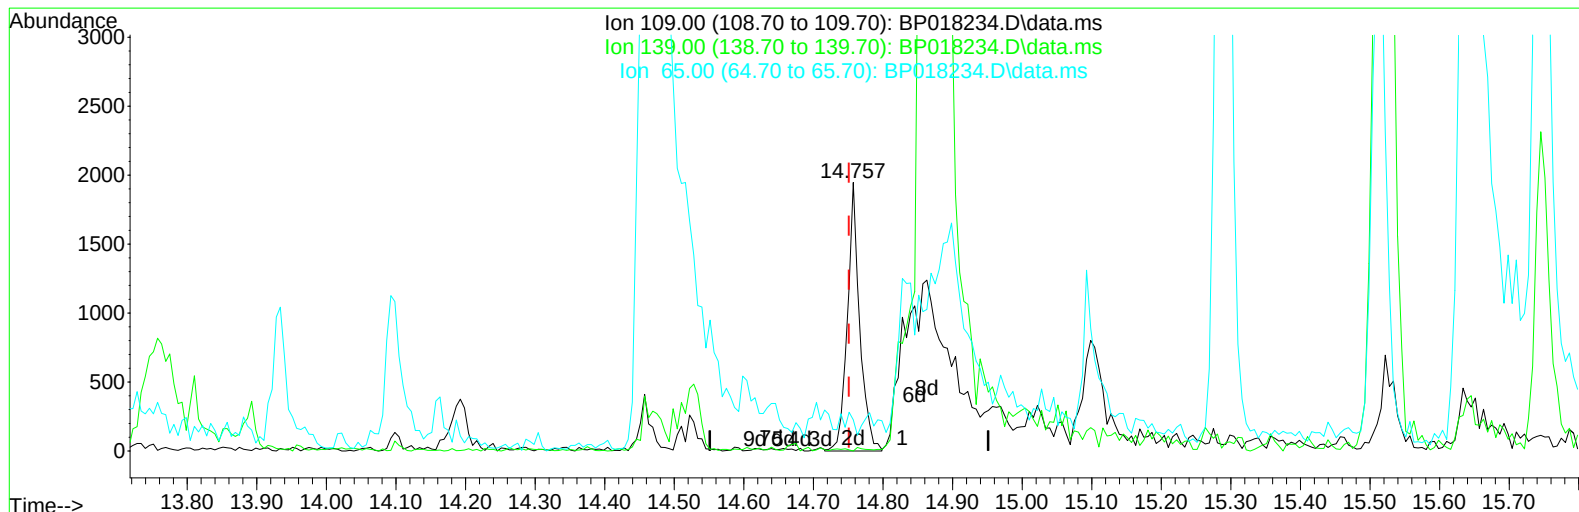

TIC: BP018234.D\data.ms

(55) 4-Nitrophenol

14.757min (+ 0.006) 1.15 ng/u1 m

response 2381

Ion	Exp%	Act%
109.00	100.00	100.00
139.00	93.60	0.00#
65.00	117.20	11.61#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
Data File : BP018234.D
Acq On : 17 Nov 2023 23:05
Operator : MA/JU
Sample : 05369-18MSD
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCDP3MSD

Manual IntegrationsAPPROVED

Quant Time: Nov 17 23:41:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 15 18:13:37 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
Supervised By :mohammad ahmed 11/19/2023

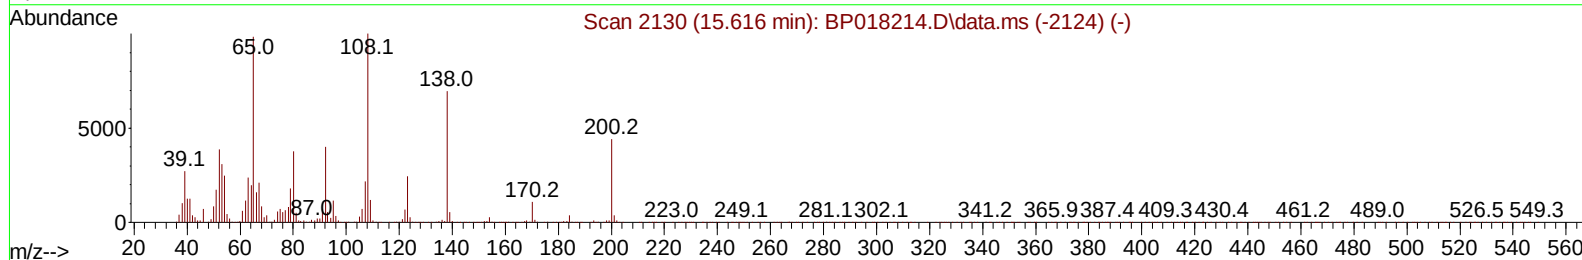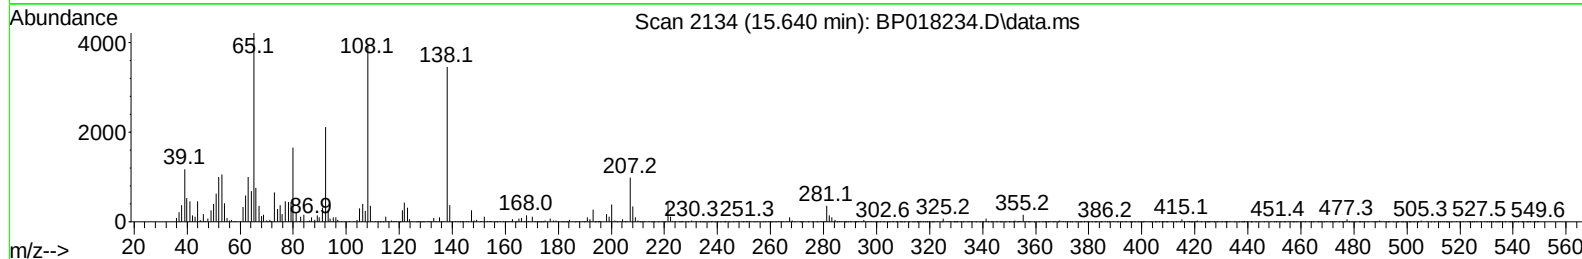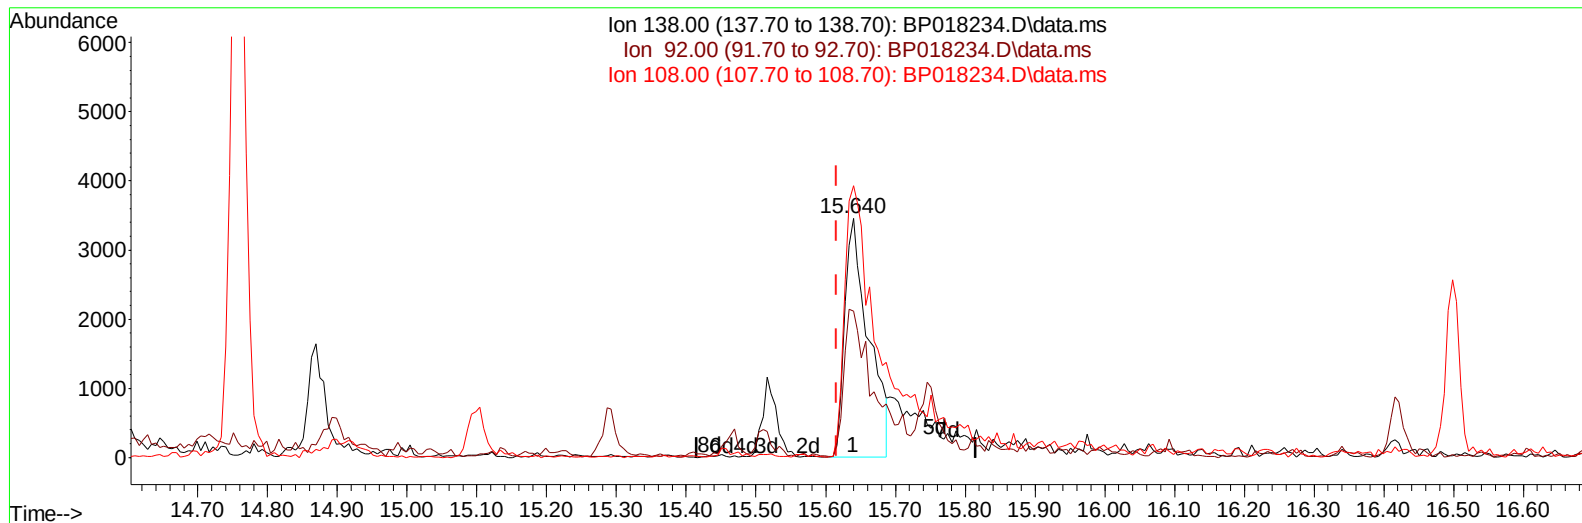

TIC: BP018234.D\data.ms

(63) 4-Nitroaniline

15.640min (+ 0.024) 4.58 ng/ul

response 8147

Ion	Exp%	Act%
138.00	100.00	100.00
92.00	58.30	61.25
108.00	130.90	113.56
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
 Data File : BP018234.D
 Acq On : 17 Nov 2023 23:05
 Operator : MA/JU
 Sample : 05369-18MSD
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCDP3MSD

Manual IntegrationsAPPROVED

Quant Time: Nov 17 23:41:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 15 18:13:37 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
 Supervised By :mohammad ahmed 11/19/2023

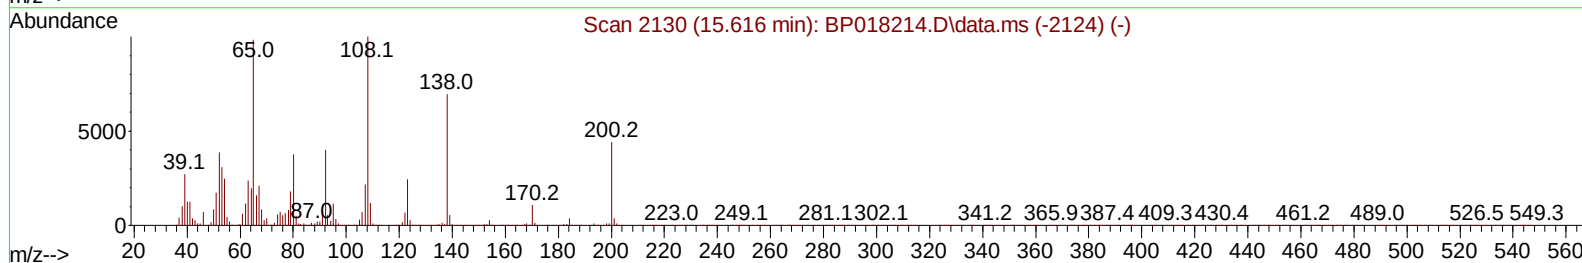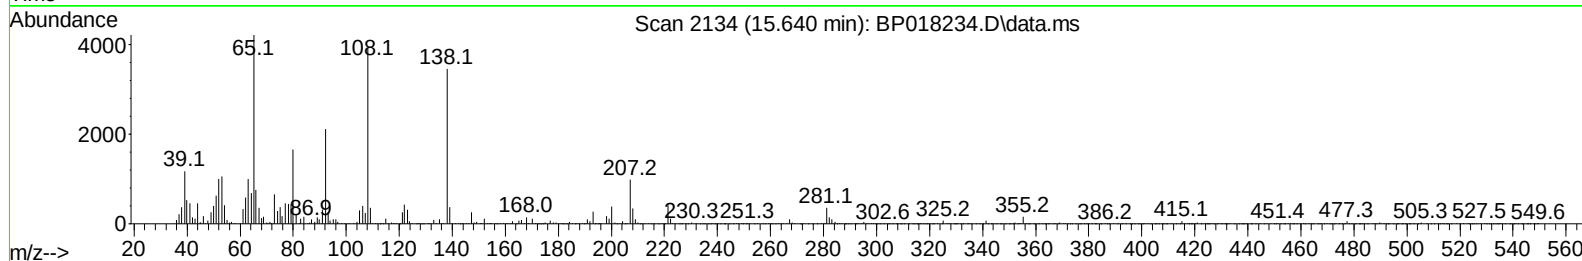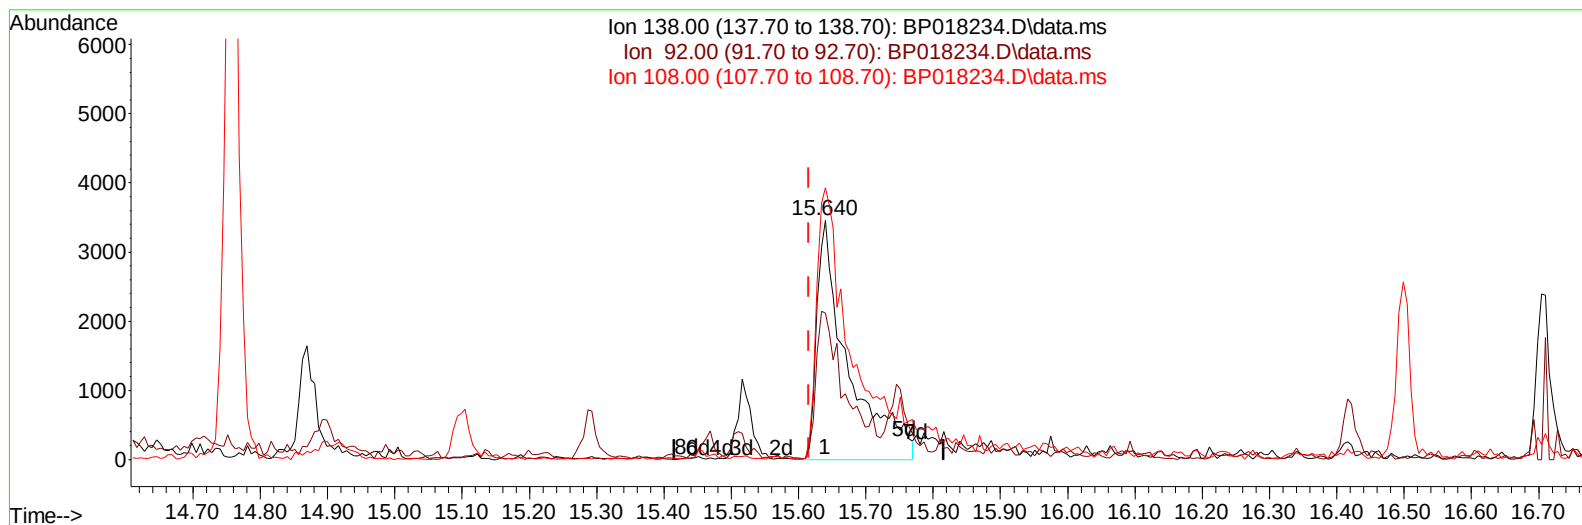

TIC: BP018234.D\data.ms

(63) 4-Nitroaniline

15.640min (+ 0.024) 6.25 ng/ul m

response 11109

Ion	Exp%	Act%
138.00	100.00	100.00
92.00	58.30	61.25
108.00	130.90	113.56
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
 Data File : BP018234.D
 Acq On : 17 Nov 2023 23:05
 Operator : MA/JU
 Sample : 05369-18MSD
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCDP3MSD

Manual IntegrationsAPPROVED

Quant Time: Nov 17 23:41:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 15 18:13:37 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
 Supervised By :mohammad ahmed 11/19/2023

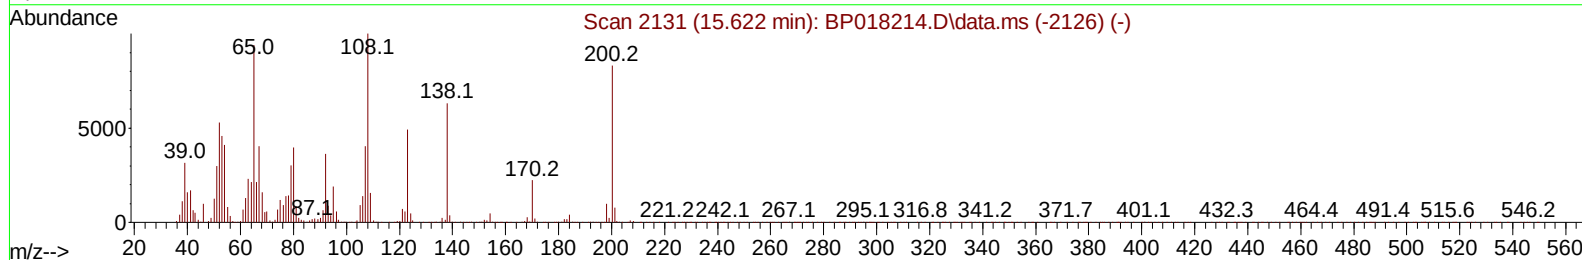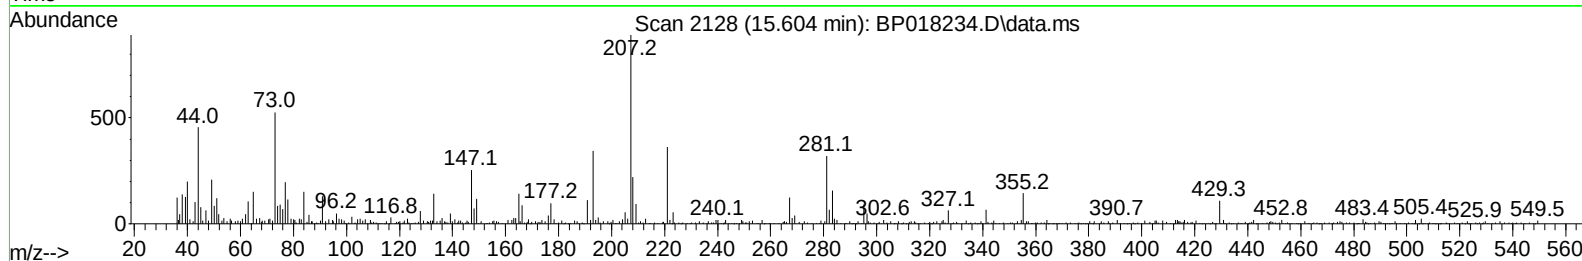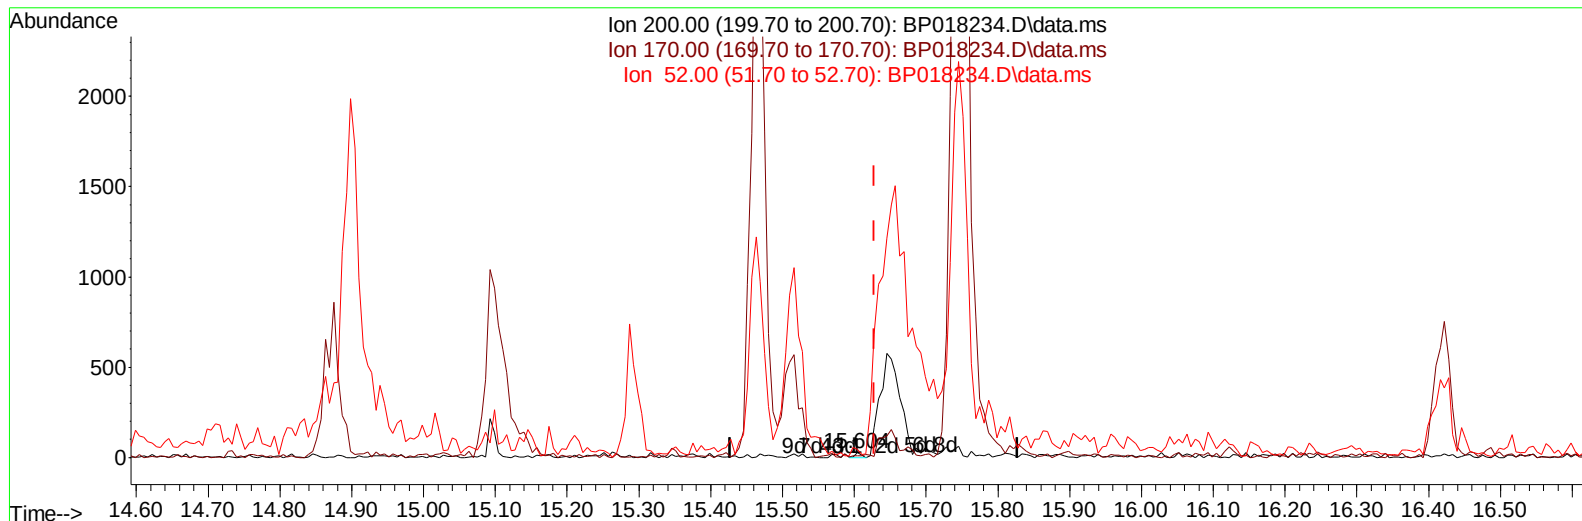

TIC: BP018234.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.604min (-0.023) 0.01 ng/ul

response 15

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	23.60	33.33#
52.00	52.00	170.37#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
Data File : BP018234.D
Acq On : 17 Nov 2023 23:05
Operator : MA/JU
Sample : 05369-18MSD
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCDP3MSD

Manual IntegrationsAPPROVED

Quant Time: Nov 17 23:41:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 15 18:13:37 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
Supervised By :mohammad ahmed 11/19/2023

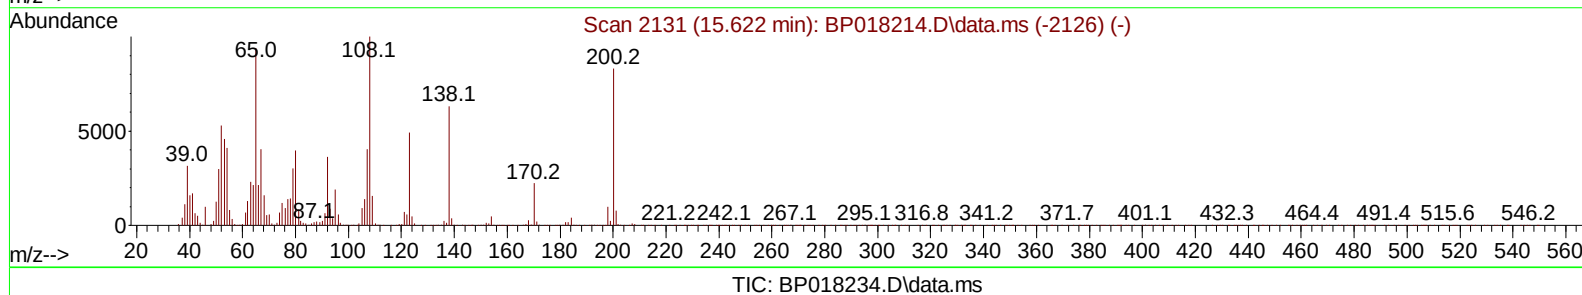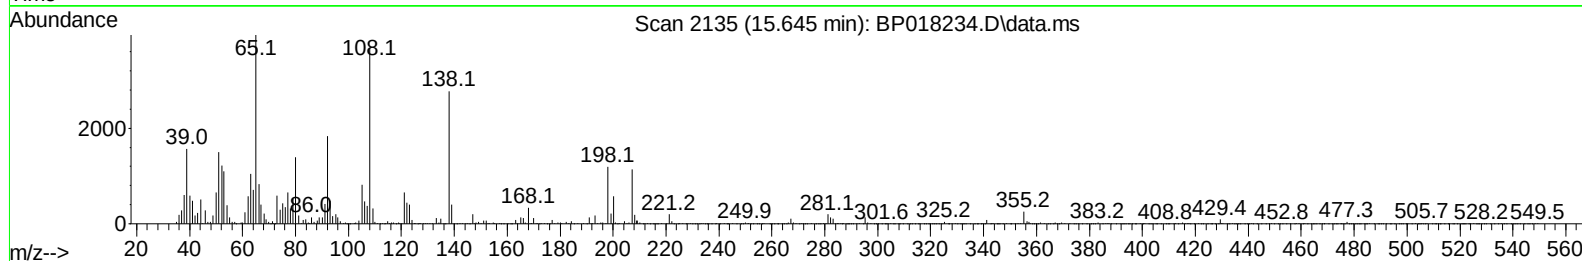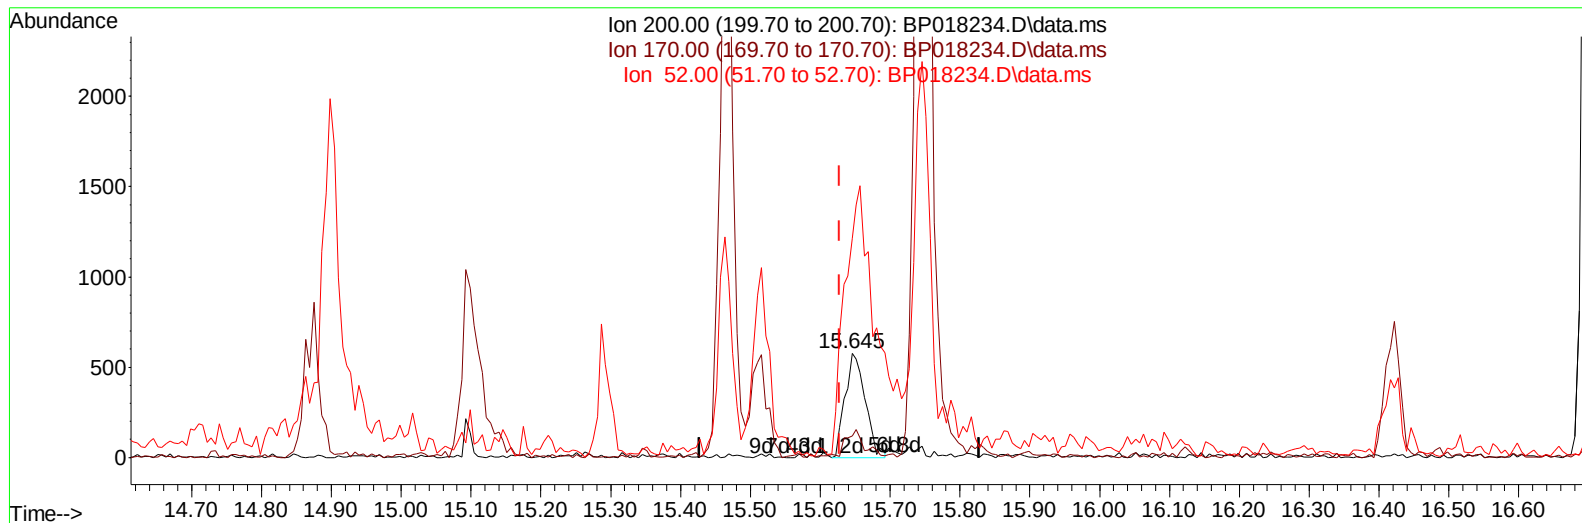

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.645min (+ 0.018) 0.61 ng/ul m

response 1156

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	23.60	20.45
52.00	52.00	210.75#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
 Data File : BP018234.D
 Acq On : 17 Nov 2023 23:05
 Operator : MA/JU
 Sample : 05369-18MSD
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCDP3MSD

Manual IntegrationsAPPROVED

Quant Time: Nov 17 23:49:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 15 18:13:37 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
 Supervised By :mohammad ahmed 11/19/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.781	152	48298	20.000	ng/ul	0.00
20) Naphthalene-d8	10.599	136	186887	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.457	164	112876	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.239	188	261015	20.000	ng/ul	0.00
79) Chrysene-d12	21.375	240	261355	20.000	ng/ul	0.00
88) Perylene-d12	23.851	264	296118	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.158	96	4427	3.233	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	6.975	99	1744	0.374	ng/ul	0.02
9) Bis-(2-Chloroethyl)eth...	7.140	67	8709	3.178	ng/ul	0.00
11) 2-Chlorophenol-d4	7.316	132	5665	1.534	ng/ul	0.01
15) 4-Methylphenol-d8	8.528	113	3943m	1.032	ng/ul	0.02
21) Nitrobenzene-d5	8.999	128	4693	2.787	ng/ul	0.00
24) 2-Nitrophenol-d4	9.716	143	3182	1.668	ng/ul	0.01
28) 2,4-Dichlorophenol-d3	10.263	165	7667m	2.255	ng/ul	0.04
31) 4-Chloroaniline-d4	10.810	131	11267m	2.417	ng/ul	0.02
46) Dimethylphthalate-d6	13.887	166	33414	3.208	ng/ul	0.00
49) Acenaphthylene-d8	14.163	160	38511	3.395	ng/ul	0.00
54) 4-Nitrophenol-d4	14.757	143	6186m	3.975	ng/ul	0.02
60) Fluorene-d10	15.463	176	32068	3.729	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.645	200	1156m	0.613	ng/ul	0.02
73) Anthracene-d10	17.345	188	49079	3.477	ng/ul	0.00
81) Pyrene-d10	19.604	212	60997	3.494	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.686	264	63127	3.666	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.199	88	4199	2.811	ng/uL	93
6) Benzaldehyde	6.975	77	20264	8.069	ng/ul	95
8) Phenol	7.005	94	18721	4.070	ng/ul	97
10) Bis(2-Chloroethyl)ether	7.234	93	29051	8.141	ng/ul	96
12) 2-Chlorophenol	7.346	128	21408	5.774	ng/ul	96
13) 2-Methylphenol	8.252	108	19493	5.609	ng/ul	95
14) 2,2'-oxybis(1-Chloropr...	8.299	45	36175m	8.878	ng/ul	
16) Acetophenone	8.646	105	46176	7.603	ng/ul	95
17) N-Nitroso-di-n-propyla...	8.605	70	25072	7.561	ng/ul	98
18) 4-Methylphenol	8.599	108	18350	4.841	ng/ul	93
19) Hexachloroethane	8.828	117	15371	8.666	ng/ul	92
22) Nitrobenzene	9.040	77	36241	7.971	ng/ul	98
23) Isophorone	9.534	82	66009	7.957	ng/ul	98
25) 2-Nitrophenol	9.746	139	12077	6.161	ng/ul	96
26) 2,4-Dimethylphenol	9.787	107	28673	6.876	ng/ul	96
27) Bis(2-Chloroethoxy)met...	10.034	93	36505	8.069	ng/ul	99
29) 2,4-Dichlorophenol	10.281	162	15004	4.622	ng/ul	96
30) Naphthalene	10.646	128	99076	8.717	ng/ul	99
32) 4-Chloroaniline	10.834	127	23251m	5.206	ng/ul	
33) Hexachlorobutadiene	10.857	225	21709	9.109	ng/ul	97
34) Caprolactam	11.646	113	4989m	4.626	ng/ul	
35) 4-Chloro-3-methylphenol	11.934	107	22765	5.828	ng/ul	93
36) 2-Methylnaphthalene	12.269	142	66055	8.466	ng/ul	96

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
 Data File : BP018234.D
 Acq On : 17 Nov 2023 23:05
 Operator : MA/JU
 Sample : 05369-18MSD
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :

BNA_P

ClientSampleId :

GCDP3MSD

Manual IntegrationsAPPROVED

Quant Time: Nov 17 23:49:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 15 18:13:37 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
 Supervised By :mohammad ahmed 11/19/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.487	142	65304	8.145	ng/ul	97
39) 1,2,4,5-Tetrachloroben...	12.628	216	37260	9.771	ng/ul	94
40) Hexachlorocyclopentadiene	12.551	237	7474	4.061	ng/ul	97
41) 2,4,6-Trichlorophenol	12.904	196	16551	6.617	ng/ul	99
42) 2,4,5-Trichlorophenol	12.993	196	17188	6.529	ng/ul	96
43) 1,1'-Biphenyl	13.287	154	88854	9.257	ng/ul	98
44) 2-Chloronaphthalene	13.340	162	70658	9.272	ng/ul	99
45) 2-Nitroaniline	13.616	65	18094	7.358	ng/ul	96
47) Dimethylphthalate	13.934	163	90256	8.834	ng/ul	99
48) 2,6-Dinitrotoluene	14.093	165	16125	7.941	ng/ul#	89
50) Acenaphthylene	14.187	152	110500	8.628	ng/ul	97
51) 3-Nitroaniline	14.463	138	8670	4.601	ng/ul#	71
52) Acenaphthene	14.528	153	80676	9.500	ng/ul	96
53) 2,4-Dinitrophenol	14.704	184	2681m	2.420	ng/ul	
55) 4-Nitrophenol	14.757	109	2381m	1.153	ng/ul	
56) Dibenzofuran	14.869	168	107891	9.271	ng/ul	90
57) 2,4-Dinitrotoluene	14.898	165	23829	7.854	ng/ul	97
58) 2,3,4,6-Tetrachlorophenol	15.098	232	15039	6.422	ng/ul	96
59) Diethylphthalate	15.293	149	100753	9.440	ng/ul	99
61) Fluorene	15.522	166	90459	9.155	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.516	204	46038	9.508	ng/ul	99
63) 4-Nitroaniline	15.640	138	11109m	6.248	ng/ul	
66) 4,6-Dinitro-2-methylph...	15.663	198	7553	3.857	ng/ul#	89
67) N-Nitrosodiphenylamine	15.745	169	73787	8.815	ng/ul	98
68) 4-Bromophenyl-phenylether	16.422	248	29241	9.940	ng/ul	92
69) Hexachlorobenzene	16.498	284	34895	10.630	ng/ul	93
70) Atrazine	16.704	200	27112	9.285	ng/ul	98
71) Pentachlorophenol	16.887	266	7537	3.782	ng/ul	94
72) Phenanthrene	17.287	178	153159	9.557	ng/ul	98
74) Anthracene	17.381	178	152990	9.354	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.240	216	37751	9.471	ng/uL	97
76) Pentachlorobenzene	14.757	250	36771	9.424	ng/uL	95
77) Carbazole	17.686	167	129401	9.111	ng/ul	97
78) Di-n-butylphthalate	18.186	149	162387	9.011	ng/ul	98
80) Fluoranthene	19.275	202	175955	8.630	ng/ul	97
82) Pyrene	19.633	202	186950	8.751	ng/ul	97
83) Butylbenzylphthalate	20.498	149	82960	9.234	ng/ul	93
84) 3,3'-Dichlorobenzidine	21.310	252	52033	8.333	ng/ul	95
85) Benzo(a)anthracene	21.357	228	203998	9.666	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.239	149	119597	9.655	ng/ul	100
87) Chrysene	21.416	228	197078	9.982	ng/ul	99
89) Di-n-octyl phthalate	22.192	149	201309	9.090	ng/ul	100
90) Benzo(b)fluoranthene	23.080	252	205613	9.757	ng/ul	98
91) Benzo(k)fluoranthene	23.133	252	205202	9.678	ng/ul	99
93) Benzo(a)pyrene	23.733	252	189965	9.545	ng/ul	98
94) Indeno(1,2,3-cd)pyrene	26.474	276	231620	9.704	ng/ul	99
95) Dibenzo(a,h)anthracene	26.498	278	191929	9.766	ng/ul	99
96) Benzo(g,h,i)perylene	27.292	276	188844	9.891	ng/ul	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

