




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
Data File : BP018251.D
Acq On : 18 Nov 2023 09:17
Operator : MA/JU
Sample : 05370-03
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCDP9

Manual IntegrationsAPPROVED

Quant Time: Nov 19 00:49:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 15 18:13:37 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
Supervised By :mohammad ahmed 11/19/2023

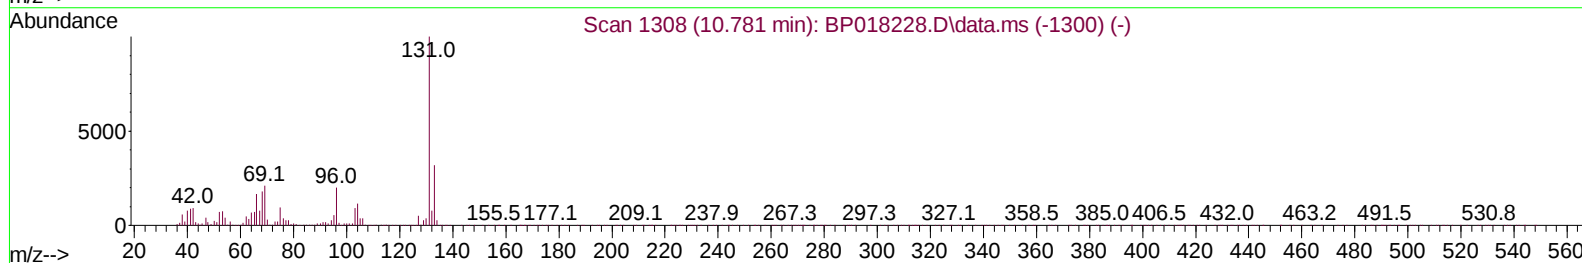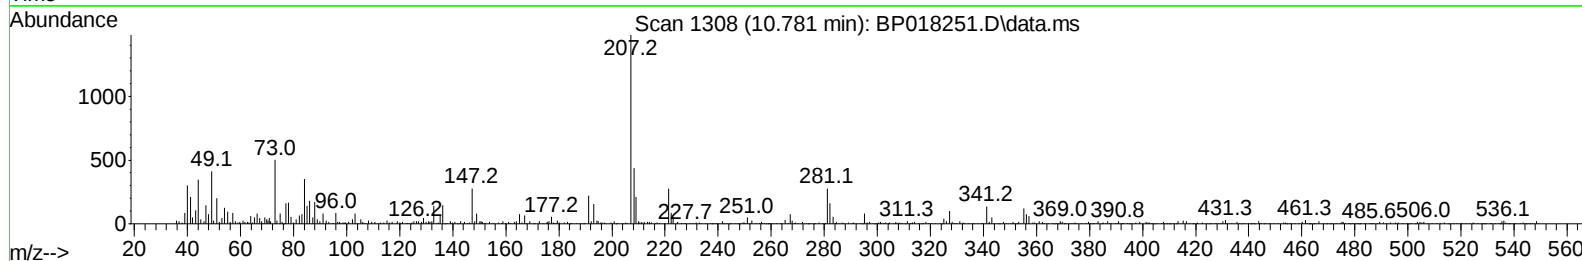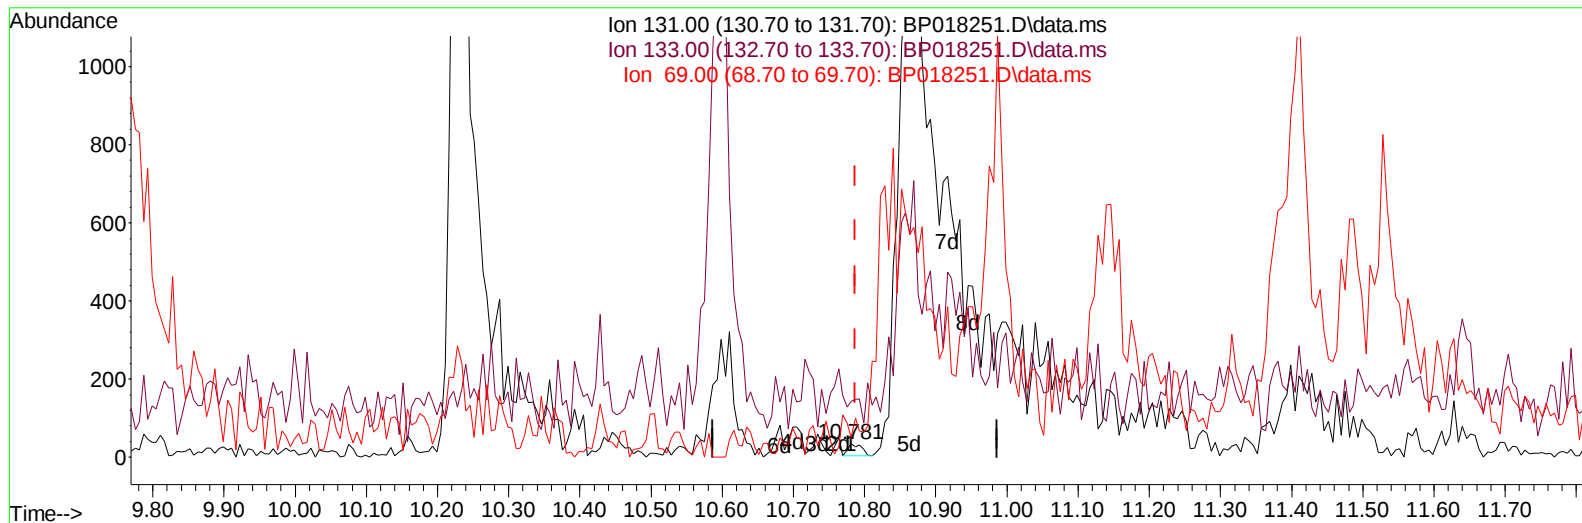

TIC: BP018251.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.781min (-0.006) 0.01 ng/u1

response 40

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.20	408.57#
69.00	20.00	148.57#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
 Data File : BP018251.D
 Acq On : 18 Nov 2023 09:17
 Operator : MA/JU
 Sample : 05370-03
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCDP9

Manual IntegrationsAPPROVED

Quant Time: Nov 19 00:49:28 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 15 18:13:37 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
 Supervised By :mohammad ahmed 11/19/2023

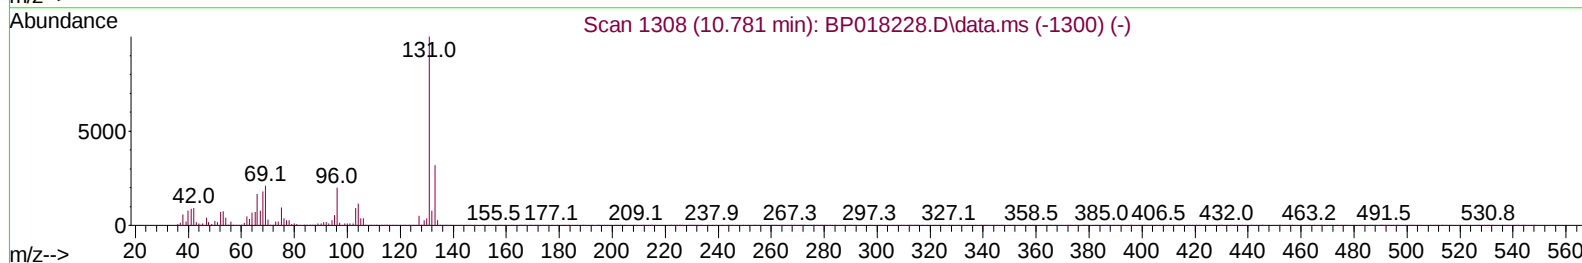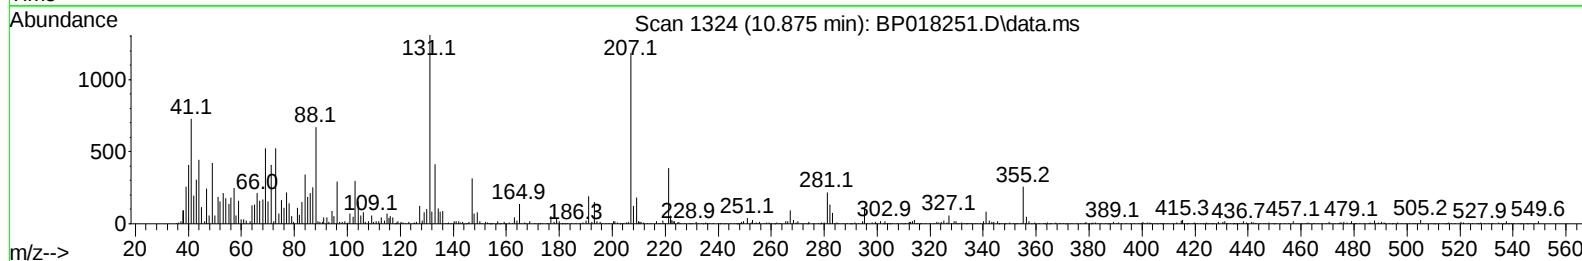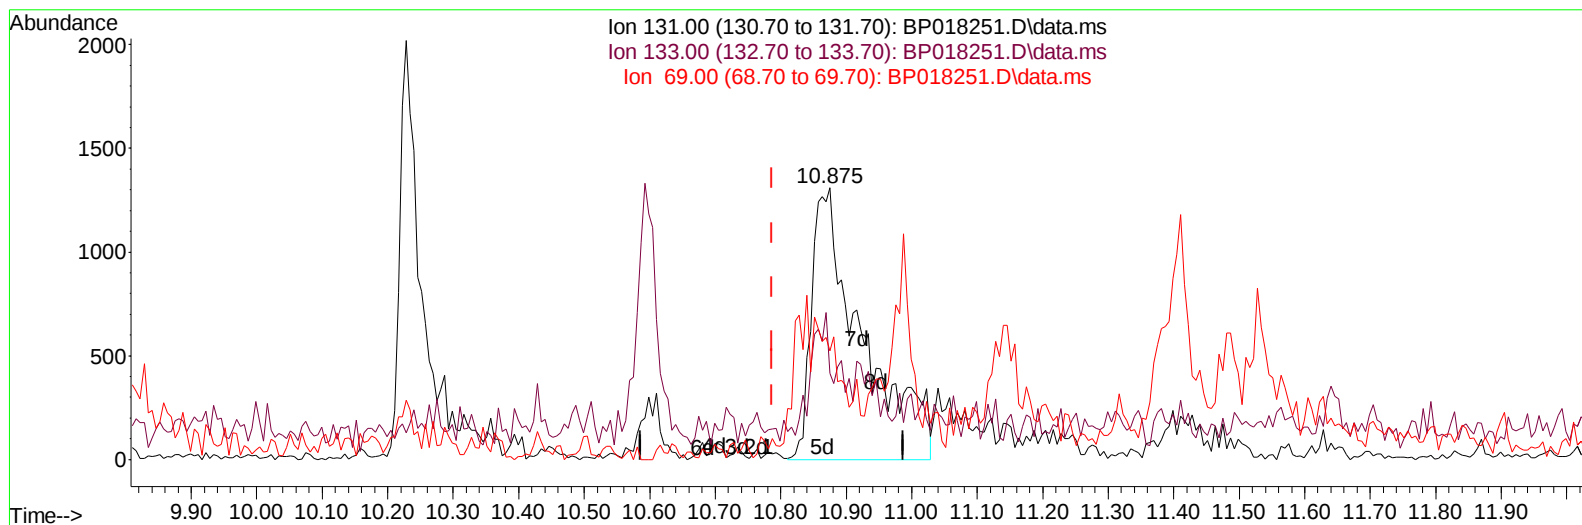

TIC: BP018251.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.875min (+ 0.088) 1.03 ng/ul m

response 6986

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.20	31.70
69.00	20.00	40.03#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
 Data File : BP018251.D
 Acq On : 18 Nov 2023 09:17
 Operator : MA/JU
 Sample : 05370-03
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCDP9

Manual IntegrationsAPPROVED

Quant Time: Nov 19 00:49:28 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 15 18:13:37 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
 Supervised By :mohammad ahmed 11/19/2023

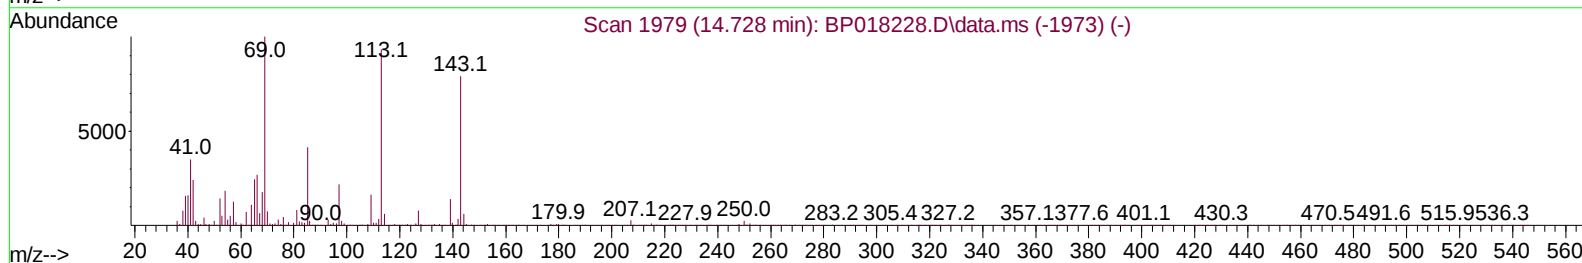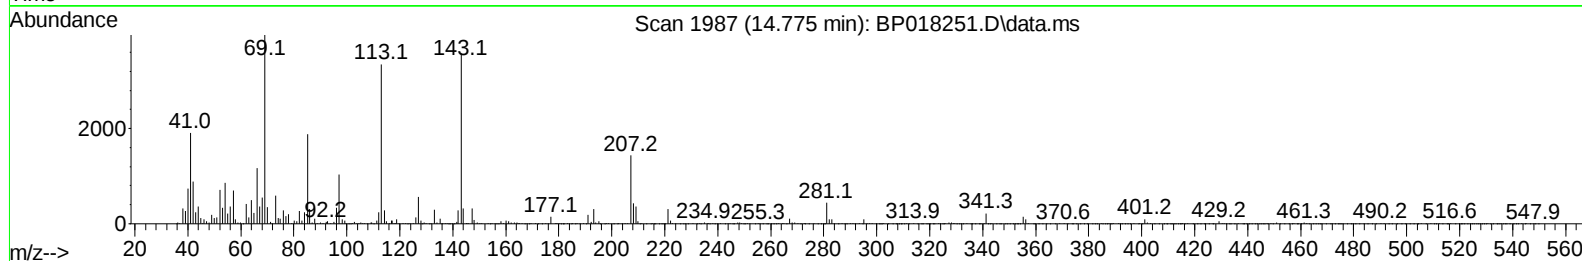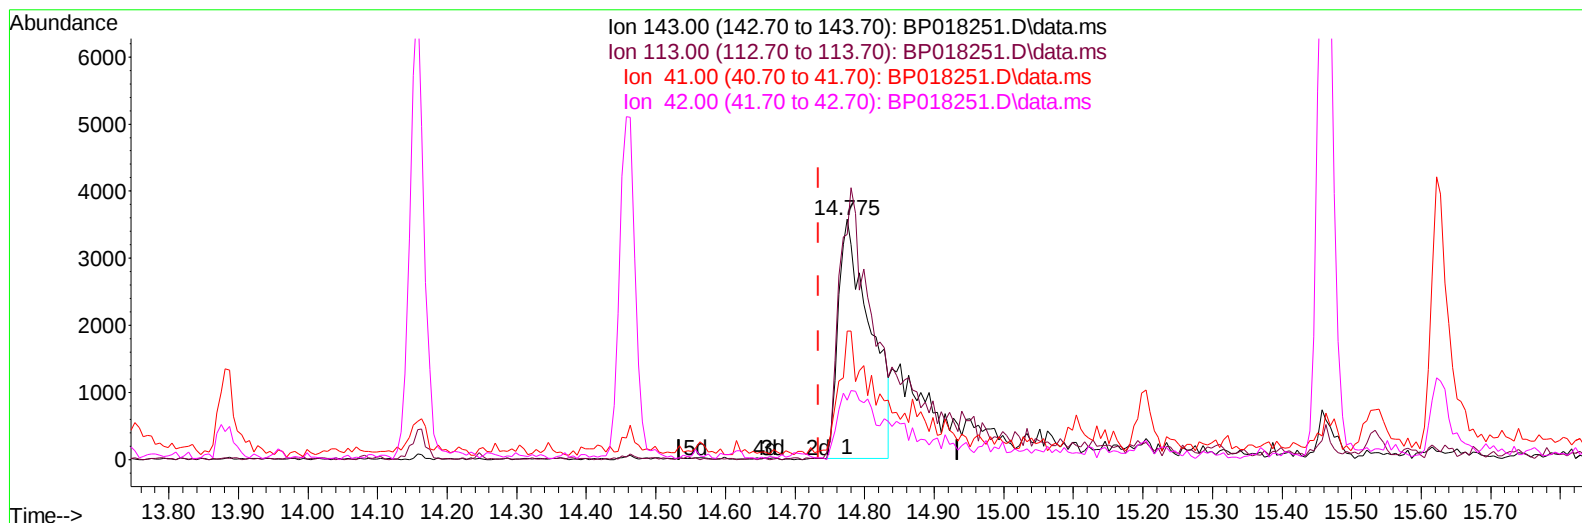

TIC: BP018251.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.775min (+ 0.041) 4.79 ng/ul

response 11166

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.00	93.63
41.00	47.70	53.38
42.00	30.10	24.61




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
Data File : BP018251.D
Acq On : 18 Nov 2023 09:17
Operator : MA/JU
Sample : 05370-03
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCDP9

Manual IntegrationsAPPROVED

Quant Time: Nov 19 00:49:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 15 18:13:37 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
Supervised By :mohammad ahmed 11/19/2023

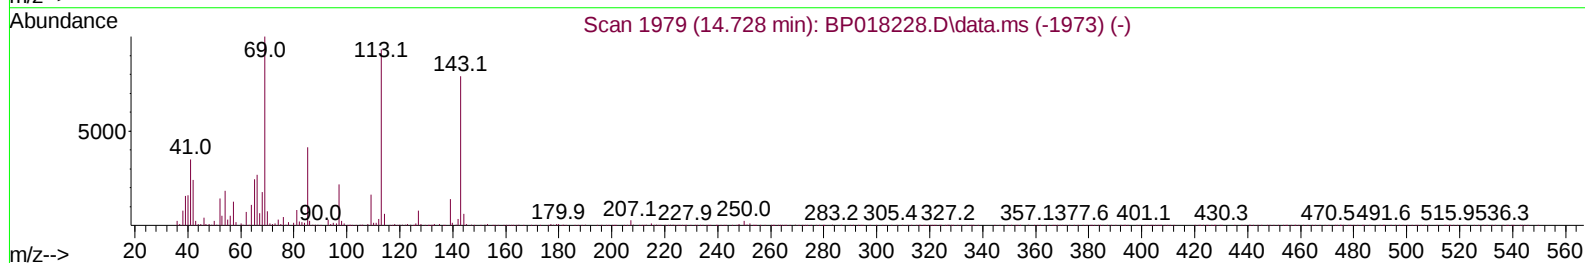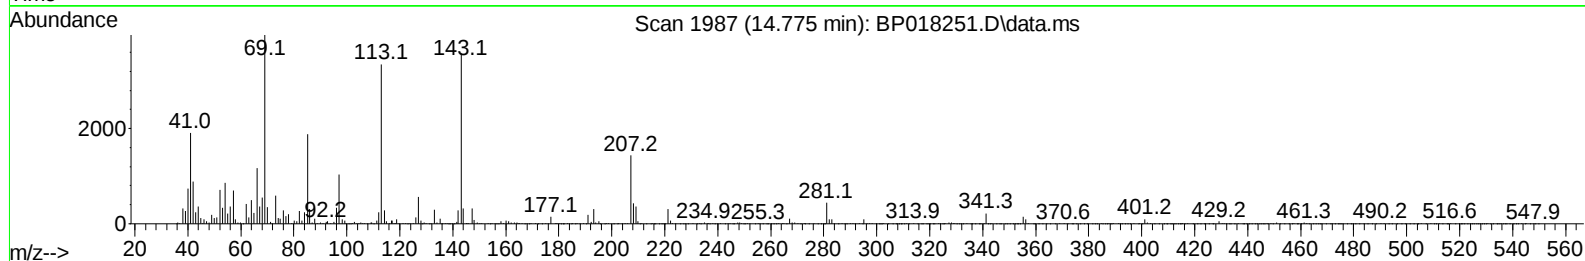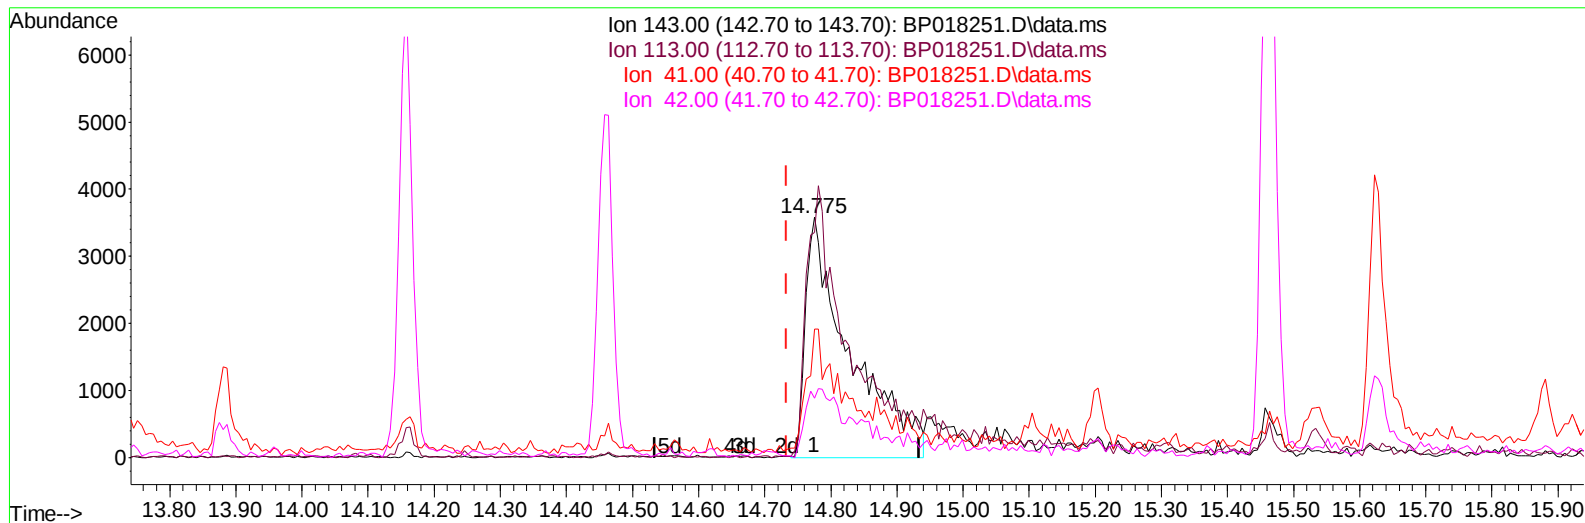

TIC: BP018251.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.775min (+ 0.041) 7.14 ng/ul m

response 16647

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.00	93.63
41.00	47.70	53.38
42.00	30.10	24.61

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
 Data File : BP018251.D
 Acq On : 18 Nov 2023 09:17
 Operator : MA/JU
 Sample : 05370-03
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCDP9

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/19/2023
 Supervised By :mohammad ahmed 11/19/2023

Quant Time: Nov 19 01:24:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 15 18:13:37 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.781	152	69175	20.000	ng/ul	0.00
20) Naphthalene-d8	10.593	136	272312	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.457	164	169096	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.245	188	394402	20.000	ng/ul	0.00
79) Chrysene-d12	21.380	240	417158	20.000	ng/ul	0.00
88) Perylene-d12	23.857	264	483129	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.158	96	7908	4.033	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	6.958	99	56253	8.423	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.128	67	103091	26.267	ng/ul	0.00
11) 2-Chlorophenol-d4	7.299	132	132574	25.068	ng/ul	0.00
15) 4-Methylphenol-d8	8.505	113	94345	17.240	ng/ul	0.00
21) Nitrobenzene-d5	8.987	128	64222	26.177	ng/ul	0.00
24) 2-Nitrophenol-d4	9.699	143	73154	26.320	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.234	165	115265	23.268	ng/ul	0.00
31) 4-Chloroaniline-d4	10.875	131	6986m	1.028	ng/ul	0.09
46) Dimethylphthalate-d6	13.881	166	482045	30.896	ng/ul	0.00
49) Acenaphthylene-d8	14.157	160	485967	28.597	ng/ul	0.00
54) 4-Nitrophenol-d4	14.775	143	16647m	7.140	ng/ul	0.04
60) Fluorene-d10	15.463	176	399946	31.049	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.628	200	68810	24.133	ng/ul	0.00
73) Anthracene-d10	17.345	188	667907	31.312	ng/ul	0.00
81) Pyrene-d10	19.604	212	876684	31.462	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.692	264	892440	31.768	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
Data File : BP018251.D
Acq On : 18 Nov 2023 09:17
Operator : MA/JU
Sample : 05370-03
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCDP9

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/19/2023
Supervised By :mohammad ahmed 11/19/2023

Quant Time: Nov 19 01:24:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 15 18:13:37 2023
Response via : Initial Calibration

