




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
 Data File : BP018253.D
 Acq On : 18 Nov 2023 10:25
 Operator : MA/JU
 Sample : 05370-05
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCDQ1

Manual IntegrationsAPPROVED

Quant Time: Nov 19 00:50:43 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 15 18:13:37 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
 Supervised By :mohammad ahmed 11/19/2023

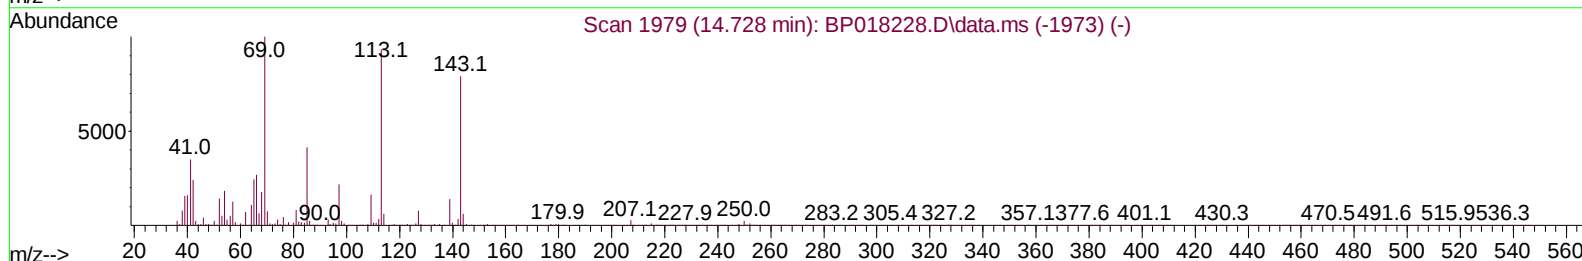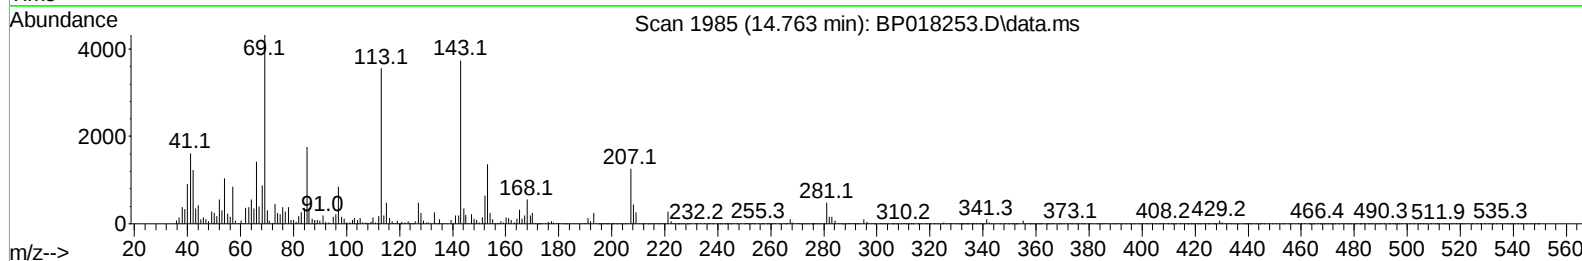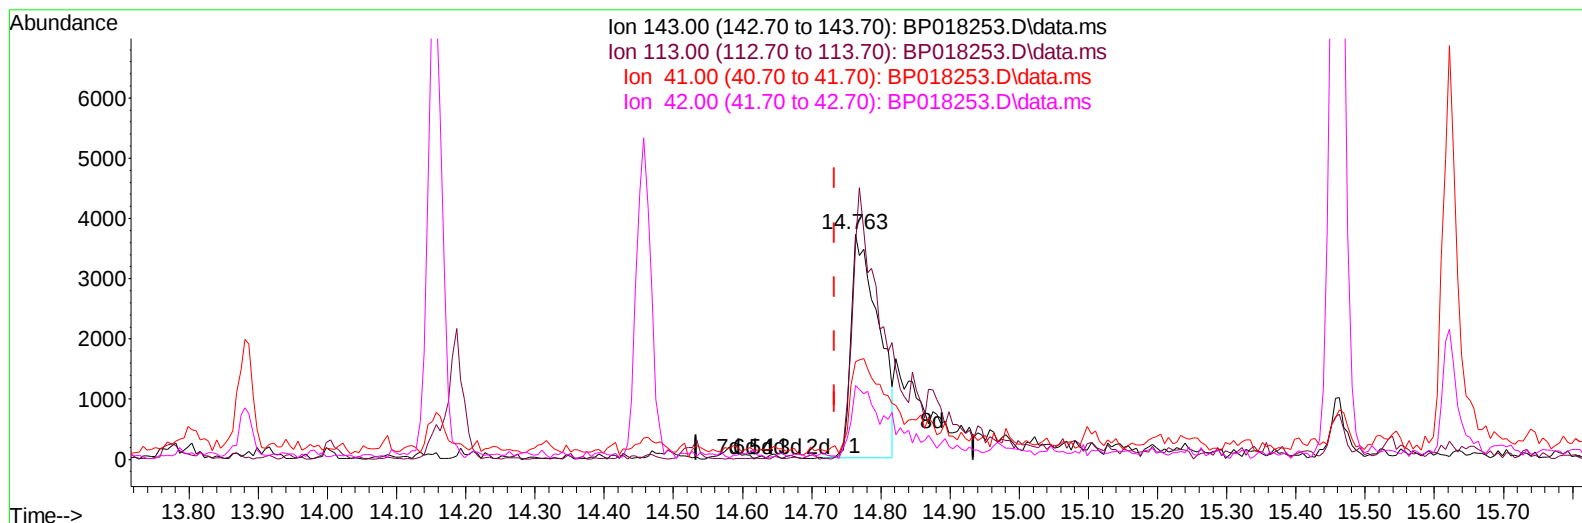

TIC: BP018253.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.763min (+ 0.030) 4.56 ng/u1

response 10120

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.00	95.16
41.00	47.70	43.29
42.00	30.10	32.80




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
Data File : BP018253.D
Acq On : 18 Nov 2023 10:25
Operator : MA/JU
Sample : 05370-05
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCDQ1

Manual IntegrationsAPPROVED

Quant Time: Nov 19 00:50:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 15 18:13:37 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
Supervised By :mohammad ahmed 11/19/2023

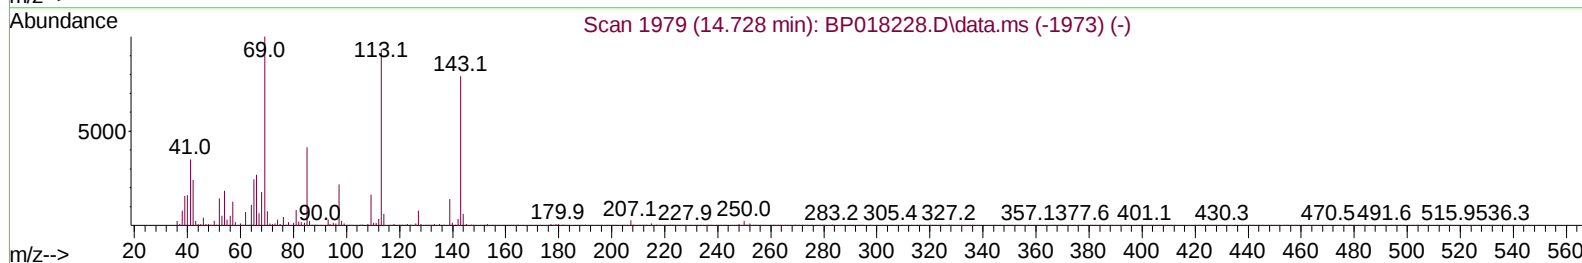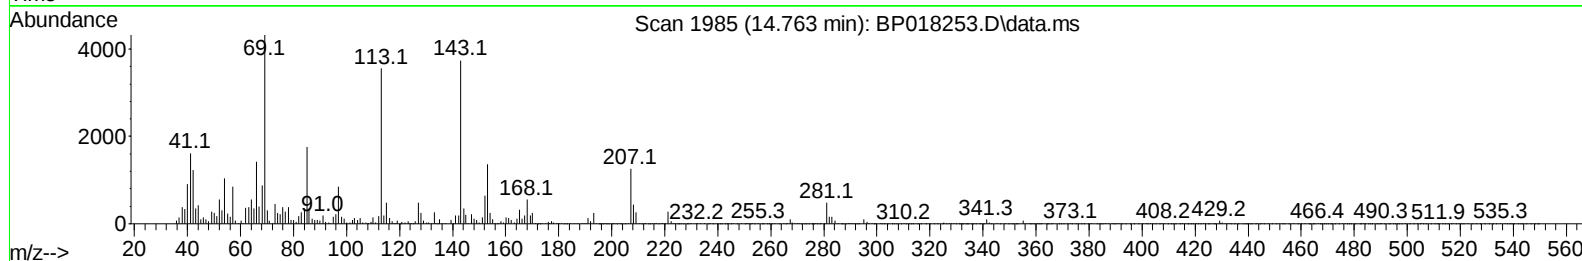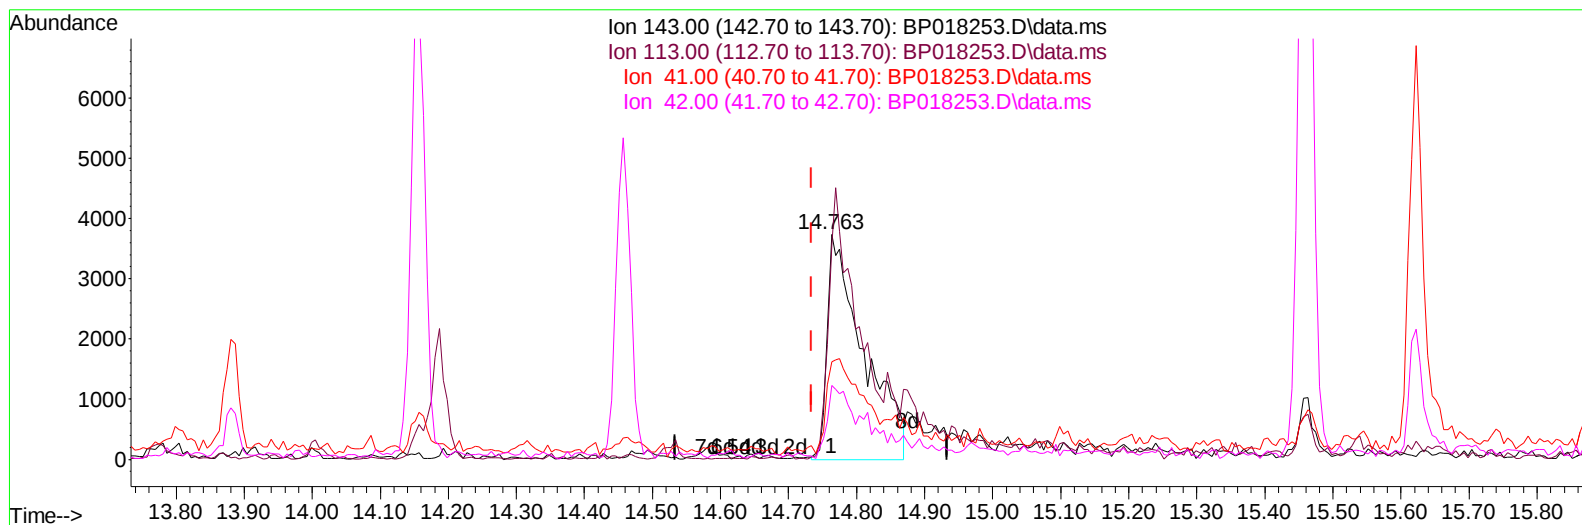

TIC: BP018253.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.763min (+ 0.030) 6.22 ng/ul m

response 13822

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.00	95.16
41.00	47.70	43.29
42.00	30.10	32.80

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
 Data File : BP018253.D
 Acq On : 18 Nov 2023 10:25
 Operator : MA/JU
 Sample : 05370-05
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCDQ1

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/19/2023
 Supervised By :mohammad ahmed 11/19/2023

Quant Time: Nov 19 02:13:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 15 18:13:37 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.775	152	59746	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.593	136	248025	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.457	164	161061	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.239	188	397578	20.000	ng/ul	0.00
79) Chrysene-d12	21.380	240	406460	20.000	ng/ul	0.00
88) Perylene-d12	23.851	264	442810	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.158	96	7604	4.490	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	6.958	99	46621	8.083	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.128	67	129138	38.097	ng/ul	0.00
11) 2-Chlorophenol-d4	7.299	132	142133	31.117	ng/ul	0.00
15) 4-Methylphenol-d8	8.511	113	93123	19.702	ng/ul	0.00
21) Nitrobenzene-d5	8.987	128	85450	38.240	ng/ul	0.00
24) 2-Nitrophenol-d4	9.699	143	95819	37.850	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.228	165	160044	35.471	ng/ul	0.00
31) 4-Chloroaniline-d4	10.775	131	796	0.129	ng/ul	-0.01
46) Dimethylphthalate-d6	13.881	166	634055	42.666	ng/ul	0.00
49) Acenaphthylene-d8	14.157	160	602594	37.229	ng/ul	0.00
54) 4-Nitrophenol-d4	14.763	143	13822m	6.224	ng/ul	0.03
60) Fluorene-d10	15.463	176	522053	42.550	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.622	200	100320	34.904	ng/ul	0.00
73) Anthracene-d10	17.345	188	881197	40.981	ng/ul	0.00
81) Pyrene-d10	19.598	212	1133385	41.745	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.692	264	1122083	43.579	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
Data File : BP018253.D
Acq On : 18 Nov 2023 10:25
Operator : MA/JU
Sample : 05370-05
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCDQ1

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/19/2023
Supervised By :mohammad ahmed 11/19/2023

Quant Time: Nov 19 02:13:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 15 18:13:37 2023
Response via : Initial Calibration

