




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
Data File : BP018255.D
Acq On : 18 Nov 2023 11:33
Operator : MA/JU
Sample : 05370-07
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCDQ3

Manual IntegrationsAPPROVED

Quant Time: Nov 19 00:51:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 15 18:13:37 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
Supervised By :mohammad ahmed 11/19/2023

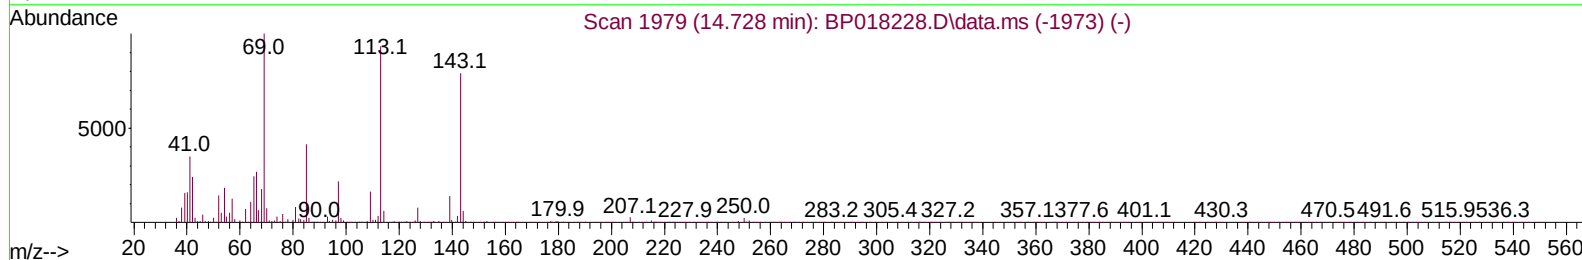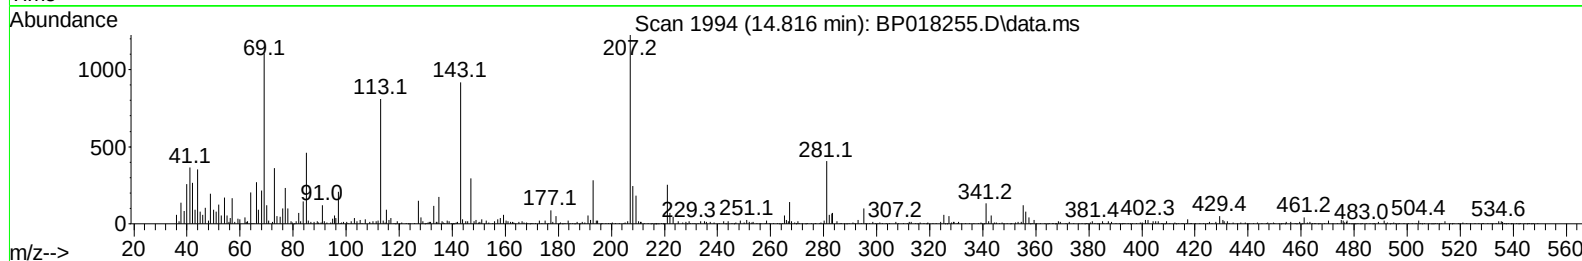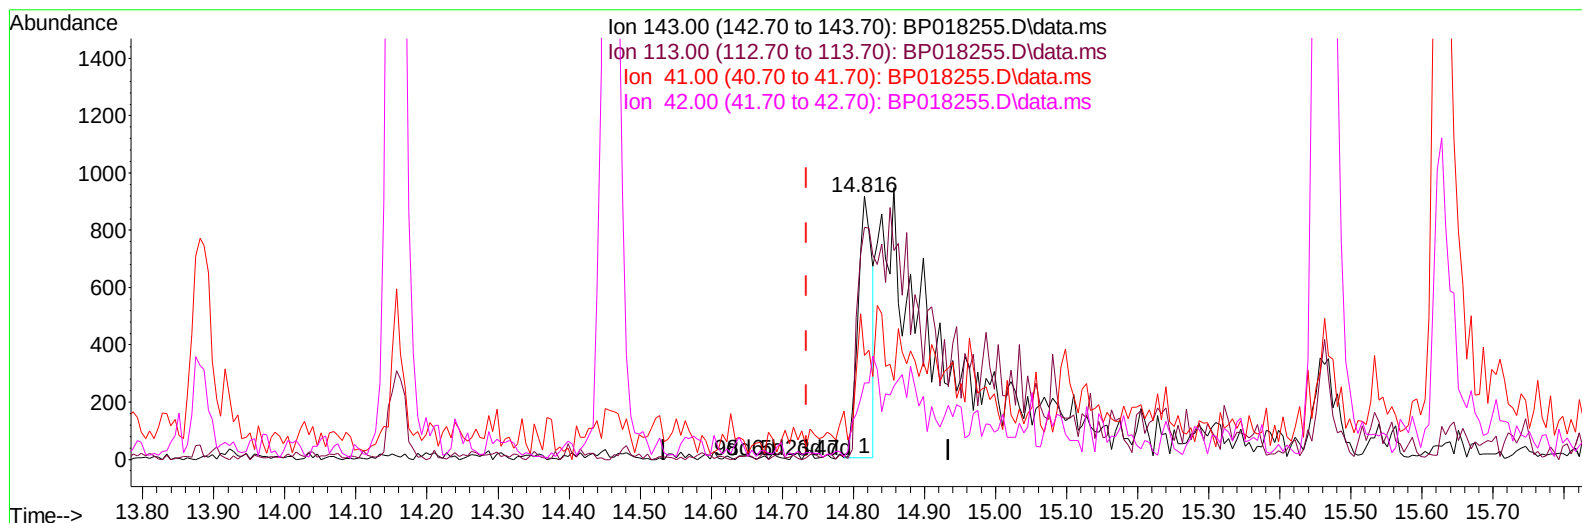

TIC: BP018255.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.816min (+ 0.082) 0.92 ng/ul

response 1276

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.00	88.25
41.00	47.70	39.61
42.00	30.10	29.05




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
 Data File : BP018255.D
 Acq On : 18 Nov 2023 11:33
 Operator : MA/JU
 Sample : 05370-07
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCDQ3

Manual IntegrationsAPPROVED

Quant Time: Nov 19 00:51:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 15 18:13:37 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
 Supervised By :mohammad ahmed 11/19/2023

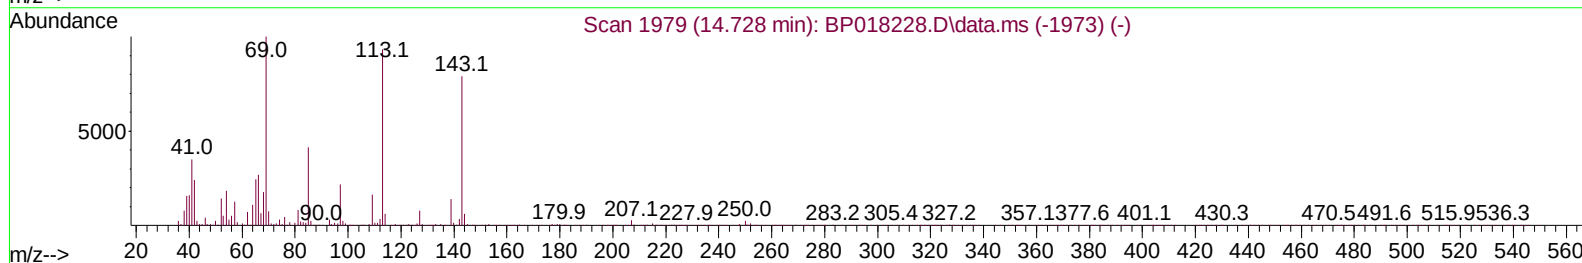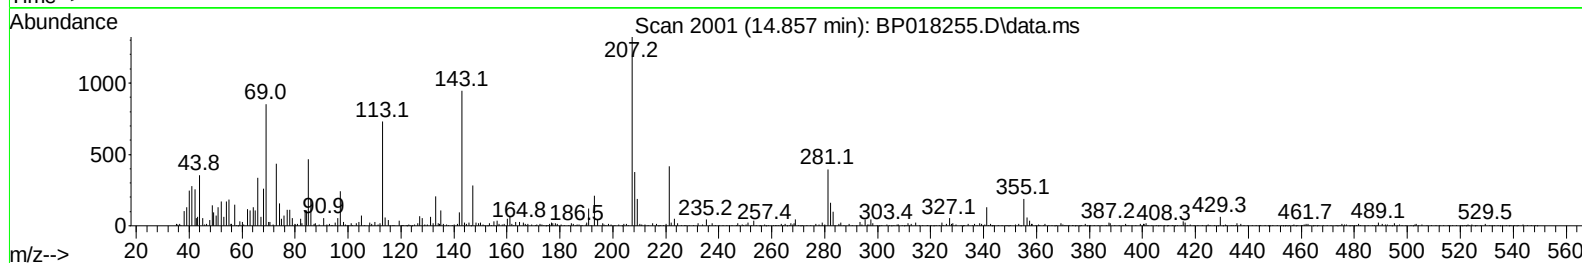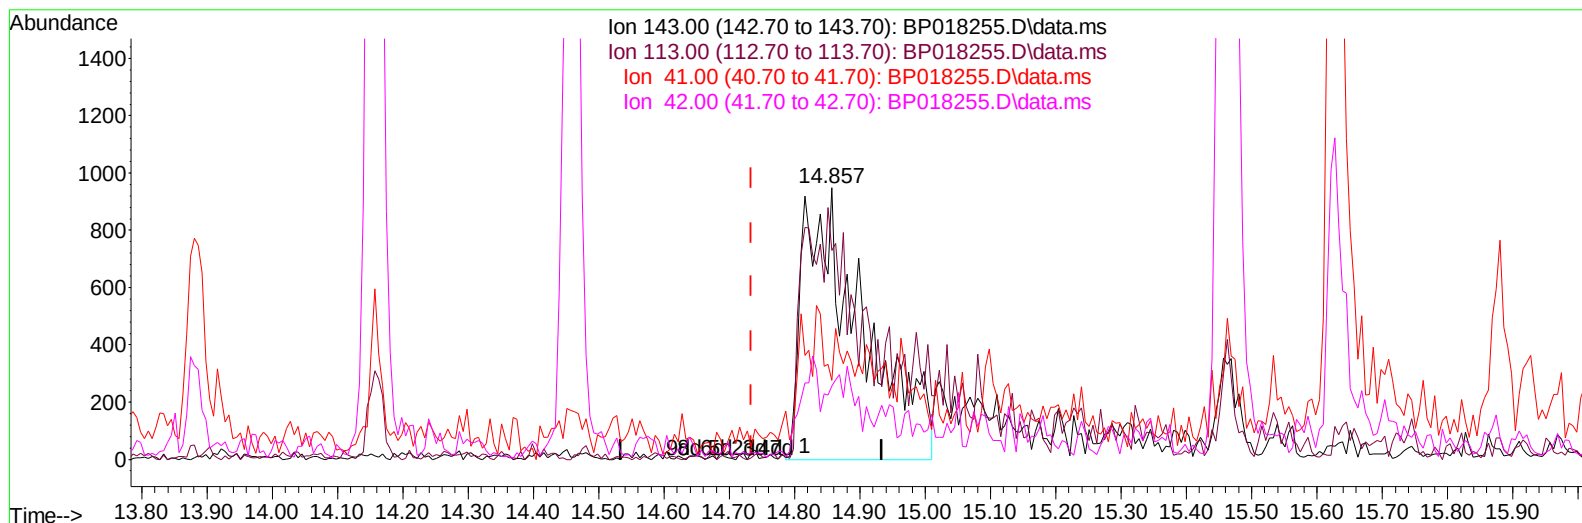

TIC: BP018255.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.857min (+ 0.123) 4.32 ng/ul m

response 5983

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.00	76.90#
41.00	47.70	29.11#
42.00	30.10	26.90

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
 Data File : BP018255.D
 Acq On : 18 Nov 2023 11:33
 Operator : MA/JU
 Sample : 05370-07
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCDQ3

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/19/2023
 Supervised By :mohammad ahmed 11/19/2023

Quant Time: Nov 19 02:23:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 15 18:13:37 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.781	152	42540	20.000	ng/ul	0.00
20) Naphthalene-d8	10.593	136	170098	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.457	164	100508	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.239	188	234280	20.000	ng/ul	0.00
79) Chrysene-d12	21.380	240	229095	20.000	ng/ul	0.00
88) Perylene-d12	23.857	264	271572	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.158	96	7696	6.382	ng/uL	0.00
4) Pyridine-d5	3.599	84	38094	12.115	ng/ul	0.00
7) Phenol-d5	6.963	99	22025	5.363	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	7.128	67	83356	34.537	ng/ul	0.00
11) 2-Chlorophenol-d4	7.305	132	82106	25.246	ng/ul	0.00
15) 4-Methylphenol-d8	8.516	113	51401	15.274	ng/ul	0.00
21) Nitrobenzene-d5	8.987	128	50989	33.272	ng/ul	0.00
24) 2-Nitrophenol-d4	9.704	143	55866	32.178	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.234	165	83603	27.018	ng/ul	0.00
31) 4-Chloroaniline-d4	10.781	131	121233	28.569	ng/ul	0.00
46) Dimethylphthalate-d6	13.881	166	363329	39.179	ng/ul	0.00
49) Acenaphthylene-d8	14.157	160	369330	36.565	ng/ul	0.00
54) 4-Nitrophenol-d4	14.857	143	5983m	4.317	ng/ul	0.12
60) Fluorene-d10	15.463	176	301542	39.384	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.628	200	50353	29.730	ng/ul	0.00
73) Anthracene-d10	17.345	188	527010	41.592	ng/ul	0.00
81) Pyrene-d10	19.598	212	723127	47.255	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.692	264	686515	43.475	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
Data File : BP018255.D
Acq On : 18 Nov 2023 11:33
Operator : MA/JU
Sample : 05370-07
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCDQ3

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/19/2023
Supervised By :mohammad ahmed 11/19/2023

Quant Time: Nov 19 02:23:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 15 18:13:37 2023
Response via : Initial Calibration

