




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
Data File : BP018257.D
Acq On : 18 Nov 2023 12:41
Operator : MA/JU
Sample : 05370-09
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCDQ5

Manual IntegrationsAPPROVED

Quant Time: Nov 19 00:52:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 15 18:13:37 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
Supervised By :mohammad ahmed 11/19/2023

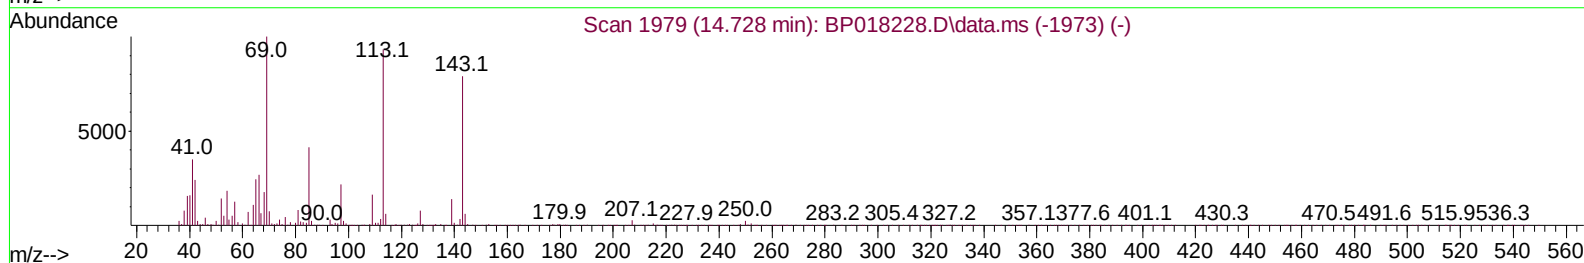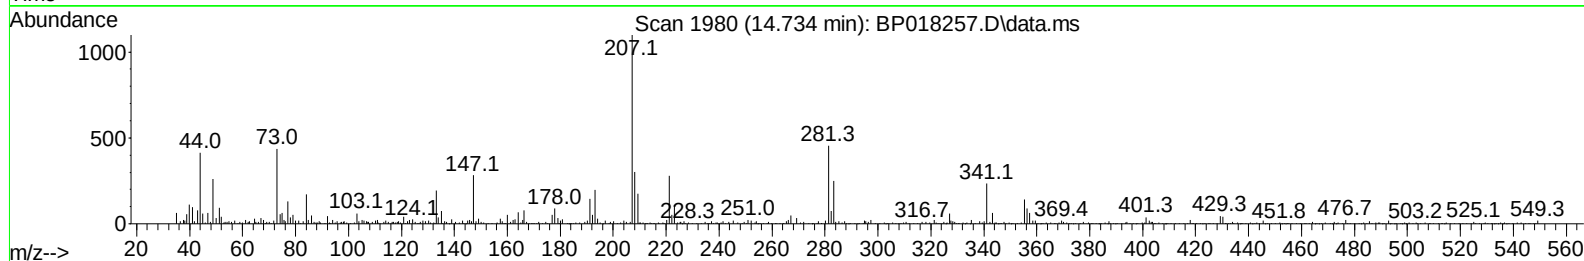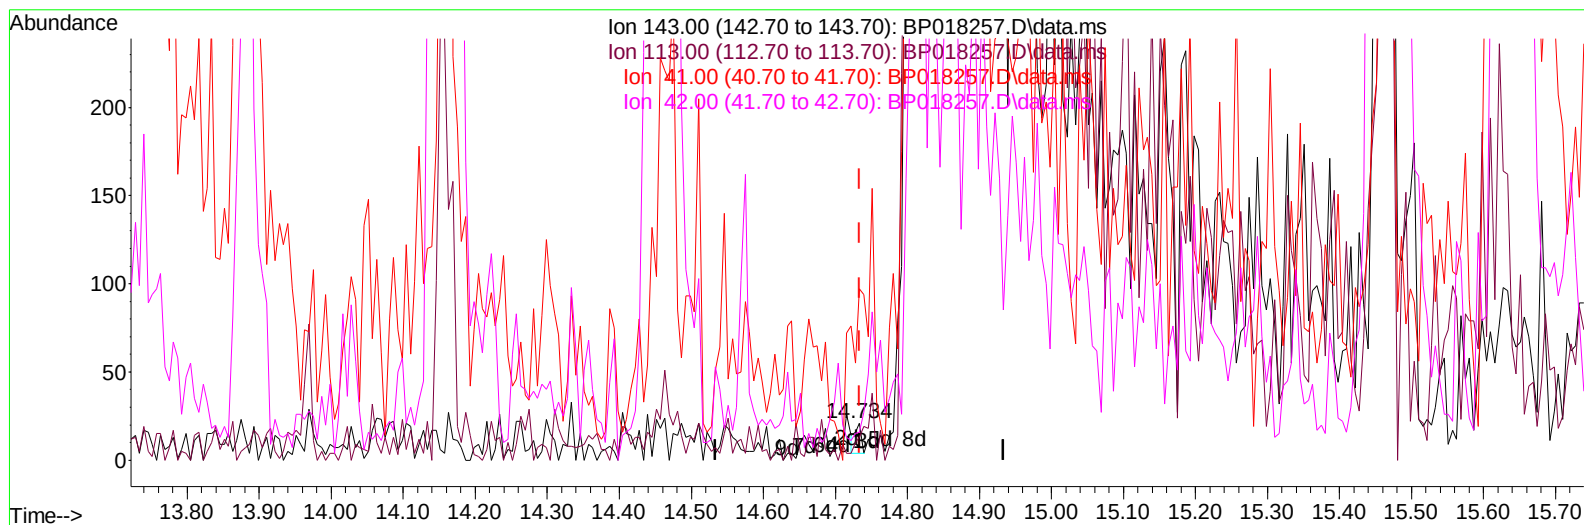

TIC: BP018257.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.734min (+ 0.000) 0.01 ng/ul

response 10

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.00	61.90#
41.00	47.70	538.10#
42.00	30.10	76.19#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
 Data File : BP018257.D
 Acq On : 18 Nov 2023 12:41
 Operator : MA/JU
 Sample : 05370-09
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCDQ5

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/19/2023
 Supervised By :mohammad ahmed 11/19/2023

Quant Time: Nov 19 02:29:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 15 18:13:37 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.781	152	49150	20.000	ng/ul	0.00
20) Naphthalene-d8	10.593	136	198922	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.457	164	125921	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.239	188	296664	20.000	ng/ul	0.00
79) Chrysene-d12	21.380	240	279597	20.000	ng/ul	0.00
88) Perylene-d12	23.857	264	327323	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.158	96	7430	5.333	ng/uL	0.00
4) Pyridine-d5	3.605	84	24252	6.676	ng/ul	0.01
7) Phenol-d5	6.963	99	24196	5.099	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	7.128	67	77306	27.723	ng/ul	0.00
11) 2-Chlorophenol-d4	7.305	132	79776	21.230	ng/ul	0.00
15) 4-Methylphenol-d8	8.510	113	50731	13.047	ng/ul	0.00
21) Nitrobenzene-d5	8.987	128	49707	27.735	ng/ul	0.00
24) 2-Nitrophenol-d4	9.704	143	51512	25.371	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.234	165	83242	23.003	ng/ul	0.00
31) 4-Chloroaniline-d4	10.787	131	95732	19.291	ng/ul	0.00
46) Dimethylphthalate-d6	13.887	166	382518	32.923	ng/ul	0.00
49) Acenaphthylene-d8	14.157	160	371003	29.318	ng/ul	0.00
54) 4-Nitrophenol-d4	14.810	143	7344m	4.230	ng/ul	0.08
60) Fluorene-d10	15.463	176	350662	36.557	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.628	200	62752	29.260	ng/ul	0.00
73) Anthracene-d10	17.345	188	594421	37.048	ng/ul	0.00
81) Pyrene-d10	19.604	212	742159	39.739	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.692	264	715182	37.576	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
Data File : BP018257.D
Acq On : 18 Nov 2023 12:41
Operator : MA/JU
Sample : 05370-09
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCDQ5

Manual IntegrationsAPPROVED

Quant Time: Nov 19 02:29:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 15 18:13:37 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
Supervised By :mohammad ahmed 11/19/2023

