

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP111723\  
 Data File : BP018215.D  
 Acq On : 17 Nov 2023 09:49  
 Operator : MA/JU  
 Sample : PB157213BL  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 SBLK213

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP111023.MA.M  
 Title : SVOA CALIBRATION

Signal : TIC: BP018215.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 3.158       | 9             | 12          | 18           | rBV      | 20877          | 27843         | 1.90%           | 0.170%        |
| 2         | 3.528       | 73            | 75          | 79           | rVB4     | 2147           | 2174          | 0.15%           | 0.013%        |
| 3         | 3.593       | 83            | 86          | 100          | rBV      | 190741         | 316007        | 21.52%          | 1.926%        |
| 4         | 3.905       | 133           | 139         | 141          | rBV6     | 4197           | 8326          | 0.57%           | 0.051%        |
| 5         | 4.252       | 196           | 198         | 203          | rVB5     | 3384           | 4661          | 0.32%           | 0.028%        |
| 6         | 4.334       | 210           | 212         | 217          | rVB6     | 1932           | 1985          | 0.14%           | 0.012%        |
| 7         | 4.640       | 262           | 264         | 265          | rBV2     | 1945           | 1909          | 0.13%           | 0.012%        |
| 8         | 5.964       | 487           | 489         | 491          | rVB3     | 1954           | 1554          | 0.11%           | 0.009%        |
| 9         | 6.028       | 496           | 500         | 502          | rBV5     | 1233           | 1651          | 0.11%           | 0.010%        |
| 10        | 6.081       | 505           | 509         | 511          | rBV5     | 847            | 1512          | 0.10%           | 0.009%        |
| 11        | 6.246       | 535           | 537         | 540          | rVV4     | 1863           | 1964          | 0.13%           | 0.012%        |
| 12        | 6.275       | 540           | 542         | 547          | rVV6     | 1798           | 3376          | 0.23%           | 0.021%        |
| 13        | 6.340       | 551           | 553         | 556          | rVB3     | 1656           | 1773          | 0.12%           | 0.011%        |
| 14        | 6.952       | 651           | 657         | 681          | rBV      | 214750         | 431334        | 29.37%          | 2.628%        |
| 15        | 7.134       | 681           | 688         | 699          | rBV      | 190026         | 308468        | 21.00%          | 1.880%        |
| 16        | 7.305       | 711           | 717         | 736          | rBV      | 274302         | 499398        | 34.01%          | 3.043%        |
| 17        | 7.622       | 769           | 771         | 774          | rVB4     | 2328           | 2289          | 0.16%           | 0.014%        |
| 18        | 7.781       | 792           | 798         | 813          | rBV      | 229801         | 413805        | 28.18%          | 2.521%        |
| 19        | 8.222       | 870           | 873         | 874          | rBV3     | 1423           | 1540          | 0.10%           | 0.009%        |
| 20        | 8.511       | 914           | 922         | 945          | rBV      | 270683         | 559182        | 38.08%          | 3.407%        |
| 21        | 8.663       | 945           | 948         | 950          | rVB3     | 1400           | 1854          | 0.13%           | 0.011%        |
| 22        | 8.987       | 994           | 1003        | 1021         | rBV      | 228147         | 468363        | 31.89%          | 2.854%        |
| 23        | 9.340       | 1061          | 1063        | 1070         | rVB8     | 2263           | 3679          | 0.25%           | 0.022%        |
| 24        | 9.405       | 1070          | 1074        | 1076         | rBV4     | 1202           | 1726          | 0.12%           | 0.011%        |
| 25        | 9.705       | 1116          | 1125        | 1146         | rBV      | 201732         | 419091        | 28.54%          | 2.554%        |
| 26        | 10.181      | 1204          | 1206        | 1208         | rBV3     | 1280           | 1481          | 0.10%           | 0.009%        |
| 27        | 10.234      | 1208          | 1215        | 1235         | rBV      | 230873         | 536296        | 36.52%          | 3.268%        |
| 28        | 10.599      | 1269          | 1277        | 1289         | rBV      | 312039         | 537643        | 36.61%          | 3.276%        |
| 29        | 10.787      | 1303          | 1309        | 1341         | rVV      | 207784         | 544061        | 37.05%          | 3.315%        |
| 30        | 11.093      | 1359          | 1361        | 1363         | rVB3     | 1941           | 1726          | 0.12%           | 0.011%        |
| 31        | 11.746      | 1466          | 1472        | 1474         | rBV7     | 1165           | 1569          | 0.11%           | 0.010%        |
| 32        | 12.263      | 1557          | 1560        | 1563         | rBV5     | 2584           | 3356          | 0.23%           | 0.020%        |
| 33        | 12.787      | 1646          | 1649        | 1653         | rBV5     | 1191           | 2228          | 0.15%           | 0.014%        |
| 34        | 13.304      | 1732          | 1737        | 1740         | rBV6     | 2724           | 4298          | 0.29%           | 0.026%        |
| 35        | 13.493      | 1764          | 1769        | 1771         | rVB6     | 1155           | 1607          | 0.11%           | 0.010%        |
| 36        | 13.887      | 1830          | 1836        | 1854         | rBV      | 571096         | 873572        | 59.48%          | 5.323%        |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP111723\  
 Data File : BP018215.D  
 Acq On : 17 Nov 2023 09:49  
 Operator : MA/JU  
 Sample : PB157213BL  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 SBLK213

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP111023.MA.M  
 Title : SVOA CALIBRATION

|    |        |      |      |      |      |         |         |         |        |
|----|--------|------|------|------|------|---------|---------|---------|--------|
| 37 | 14.157 | 1876 | 1882 | 1902 | rVV  | 615499  | 937690  | 63.85%  | 5.714% |
| 38 | 14.463 | 1927 | 1934 | 1946 | rBV  | 446988  | 680107  | 46.31%  | 4.144% |
| 39 | 14.757 | 1978 | 1984 | 2005 | rBV4 | 56183   | 250796  | 17.08%  | 1.528% |
| 40 | 15.416 | 2093 | 2096 | 2098 | rBV3 | 1183    | 1669    | 0.11%   | 0.010% |
| 41 | 15.463 | 2098 | 2104 | 2116 | rBV  | 837135  | 1208817 | 82.31%  | 7.366% |
| 42 | 15.628 | 2127 | 2132 | 2145 | rBV  | 164873  | 332721  | 22.66%  | 2.027% |
| 43 | 15.804 | 2160 | 2162 | 2166 | rVB5 | 1973    | 2569    | 0.17%   | 0.016% |
| 44 | 16.210 | 2228 | 2231 | 2235 | rVB6 | 1242    | 1991    | 0.14%   | 0.012% |
| 45 | 16.269 | 2239 | 2241 | 2246 | rVB6 | 1862    | 2568    | 0.17%   | 0.016% |
| 46 | 16.492 | 2276 | 2279 | 2282 | rBV5 | 1427    | 2182    | 0.15%   | 0.013% |
| 47 | 17.051 | 2369 | 2374 | 2377 | rBV7 | 2169    | 3626    | 0.25%   | 0.022% |
| 48 | 17.081 | 2377 | 2379 | 2384 | rVB6 | 1385    | 1643    | 0.11%   | 0.010% |
| 49 | 17.245 | 2401 | 2407 | 2417 | rBV  | 605241  | 843799  | 57.46%  | 5.142% |
| 50 | 17.345 | 2418 | 2424 | 2444 | rVV  | 863505  | 1315897 | 89.60%  | 8.018% |
| 51 | 17.545 | 2456 | 2458 | 2461 | rBV4 | 1914    | 1700    | 0.12%   | 0.010% |
| 52 | 17.587 | 2461 | 2465 | 2467 | rVB5 | 1649    | 1958    | 0.13%   | 0.012% |
| 53 | 17.739 | 2486 | 2491 | 2494 | rBV7 | 1240    | 2220    | 0.15%   | 0.014% |
| 54 | 17.875 | 2512 | 2514 | 2518 | rBV4 | 1854    | 2010    | 0.14%   | 0.012% |
| 55 | 18.110 | 2551 | 2554 | 2555 | rBV3 | 2062    | 2148    | 0.15%   | 0.013% |
| 56 | 18.134 | 2555 | 2558 | 2559 | rVV3 | 2339    | 2441    | 0.17%   | 0.015% |
| 57 | 18.634 | 2641 | 2643 | 2644 | rBV2 | 2661    | 2302    | 0.16%   | 0.014% |
| 58 | 18.839 | 2675 | 2678 | 2680 | rVB4 | 1812    | 1902    | 0.13%   | 0.012% |
| 59 | 18.863 | 2680 | 2682 | 2684 | rBV3 | 1875    | 2189    | 0.15%   | 0.013% |
| 60 | 19.175 | 2731 | 2735 | 2740 | rBV4 | 10668   | 17010   | 1.16%   | 0.104% |
| 61 | 19.257 | 2744 | 2749 | 2754 | rVV3 | 8890    | 15202   | 1.04%   | 0.093% |
| 62 | 19.598 | 2802 | 2807 | 2824 | rBV  | 1035429 | 1456138 | 99.15%  | 8.873% |
| 63 | 21.375 | 3105 | 3109 | 3122 | rBV  | 591388  | 900593  | 61.32%  | 5.488% |
| 64 | 23.680 | 3494 | 3501 | 3512 | rBV3 | 724518  | 1468591 | 100.00% | 8.949% |
| 65 | 23.845 | 3523 | 3529 | 3544 | rVB  | 399904  | 905625  | 61.67%  | 5.518% |
| 66 | 27.904 | 4215 | 4219 | 4221 | rBV3 | 30386   | 50042   | 3.41%   | 0.305% |




Sum of corrected areas: 16411447

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP111723\  
Data File : BP018215.D  
Acq On : 17 Nov 2023 09:49  
Operator : MA/JU  
Sample : PB157213BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
SBLK213

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP111023.MA.M  
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L  
TIC Integration Parameters: LSCINT.P

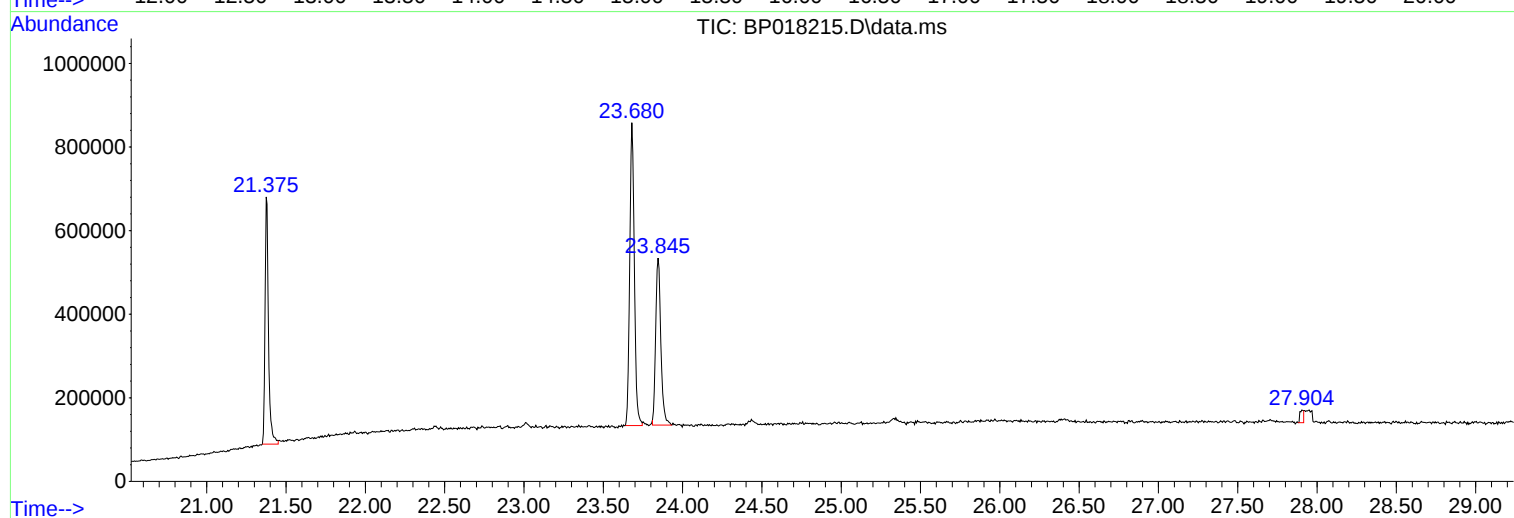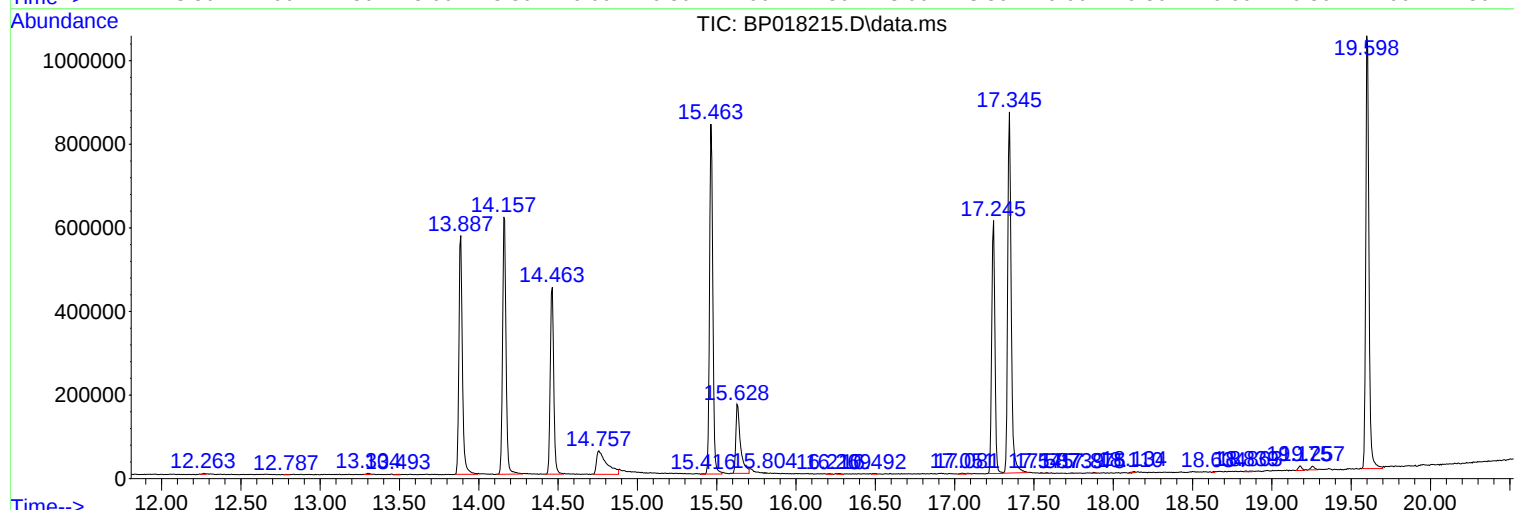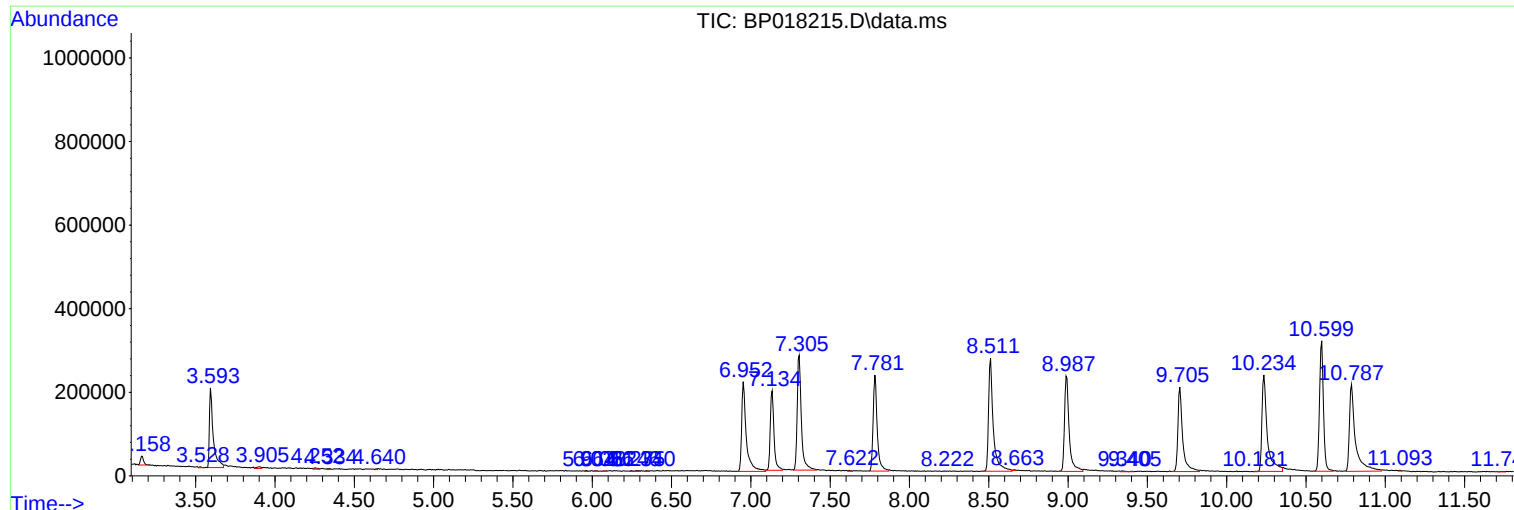

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP111723\  
Data File : BP018215.D  
Acq On : 17 Nov 2023 09:49  
Operator : MA/JU  
Sample : PB157213BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
SBLK213

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP111023.MA.M  
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP111723\  
Data File : BP018215.D  
Acq On : 17 Nov 2023 09:49  
Operator : MA/JU  
Sample : PB157213BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
SBLK213

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP111023.MA.M  
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|