

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
 Data File : BP018229.D
 Acq On : 17 Nov 2023 20:15
 Operator : MA/JU
 Sample : PB157215BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK215

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018229.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.158	8	12	19	rVB	24676	32766	1.73%	0.187%
2	3.458	61	63	65	rBV2	3104	2493	0.13%	0.014%
3	3.593	83	86	111	rBV	233103	388989	20.57%	2.217%
4	3.899	134	138	143	rVB6	3770	6262	0.33%	0.036%
5	4.164	181	183	187	rVB5	2559	2925	0.15%	0.017%
6	4.193	187	188	193	rVV5	2610	3565	0.19%	0.020%
7	4.252	197	198	203	rVB4	3482	3545	0.19%	0.020%
8	4.681	267	271	273	rBV5	2035	3354	0.18%	0.019%
9	6.952	651	657	679	rVV	258921	511440	27.05%	2.914%
10	7.128	682	687	705	rVB	221368	368238	19.48%	2.098%
11	7.299	711	716	736	rBV	303797	560083	29.62%	3.192%
12	7.781	791	798	811	rBV	147661	293300	15.51%	1.671%
13	8.052	842	844	847	rVB4	2557	2164	0.11%	0.012%
14	8.240	873	876	878	rBV4	1671	1899	0.10%	0.011%
15	8.505	915	921	945	rVV	324476	672600	35.57%	3.833%
16	8.987	997	1003	1022	rBV	286913	549230	29.05%	3.130%
17	9.322	1057	1060	1065	rBV6	1035	2036	0.11%	0.012%
18	9.699	1117	1124	1147	rBV	240800	503427	26.63%	2.869%
19	10.228	1208	1214	1245	rBV	276701	671891	35.54%	3.829%
20	10.599	1269	1277	1287	rBV	193403	339087	17.93%	1.932%
21	10.781	1301	1308	1340	rBV	263810	659086	34.86%	3.756%
22	12.269	1554	1561	1567	rBV	4202	10335	0.55%	0.059%
23	12.740	1639	1641	1646	rVB6	1836	2270	0.12%	0.013%
24	13.298	1733	1736	1742	rVB5	4865	7489	0.40%	0.043%
25	13.887	1829	1836	1850	rBV	679094	1067910	56.48%	6.085%
26	14.157	1876	1882	1897	rBV	759899	1142921	60.45%	6.513%
27	14.463	1927	1934	1950	rVB	276271	431607	22.83%	2.460%
28	14.745	1975	1982	2010	rBV	89137	383730	20.30%	2.187%
29	15.228	2062	2064	2067	rBV4	1911	2641	0.14%	0.015%
30	15.463	2098	2104	2114	rBV	1000625	1445608	76.46%	8.238%
31	15.628	2126	2132	2144	rBV	250439	463311	24.51%	2.640%
32	16.492	2276	2279	2281	rBV4	1423	1891	0.10%	0.011%
33	17.092	2379	2381	2385	rVB5	1721	1950	0.10%	0.011%
34	17.134	2385	2388	2390	rBV3	1832	2343	0.12%	0.013%
35	17.245	2401	2407	2415	rBV	372480	530195	28.04%	3.021%
36	17.345	2418	2424	2443	rVV	1059736	1590523	84.12%	9.064%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
Data File : BP018229.D
Acq On : 17 Nov 2023 20:15
Operator : MA/JU
Sample : PB157215BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK215

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Title : SVOA CALIBRATION

37	17.651	2474	2476	2480	rVB5	2229	2262	0.12%	0.013%
38	18.004	2531	2536	2537	rBV5	2092	3310	0.18%	0.019%
39	18.134	2552	2558	2564	rBV10	3534	8118	0.43%	0.046%
40	18.728	2655	2659	2660	rBV4	2038	2846	0.15%	0.016%
41	19.175	2731	2735	2743	rVB5	12959	18262	0.97%	0.104%
42	19.257	2745	2749	2755	rVB3	10478	15919	0.84%	0.091%
43	19.598	2802	2807	2825	rBV	1332993	1890667	100.00%	10.774%
44	21.380	3105	3110	3121	rBV	359807	560203	29.63%	3.192%
45	23.680	3494	3501	3521	rVB	899039	1828687	96.72%	10.421%
46	23.851	3524	3530	3544	rVB	244038	555107	29.36%	3.163%




Sum of corrected areas: 17548485

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
Data File : BP018229.D
Acq On : 17 Nov 2023 20:15
Operator : MA/JU
Sample : PB157215BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK215

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

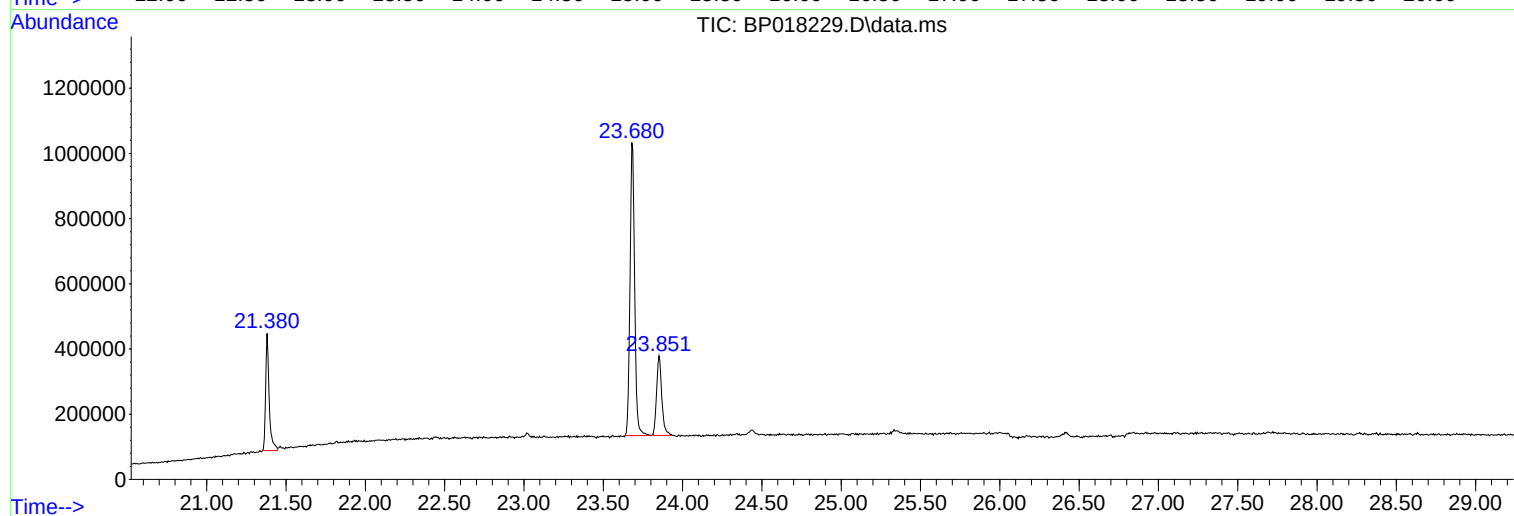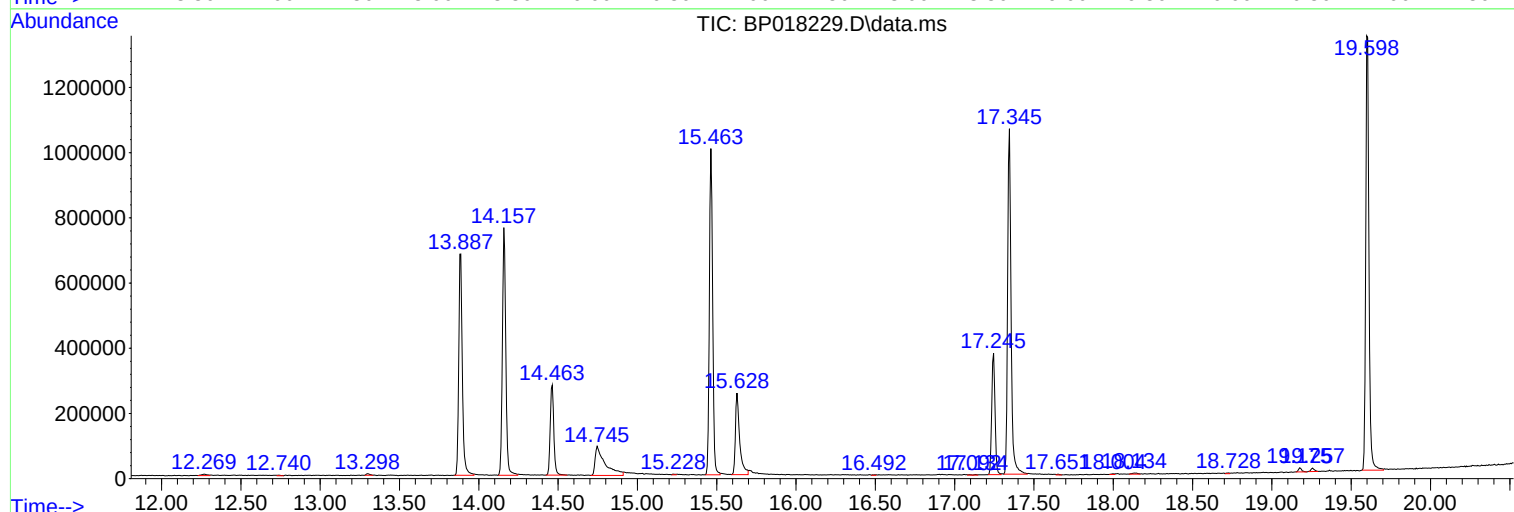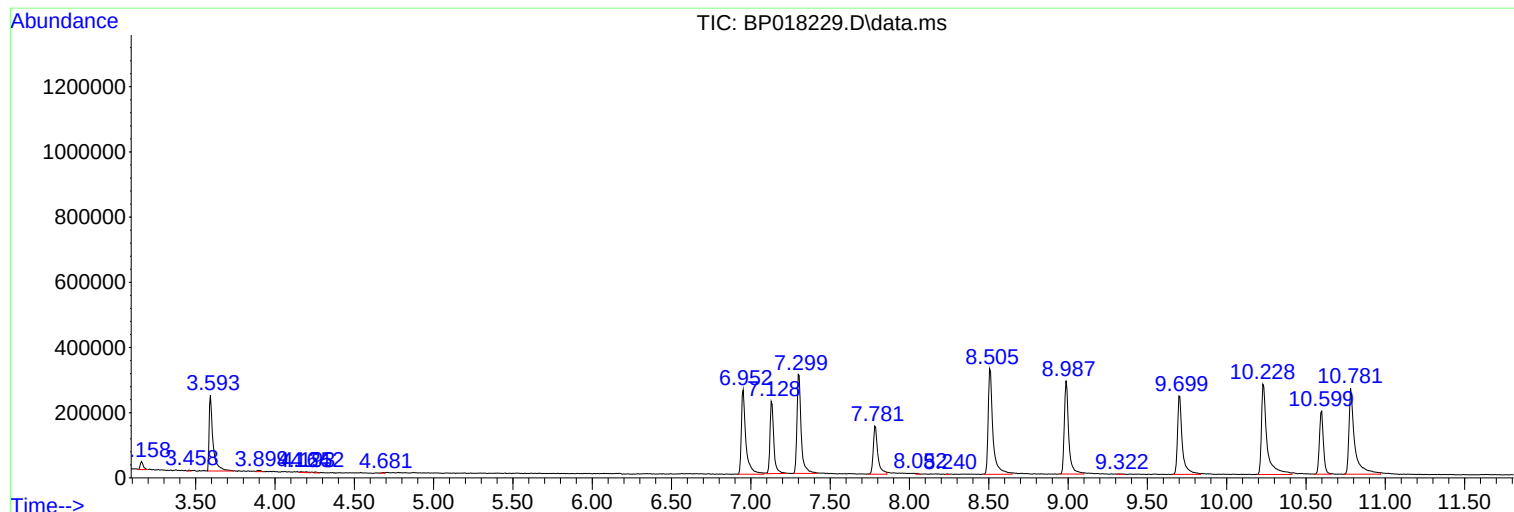

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
Data File : BP018229.D
Acq On : 17 Nov 2023 20:15
Operator : MA/JU
Sample : PB157215BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK215

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
Data File : BP018229.D
Acq On : 17 Nov 2023 20:15
Operator : MA/JU
Sample : PB157215BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK215

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------