

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
 Data File : BP018230.D
 Acq On : 17 Nov 2023 20:48
 Operator : MA/JU
 Sample : PB157219BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK219

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018230.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.129	5	7	9	rBV3	2416	2721	0.22%	0.021%
2	3.158	9	12	17	rVV	18740	23946	1.94%	0.189%
3	3.358	44	46	47	rBV2	1909	1341	0.11%	0.011%
4	3.434	55	59	62	rBV6	1651	2300	0.19%	0.018%
5	3.593	83	86	103	rBV	130476	227667	18.47%	1.796%
6	3.899	136	138	144	rVB7	2696	3868	0.31%	0.031%
7	4.176	184	185	190	rBV5	2153	2288	0.19%	0.018%
8	4.599	255	257	262	rVB7	1197	1702	0.14%	0.013%
9	5.287	372	374	376	rVB3	1643	1304	0.11%	0.010%
10	5.346	383	384	386	rBV2	1710	1265	0.10%	0.010%
11	5.699	441	444	446	rBV4	1302	1807	0.15%	0.014%
12	6.105	511	513	515	rBV2	1670	1382	0.11%	0.011%
13	6.293	544	545	548	rBV3	1158	1269	0.10%	0.010%
14	6.475	575	576	581	rBV5	1042	1403	0.11%	0.011%
15	6.805	629	632	635	rVB5	1193	1542	0.13%	0.012%
16	6.840	635	638	639	rBV2	1711	1336	0.11%	0.011%
17	6.952	649	657	674	rBV	182491	379806	30.82%	2.997%
18	7.134	682	688	702	rBV	155435	262885	21.33%	2.074%
19	7.305	710	717	730	rBV	221409	400812	32.52%	3.162%
20	7.387	730	731	736	rVB5	3682	4071	0.33%	0.032%
21	7.493	745	749	751	rVB5	1033	1562	0.13%	0.012%
22	7.675	779	780	783	rVB3	1446	1287	0.10%	0.010%
23	7.781	790	798	812	rBV	170132	312940	25.39%	2.469%
24	7.952	824	827	830	rBV5	1387	1699	0.14%	0.013%
25	8.069	845	847	850	rBV3	1189	1281	0.10%	0.010%
26	8.387	898	901	904	rBV5	1237	1904	0.15%	0.015%
27	8.511	916	922	939	rBV	214255	442095	35.87%	3.488%
28	8.722	955	958	965	rVB8	1459	2672	0.22%	0.021%
29	8.987	997	1003	1023	rBV	188389	381739	30.97%	3.012%
30	9.393	1070	1072	1078	rVB5	1590	2547	0.21%	0.020%
31	9.440	1078	1080	1084	rBV5	1674	2497	0.20%	0.020%
32	9.705	1118	1125	1140	rBV	161305	331111	26.87%	2.612%
33	10.040	1180	1182	1185	rVB3	1194	1234	0.10%	0.010%
34	10.234	1207	1215	1236	rBV	174310	435853	35.36%	3.439%
35	10.599	1270	1277	1287	rBV	209355	362153	29.38%	2.857%
36	10.787	1303	1309	1330	rBV	132237	363600	29.50%	2.869%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
 Data File : BP018230.D
 Acq On : 17 Nov 2023 20:48
 Operator : MA/JU
 Sample : PB157219BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK219

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

37	11.175	1369	1375	1377	rBV7	1019	1395	0.11%	0.011%
38	11.410	1412	1415	1421	rVB8	1355	2320	0.19%	0.018%
39	11.463	1421	1424	1426	rBV4	989	1299	0.11%	0.010%
40	11.646	1452	1455	1457	rVB4	1543	1763	0.14%	0.014%

41	11.669	1457	1459	1464	rVB6	1254	1445	0.12%	0.011%
42	11.781	1476	1478	1481	rVB4	1608	1479	0.12%	0.012%
43	11.822	1483	1485	1487	rVB2	1675	1458	0.12%	0.012%
44	12.005	1512	1516	1518	rBV4	1106	1590	0.13%	0.013%
45	12.269	1557	1561	1563	rBV5	2017	3350	0.27%	0.026%

46	13.081	1695	1699	1700	rVB4	1215	1300	0.11%	0.010%
47	13.299	1732	1736	1739	rBV6	1943	2877	0.23%	0.023%
48	13.410	1753	1755	1760	rVB6	1186	1290	0.10%	0.010%
49	13.887	1830	1836	1855	rBV	450555	704714	57.18%	5.560%
50	14.157	1876	1882	1893	rBV	494458	723167	58.68%	5.706%

51	14.393	1919	1922	1924	rVB4	1363	1413	0.11%	0.011%
52	14.463	1926	1934	1949	rVV	311047	479329	38.89%	3.782%
53	14.687	1971	1972	1978	rVB6	1134	1610	0.13%	0.013%
54	14.757	1978	1984	1995	rBV3	43344	159331	12.93%	1.257%
55	15.075	2036	2038	2043	rBV6	1324	2271	0.18%	0.018%

56	15.163	2051	2053	2054	rBV2	1756	1688	0.14%	0.013%
57	15.251	2063	2068	2070	rBV5	1562	2694	0.22%	0.021%
58	15.463	2097	2104	2119	rBV	646033	948028	76.92%	7.480%
59	15.628	2127	2132	2144	rBV2	134852	286578	23.25%	2.261%
60	15.922	2180	2182	2185	rBV4	1396	1503	0.12%	0.012%

61	16.022	2197	2199	2201	rVB3	1603	1331	0.11%	0.011%
62	16.040	2201	2202	2204	rBV2	1691	1472	0.12%	0.012%
63	16.098	2211	2212	2215	rBV3	1191	1239	0.10%	0.010%
64	16.416	2264	2266	2269	rBV3	1338	1506	0.12%	0.012%
65	16.892	2343	2347	2349	rBV5	1891	2300	0.19%	0.018%

66	17.240	2400	2406	2416	rBV	411430	589058	47.80%	4.648%
67	17.345	2418	2424	2444	rVB	667076	1040182	84.40%	8.207%
68	17.575	2461	2463	2466	rVB4	1573	1480	0.12%	0.012%
69	17.716	2485	2487	2489	rBV3	1803	1847	0.15%	0.015%
70	18.122	2552	2556	2558	rBV5	2168	3343	0.27%	0.026%

71	18.487	2616	2618	2620	rVB2	1801	1374	0.11%	0.011%
72	18.510	2620	2622	2624	rBV2	1754	1674	0.14%	0.013%
73	18.598	2635	2637	2640	rBV4	1221	1373	0.11%	0.011%
74	18.710	2653	2656	2657	rBV3	1480	1616	0.13%	0.013%
75	18.734	2659	2660	2662	rBV2	1531	1339	0.11%	0.011%

76	18.957	2696	2698	2701	rVB4	1987	1751	0.14%	0.014%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
Data File : BP018230.D
Acq On : 17 Nov 2023 20:48
Operator : MA/JU
Sample : PB157219BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK219

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Title : SVOA CALIBRATION

77	19.181	2732	2736	2740	rVB5	7627	10438	0.85%	0.082%
78	19.257	2745	2749	2755	rVV2	7201	9929	0.81%	0.078%
79	19.598	2802	2807	2821	rBV	877860	1232445	100.00%	9.724%
80	19.775	2836	2837	2839	rBV2	4137	2320	0.19%	0.018%
81	19.798	2839	2841	2842	rBV2	2941	2123	0.17%	0.017%
82	21.380	3105	3110	3122	rBV	404896	621154	50.40%	4.901%
83	23.680	3495	3501	3517	rVB2	596799	1206377	97.88%	9.518%
84	23.851	3523	3530	3540	rBV	284230	631817	51.27%	4.985%




Sum of corrected areas: 12674269

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
Data File : BP018230.D
Acq On : 17 Nov 2023 20:48
Operator : MA/JU
Sample : PB157219BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK219

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

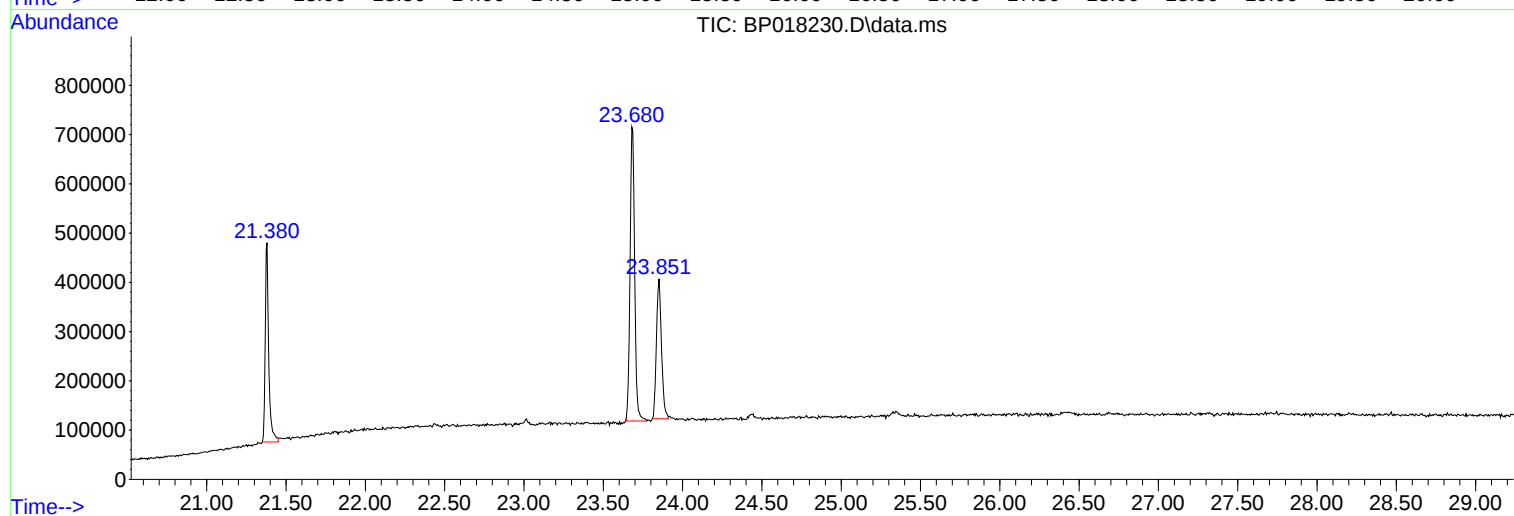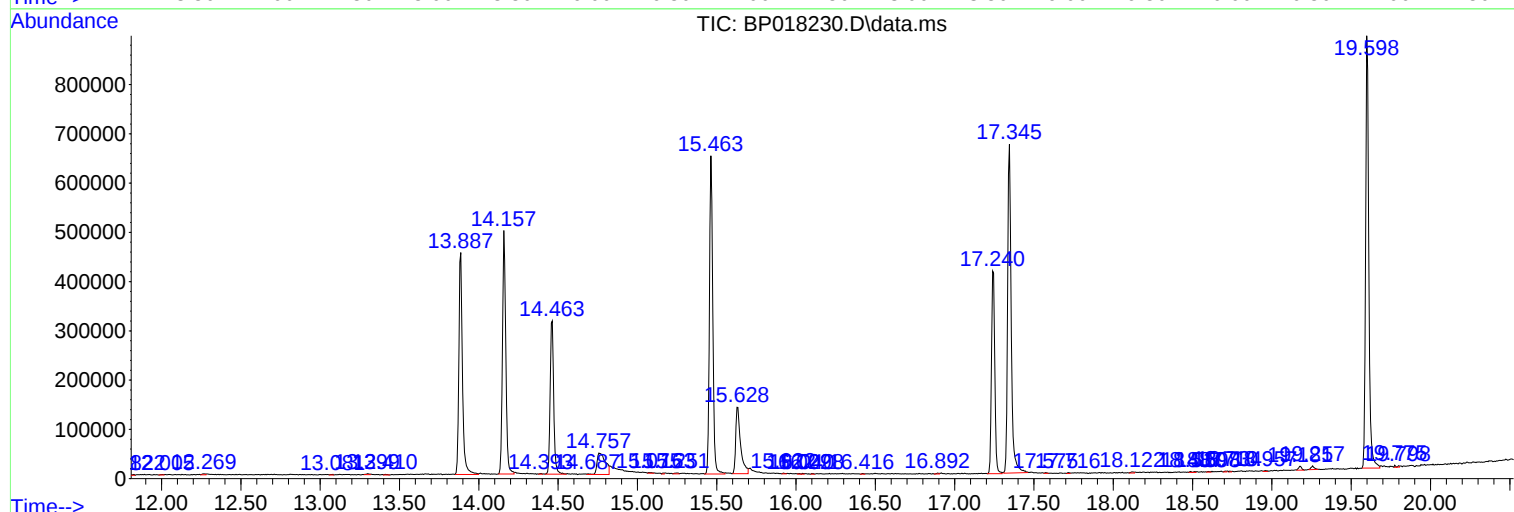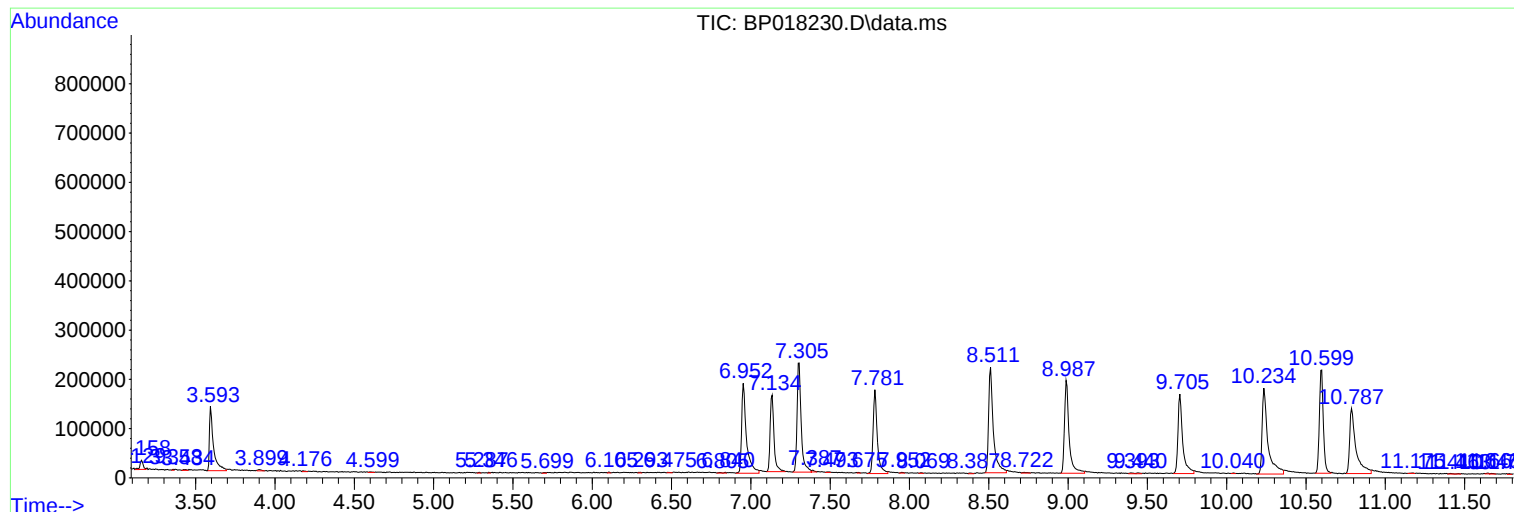

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
Data File : BP018230.D
Acq On : 17 Nov 2023 20:48
Operator : MA/JU
Sample : PB157219BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK219

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
Data File : BP018230.D
Acq On : 17 Nov 2023 20:48
Operator : MA/JU
Sample : PB157219BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK219

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------